

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041218\
 Data File : BF104464.D
 Acq On : 12 Apr 2018 21:10
 Operator : JU/SJ
 Sample : J2337-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Apr 13 00:17:46 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 12 17:07:03 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.81	152	117419	20.00	ng	0.00
21) Naphthalene-d8	8.09	136	431159	20.00	ng	0.00
38) Acenaphthene-d10	9.85	164	162589	20.00	ng	0.00
63) Phenanthrene-d10	11.34	188	261726	20.00	ng	0.00
75) Chrysene-d12	13.99	240	216139	20.00	ng	0.00
86) Perylene-d12	15.45	264	152951	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.44	112	938136	122.17	ng	0.02
7) Phenol-d6	6.45	99	1011537	107.21	ng	0.00
23) Nitrobenzene-d5	7.38	82	739145	111.94	ng	0.00
41) 2,4,6-Tribromophenol	10.65	330	228947	135.75	ng	0.00
44) 2-Fluorobiphenyl	9.17	172	1213490	117.91	ng	0.00
78) Terphenyl-d14	12.93	244	1042066	109.92	ng	0.00
Target Compounds						
9) Benzaldehyde	6.59	77	21613	2.220	ng	84
19) n-Nitroso-di-n-propylamine	7.38	70	97773	15.858	ng	# 72
25) Isophorone	7.38	82	739139	52.936	ng	# 64
50) 2,6-Dinitrotoluene	9.85	165	21352	9.000	ng	# 25
56) 2,4-Dinitrotoluene	9.85	165	21352	6.861	ng	# 22
64) 4,6-Dinitro-2-methylphenol	10.65	198	362	7.588	ng	# 1
66) 4-Bromophenyl-phenylether	10.65	248	14359	5.158	ng	# 1
76) Benzydine	12.93	184	13847	Below Cal		98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041218\
Data File : BF104464.D
Acq On : 12 Apr 2018 21:10
Operator : JU/SJ
Sample : J2337-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Apr 13 00:17:46 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 12 17:07:03 2018
Response via : Initial Calibration

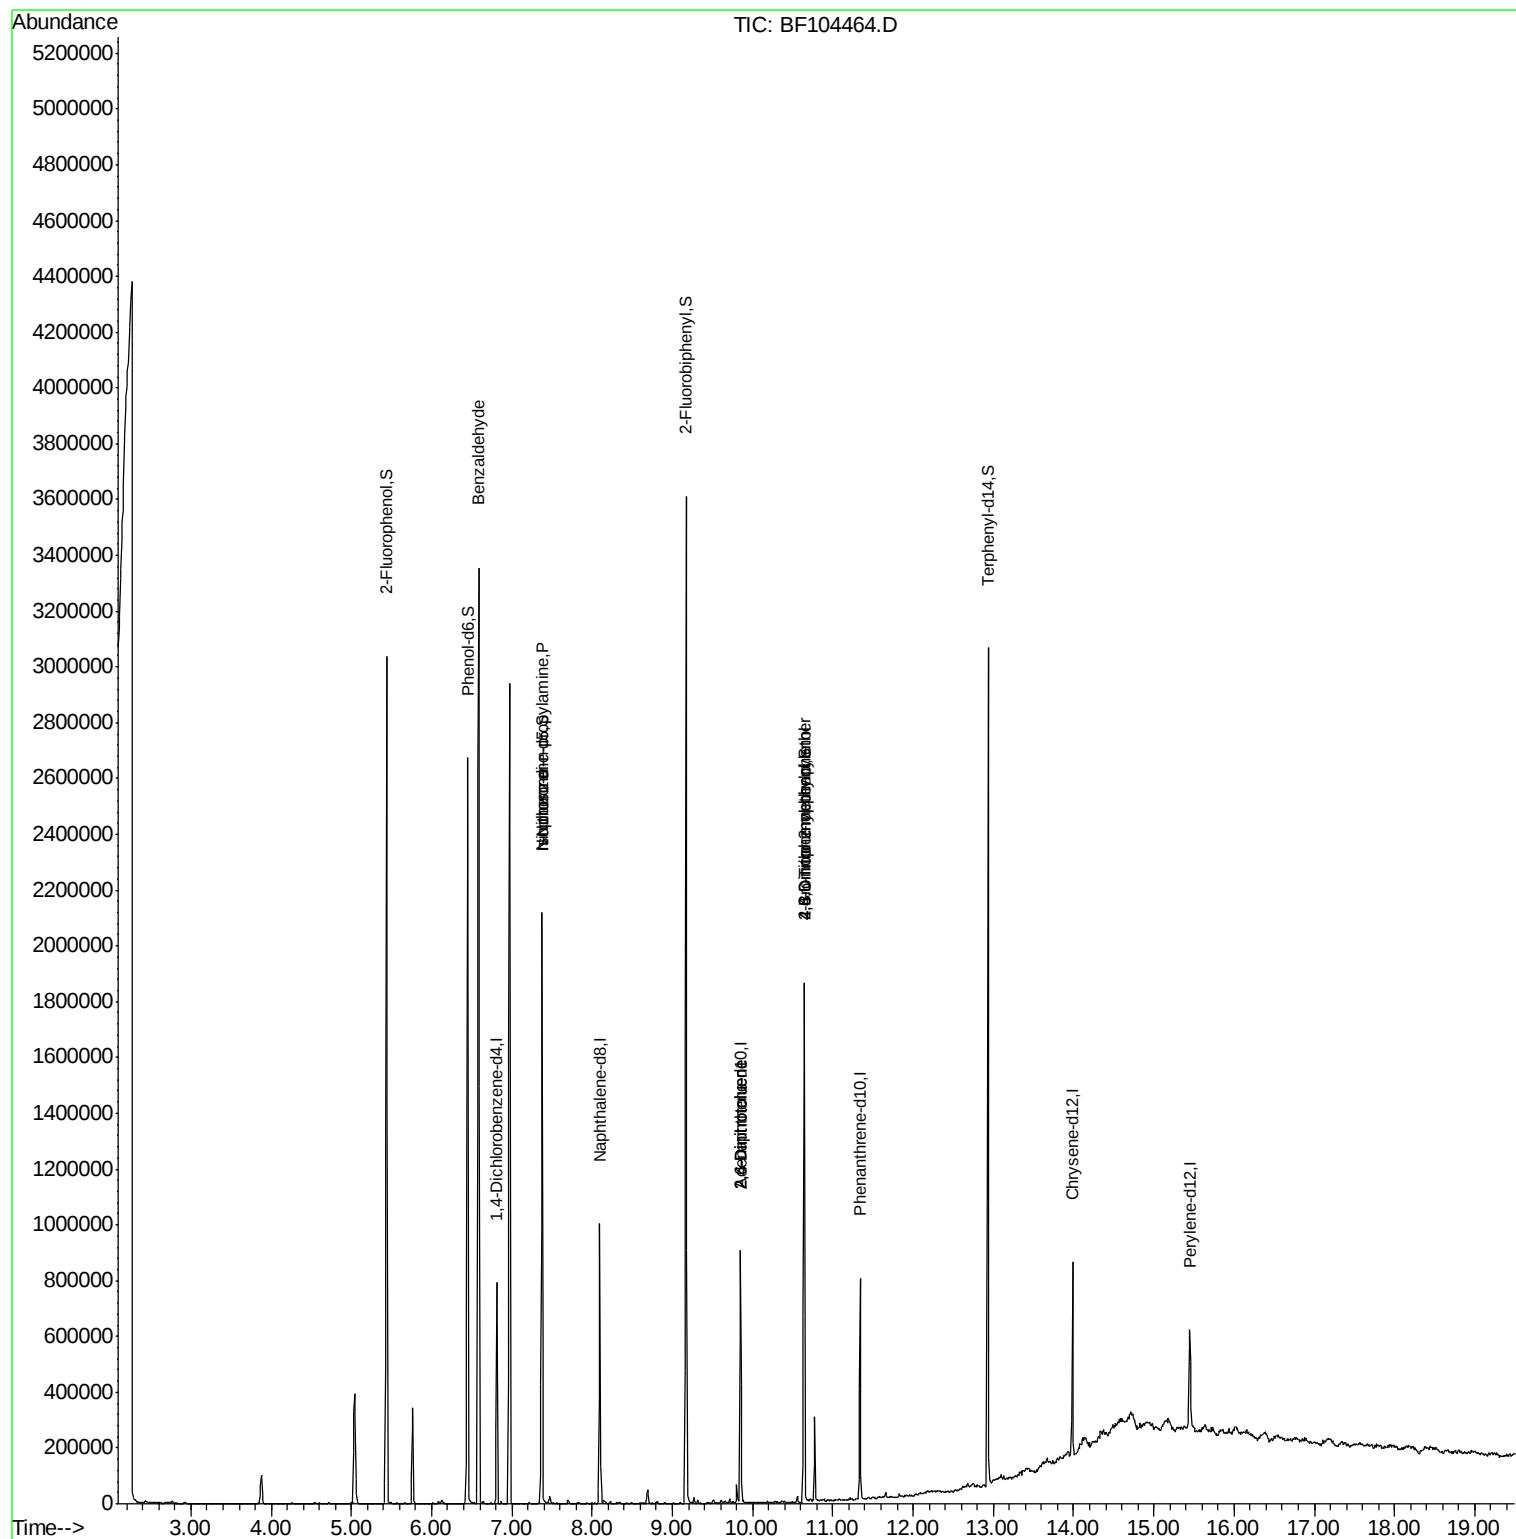




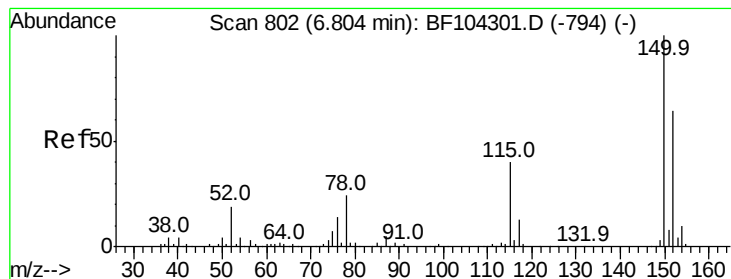


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.81 min Scan# 803
Delta R.T. 0.00 min
Lab File: BF104464.D
Acq: 12 Apr 2018 21:10

Instrument :
BNA_F
ClientSampleId :




Tot Ion:152 Resp: 117419
Ion Ratio Lower Upper
152 100
150 157.7 124.6 186.8
115 65.5 50.1 75.1

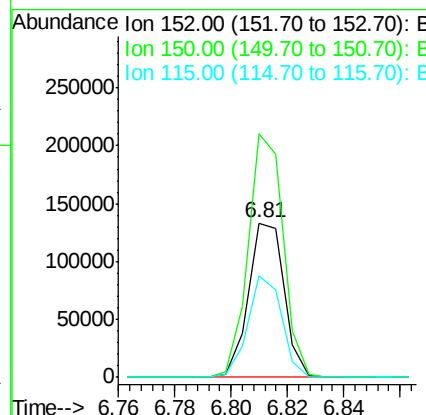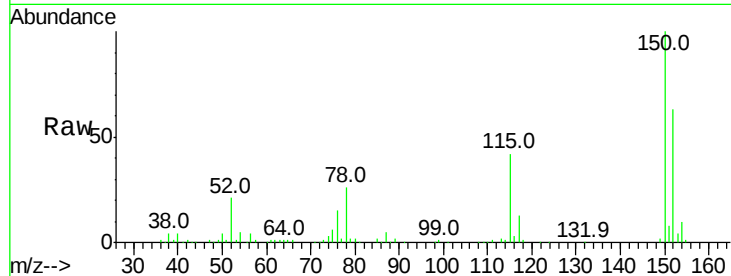


#5

2-Fluorophenol
Concen: 122.166 ng
RT: 5.44 min Scan# 570
Delta R.T. 0.02 min
Lab File: BF104464.D
Acq: 12 Apr 2018 21:10

Tgt Ion:112 Resp: 938136
Ion Ratio Lower Upper
112 100
64 56.4 47.9 71.9
63 28.9 23.7 35.5

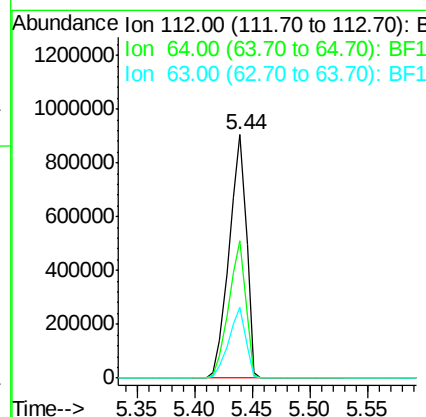

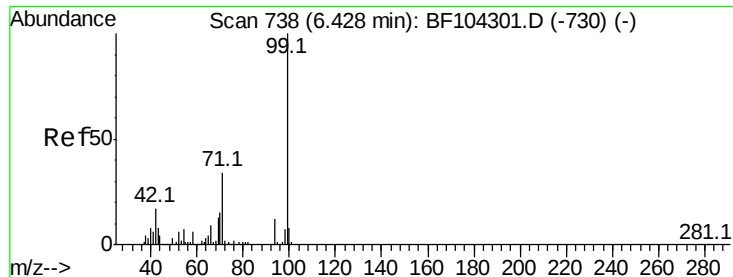

#7

Phenol-d6

Concen: 107.209 ng

RT: 6.45 min Scan# 742

Delta R.T. 0.01 min

Lab File: BF104464.D

Acq: 12 Apr 2018 21:10

Instrument :

BNA_F

ClientSampled :


Tot Ion: 99 Resp: 1011537

Ion Ratio Lower Upper




99 100

42 15.9 14.5 21.7

71 33.1 25.4 38.0

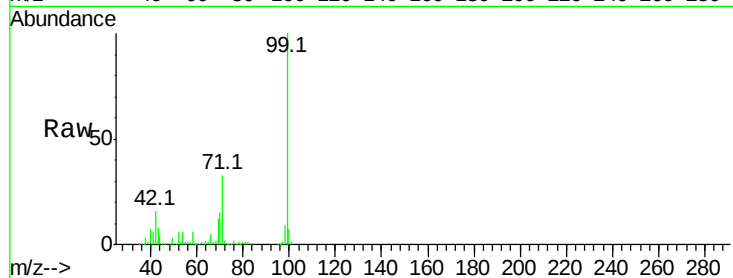

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

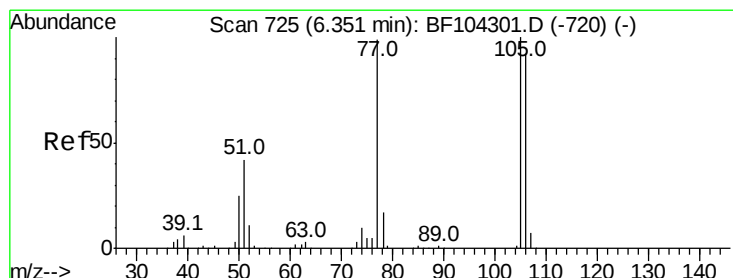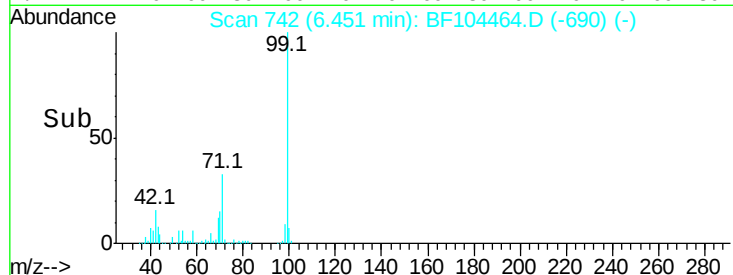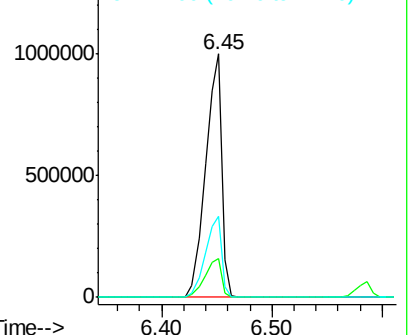

#9

Benzaldehyde

Concen: 2.220 ng

RT: 6.59 min Scan# 765

Delta R.T. 0.22 min

Lab File: BF104464.D

Acq: 12 Apr 2018 21:10


Tgt Ion: 77 Resp: 21613

Ion Ratio Lower Upper



77 100

105 85.8 81.1 121.1

106 77.3 74.5 114.5

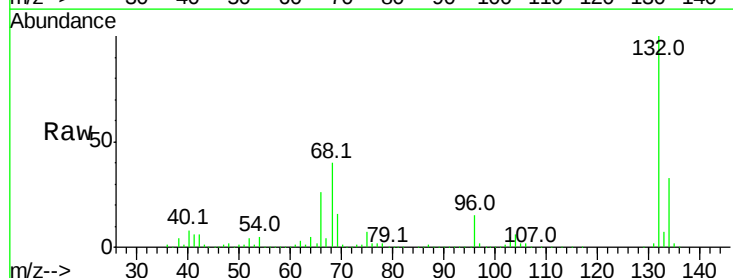

Abundance Ion 77.00 (76.70 to 77.70): BF1
Ion 105.00 (104.70 to 105.70): BF1
Ion 106.00 (105.70 to 106.70): BF1

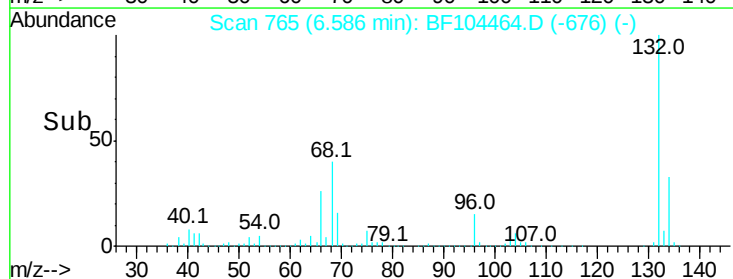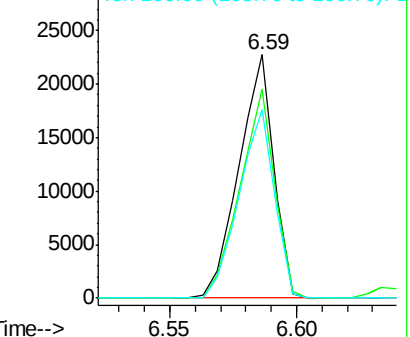



#19

n-Nitroso-di-n-propylamine

Concen: 15.858 ng

RT: 7.38 min Scan# 900

Delta R.T. 0.15 min

Lab File: BF104464.D

Acq: 12 Apr 2018 21:10

Instrument :

BNA_F

ClientSampleId :

Tot Ion: 70 Resp: 97773


Ion Ratio Lower Upper

70 100

42 41.0 47.5 71.3#

101 0.0 7.4 11.2#

130 2.4 16.6 25.0#



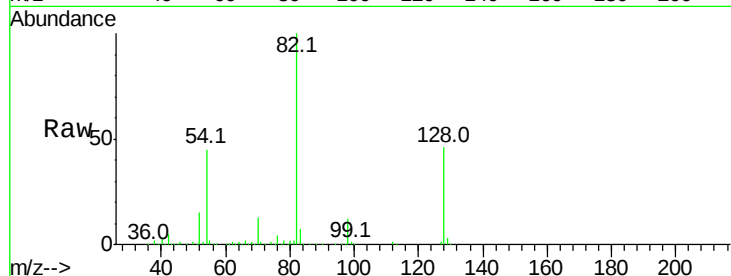


Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

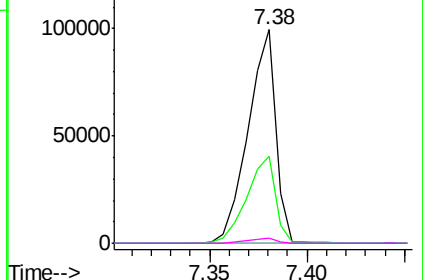

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.09 min Scan# 1021

Delta R.T. -0.01 min

Lab File: BF104464.D

Acq: 12 Apr 2018 21:10

Tgt Ion:136 Resp: 431159


Ion Ratio Lower Upper

136 100

137 11.2 8.9 13.3

54 7.2 6.6 9.8

68 6.3 5.0 7.4





Abundance Ion 136.00 (135.70 to 136.70): BF1

Ion 137.00 (136.70 to 137.70): BF1

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1



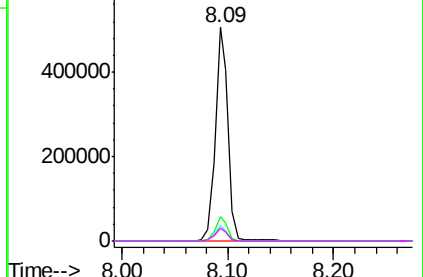





#23
Nitrobenzene-d5
Concen: 111.942 ng
RT: 7.38 min Scan# 900
Delta R.T. 0.00 min
Lab File: BF104464.D
Acq: 12 Apr 2018 21:10




Instrument :
BNA_F
ClientSampleId :


Tot Ion: 82 Resp: 739145
Ion Ratio Lower Upper
82 100
128 46.1 36.1 54.1
54 44.8 41.4 62.2

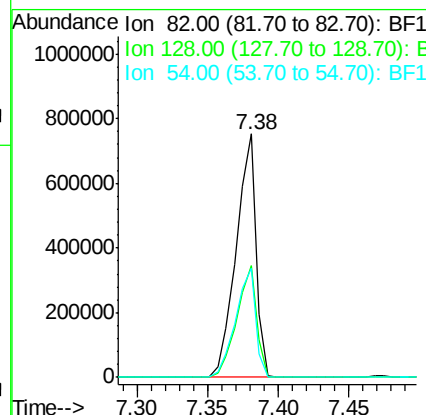

#25
Isophorone
Concen: 52.936 ng
RT: 7.38 min Scan# 900
Delta R.T. -0.25 min
Lab File: BF104464.D
Acq: 12 Apr 2018 21:10

Tgt Ion: 82 Resp: 739139
Ion Ratio Lower Upper
82 100
95 0.0 5.2 7.8#
138 0.0 14.9 22.3#


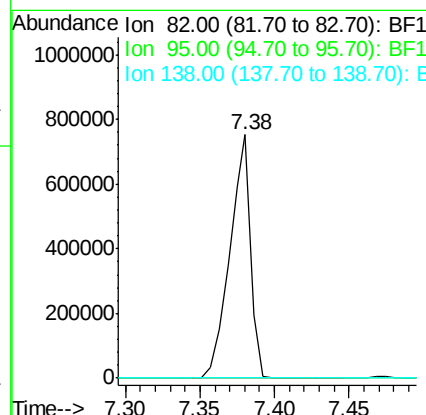




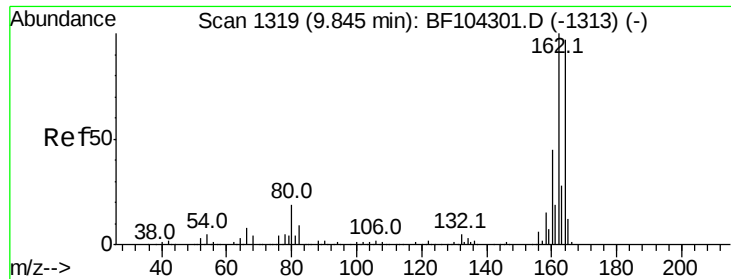

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.85 min Scan# 1320
 Delta R.T. 0.00 min
 Lab File: BF104464.D
 Acq: 12 Apr 2018 21:10




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:164 Resp: 162589
 Ion Ratio Lower Upper
 164 100
 162 104.4 86.1 129.1
 160 45.7 38.3 57.5

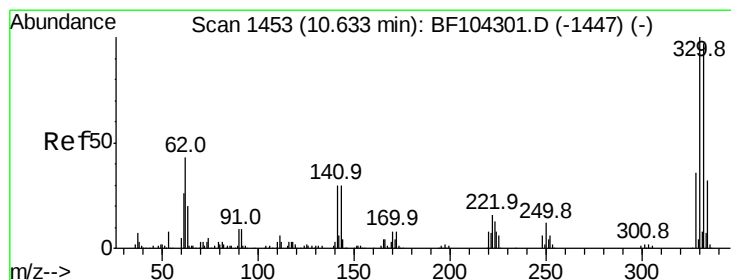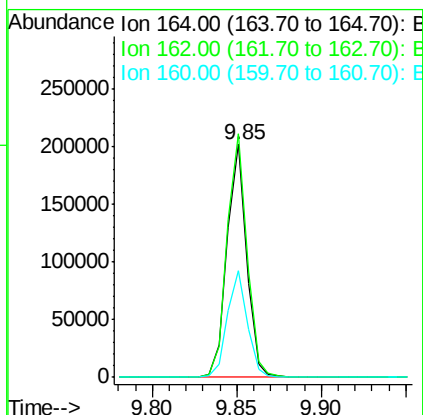

#41
 2,4,6-Tribromophenol
 Concen: 135.746 ng
 RT: 10.65 min Scan# 1455
 Delta R.T. 0.00 min
 Lab File: BF104464.D
 Acq: 12 Apr 2018 21:10

Tgt Ion:330 Resp: 228947
 Ion Ratio Lower Upper
 330 100
 332 97.9 77.0 115.6
 141 33.1 29.9 44.9

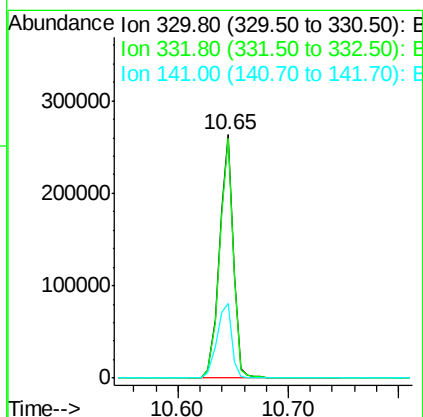







#44
 2-Fluorobiphenyl
 Concen: 117.905 ng
 RT: 9.17 min Scan# 1205
 Delta R.T. 0.00 min
 Lab File: BF104464.D
 Acq: 12 Apr 2018 21:10

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:172 Resp: 1213490




Ion	Ratio	Lower	Upper
172	100		
171	36.0	29.7	44.5
170	24.5	19.6	29.4

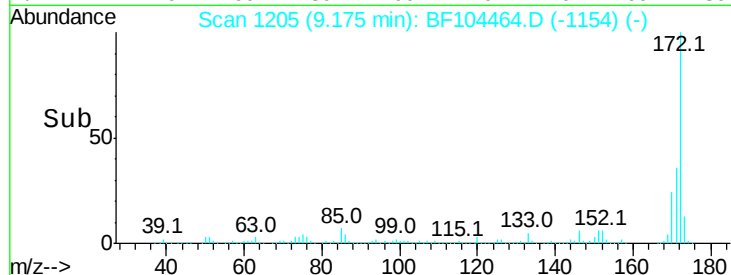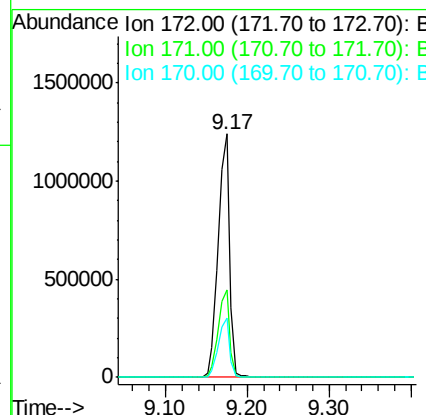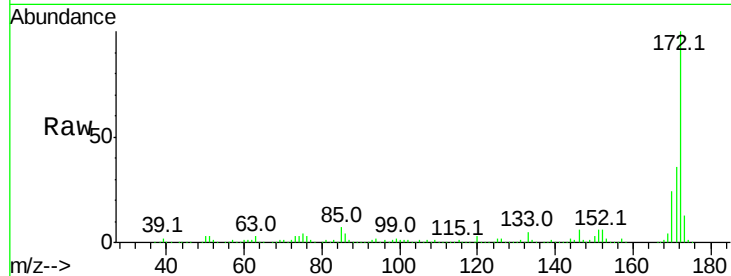


#50
 2,6-Dinitrotoluene
 Concen: 9.000 ng
 RT: 9.85 min Scan# 1320
 Delta R.T. 0.21 min
 Lab File: BF104464.D
 Acq: 12 Apr 2018 21:10

Tgt Ion:165 Resp: 21352

Ion	Ratio	Lower	Upper
165	100		
63	0.0	44.7	67.1#
89	1.5	44.0	66.0#

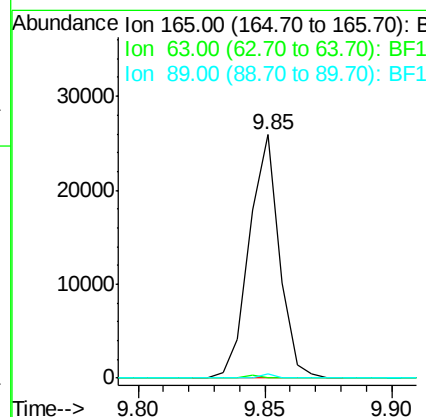

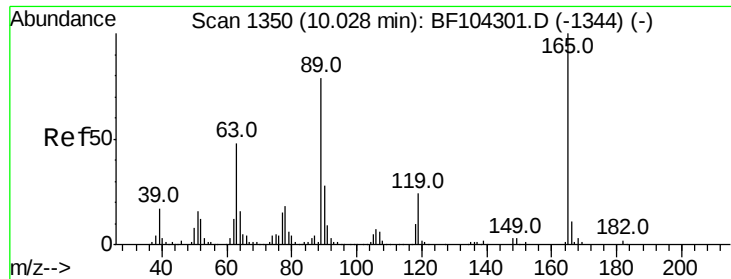

#56

2,4-Dinitrotoluene

Concen: 6.861 ng

RT: 9.85 min Scan# 1320

Delta R.T. -0.19 min

Lab File: BF104464.D

Acq: 12 Apr 2018 21:10

Instrument :
BNA_F
ClientSampleId :

Tot Ion:165 Resp: 21352


Ion Ratio Lower Upper

165 100

63 0.0 36.4 54.6#

89 1.5 57.8 86.6#

182 0.0 1.6 2.4#



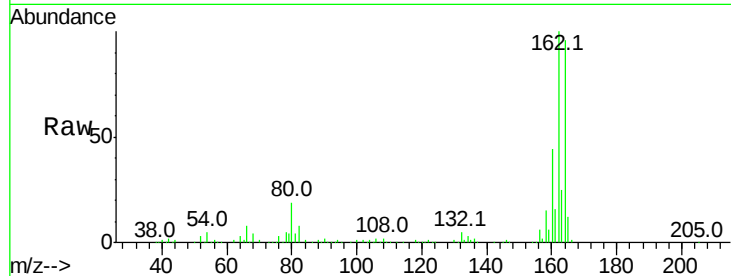


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E

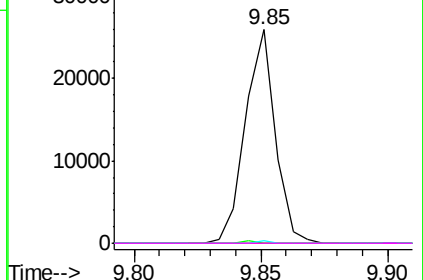

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.34 min Scan# 1573

Delta R.T. 0.00 min

Lab File: BF104464.D

Acq: 12 Apr 2018 21:10


Tgt Ion:188 Resp: 261726

Ion Ratio Lower Upper

188 100

94 10.4 8.5 12.7



80 11.3 9.2 13.8




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

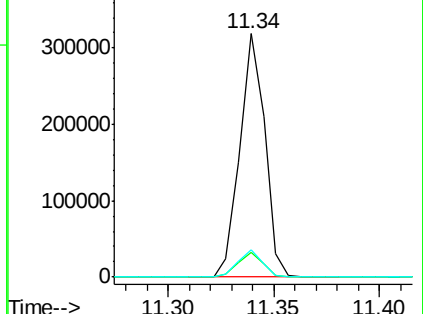

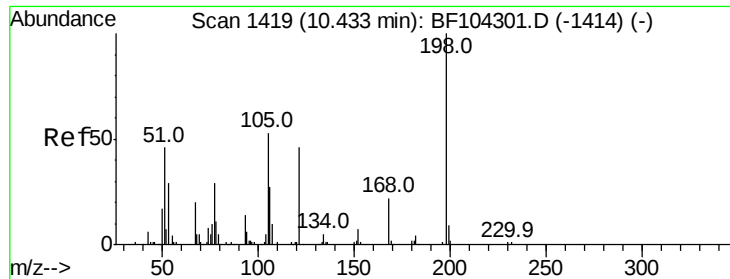

#64

4,6-Dinitro-2-methylphenol

Concen: 7.588 ng

RT: 10.65 min Scan# 1455

Delta R.T. 0.19 min

Lab File: BF104464.D

Acq: 12 Apr 2018 21:10

Instrument :

BNA_F

ClientSampled :


Tot Ion:198 Resp: 362

Ion Ratio Lower Upper

198 100

51 176.1 37.7 77.7#




105 201.2 36.3 76.3#

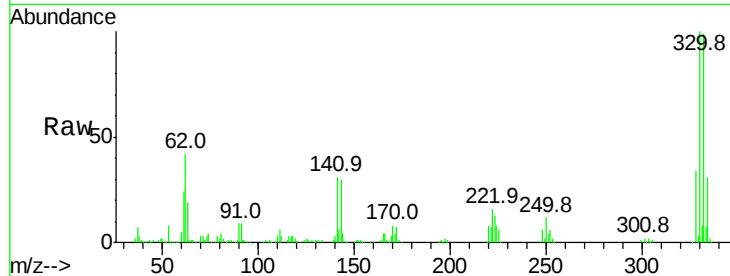

Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BF1

Ion 105.00 (104.70 to 105.70): E

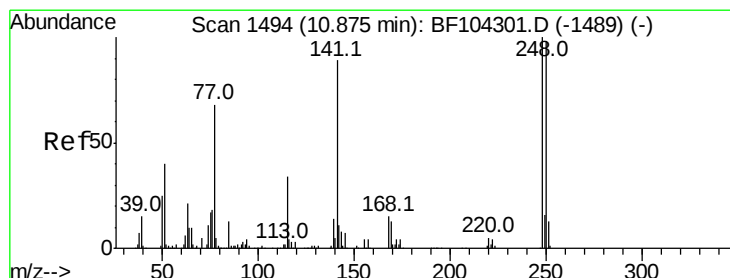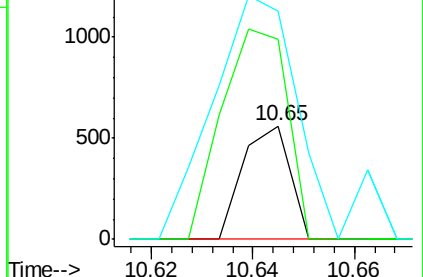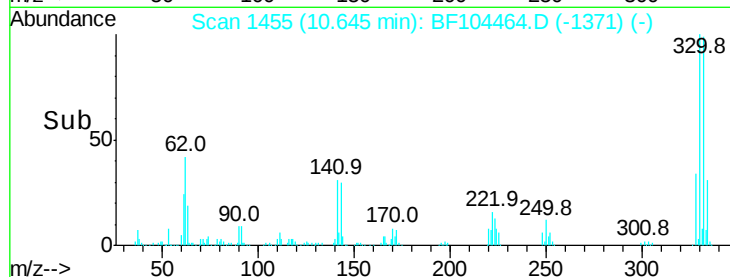

#66

4-Bromophenyl-phenylether

Concen: 5.158 ng

RT: 10.65 min Scan# 1455

Delta R.T. -0.24 min

Lab File: BF104464.D

Acq: 12 Apr 2018 21:10


Tgt Ion:248 Resp: 14359

Ion Ratio Lower Upper

248 100

250 198.5 76.9 115.3#



141 493.8 74.4 111.6#

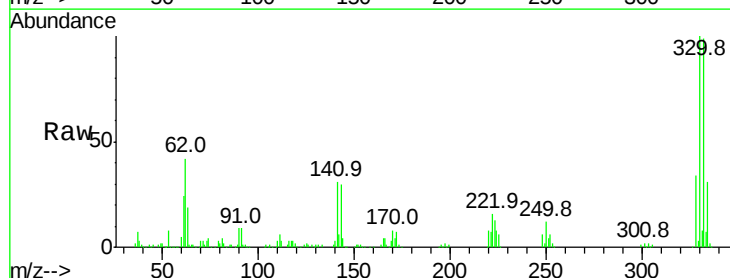


Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

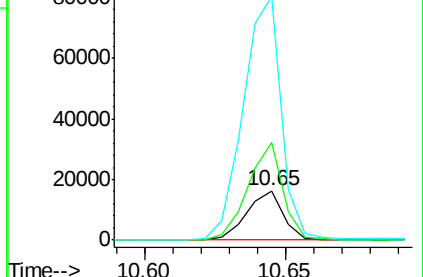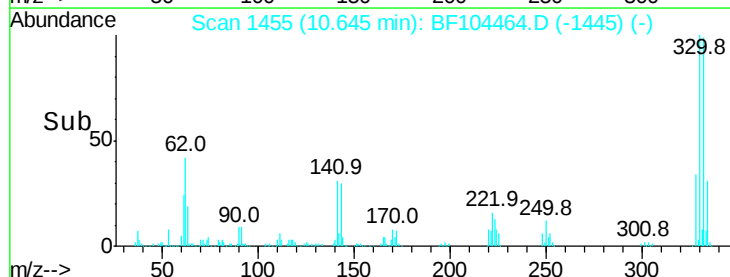



#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.99 min Scan# 2023

Delta R.T. -0.01 min

Lab File: BF104464.D

Acq: 12 Apr 2018 21:10

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 216139

Ion Ratio Lower Upper

240 100

120 12.0 9.5 14.3



236 25.9 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

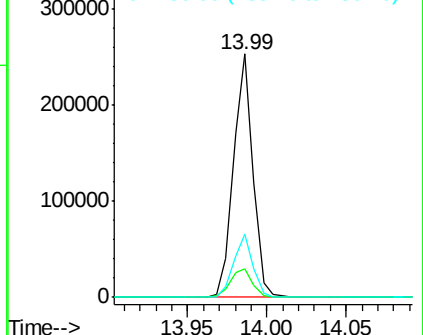

#78

Terphenyl-d14

Concen: 109.917 ng

RT: 12.93 min Scan# 1844

Delta R.T. 0.00 min

Lab File: BF104464.D

Acq: 12 Apr 2018 21:10


Tgt Ion:244 Resp: 1042066

Ion Ratio Lower Upper

244 100

212 7.1 5.4 8.0



122 12.6 11.0 16.4




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

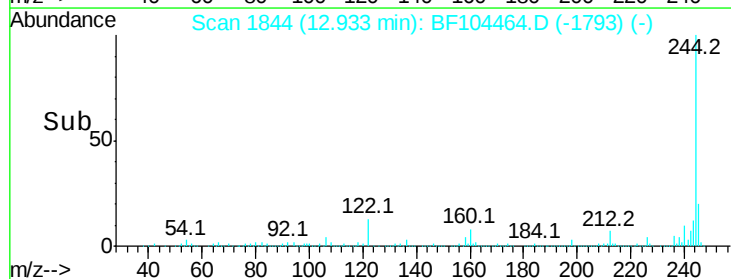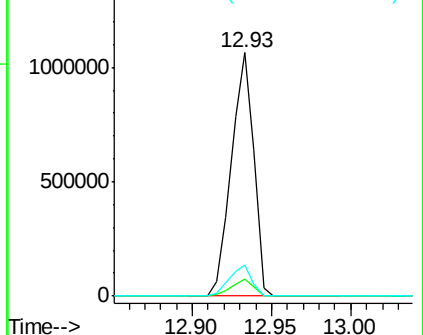


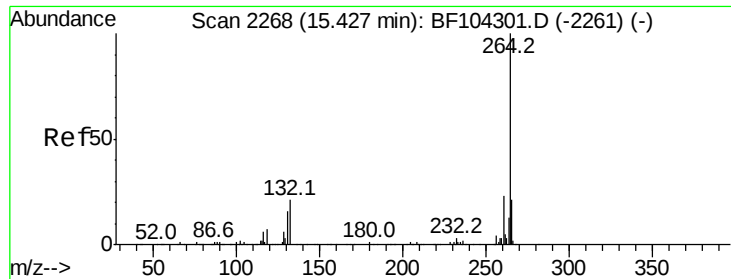

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.45 min Scan# 2272
Delta R.T. -0.01 min
Lab File: BF104464.D
Acq: 12 Apr 2018 21:10

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.4	19.2	28.8
265	21.0	17.5	26.3

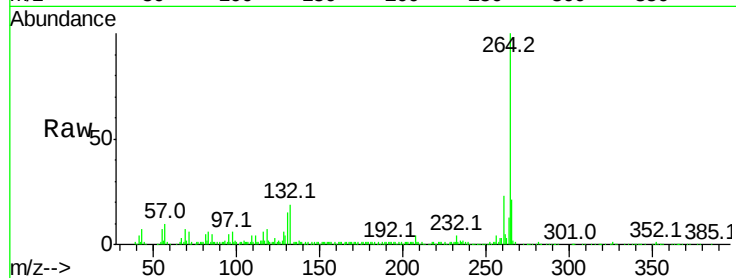

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

