
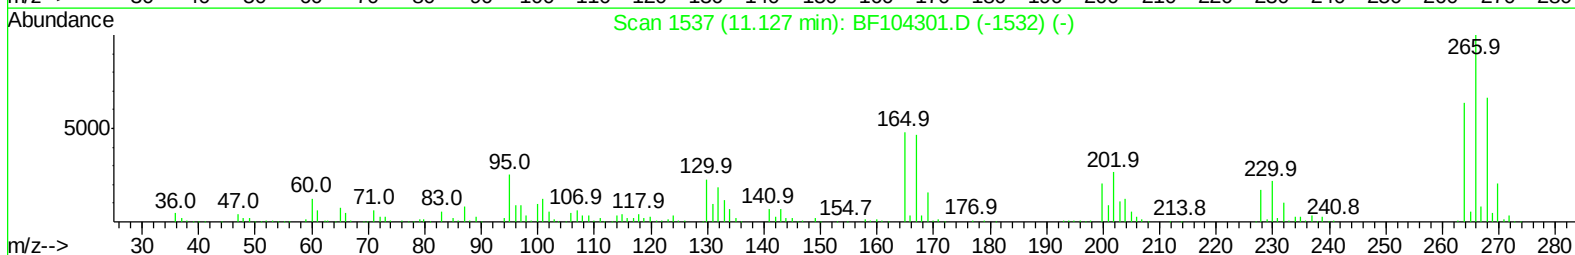
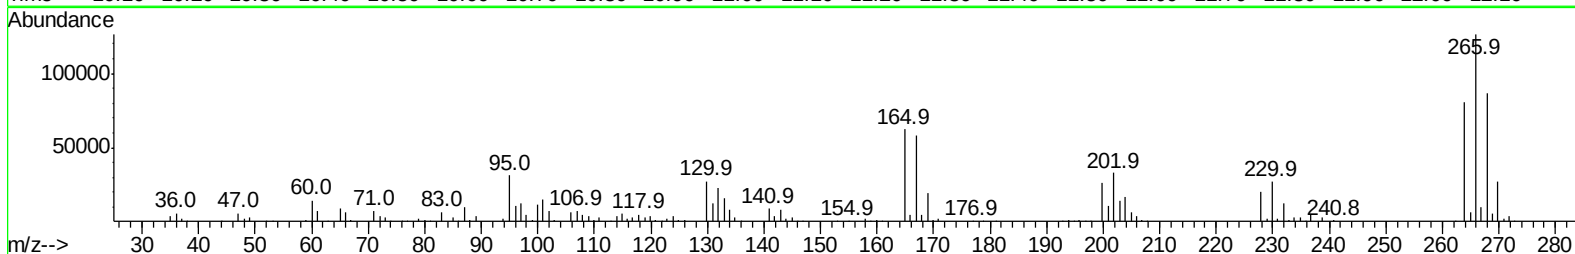


Data Path : Z:\HPCHEM1\BNA F\DATA\BF041218\
Data File : BF104445.D
Acq On : 12 Apr 2018 12:35
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 01:54:19 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 12 17:07:03 2018
Response via : Initial Calibration

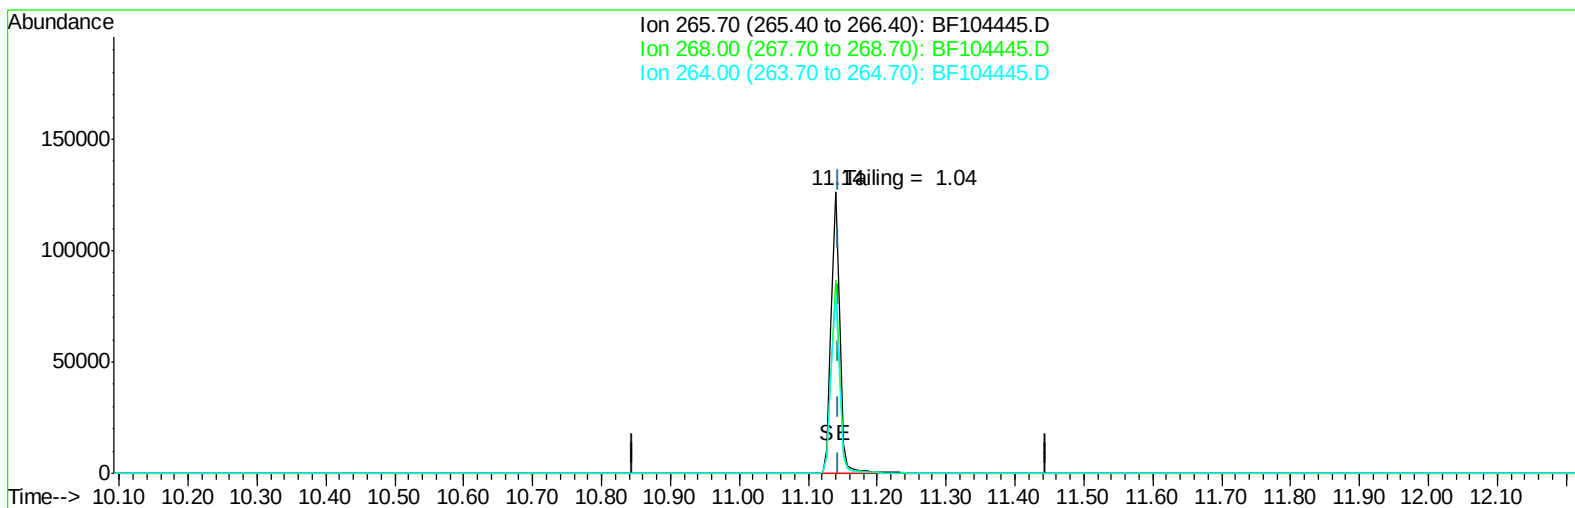

TIC: BF104445.D

(69) Pentachlorophenol (C)




11.139min (-0.006) 28993.36ng

response 106910

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	68.62
264.00	61.90	63.77
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041218\
Data File : BF104445.D
Acq On : 12 Apr 2018 12:35
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 01:54:19 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 12 17:07:03 2018
Response via : Initial Calibration

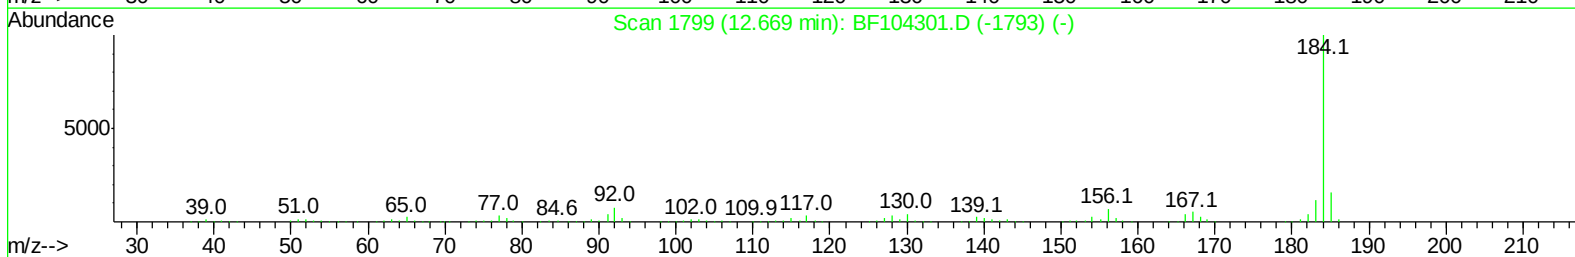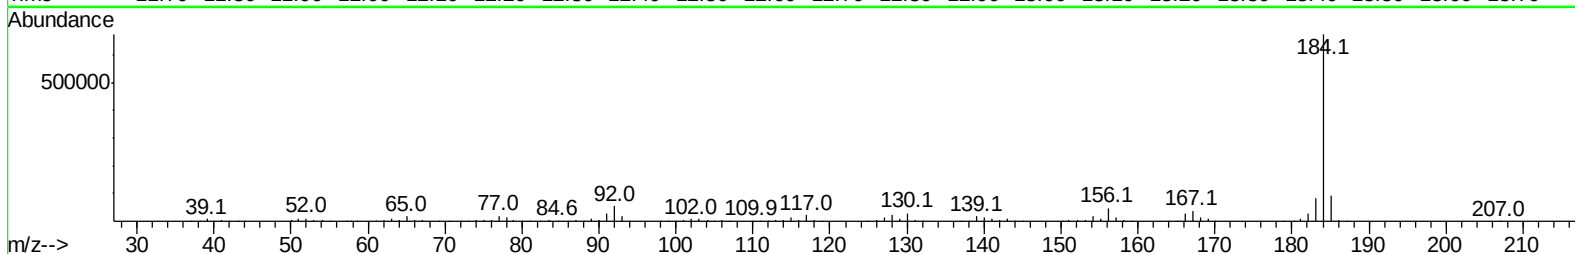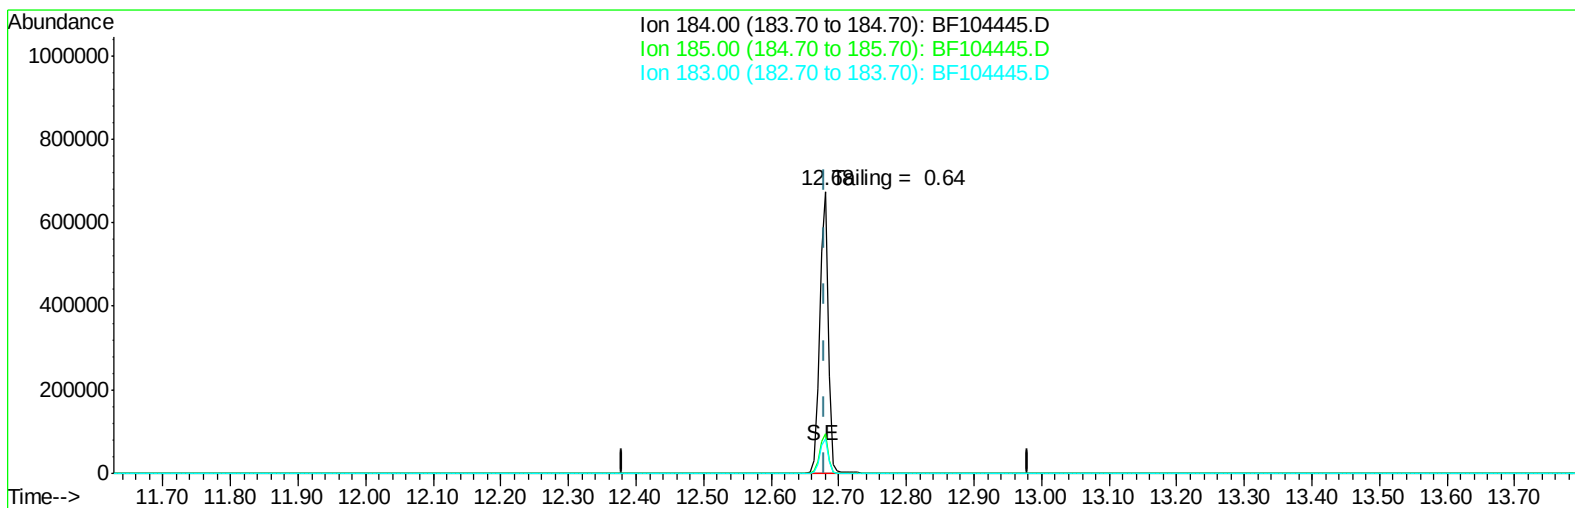

TIC: BF104445.D

(76) Benzidine

12.680min (+0.000) 0.00ng

response 610147

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.90
183.00	11.60	12.30
0.00	0.00	0.00