


Data Path : Z:\HPCHEM1\BNA F\Data\BF041218\
 Data File : BF104445.D
 Acq On : 12 Apr 2018 12:35
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 12 17:07:03 2018

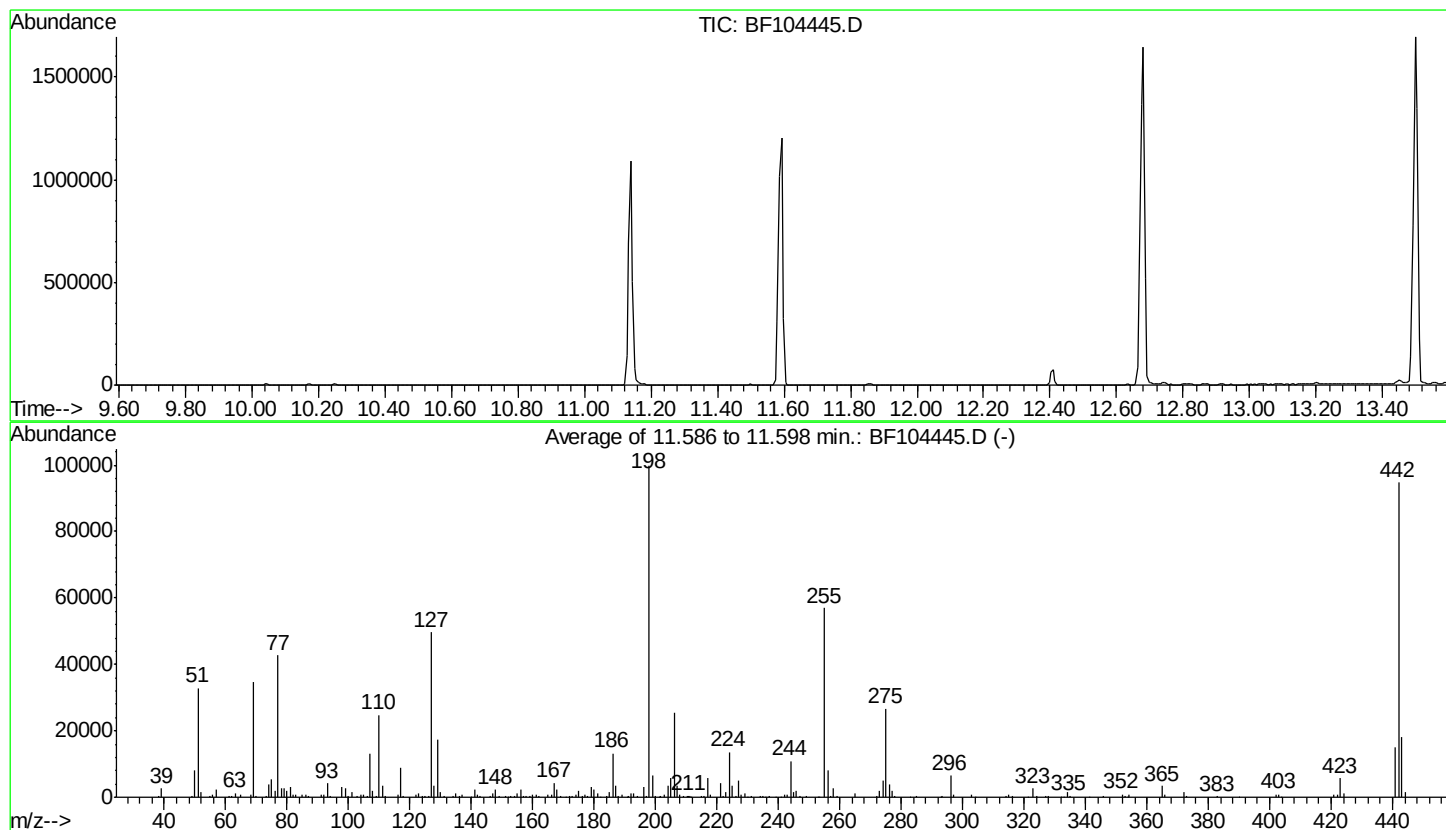

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	32837	PASS
68	69	0.00	2	1.8	614	PASS
69	198	0.00	100	34.6	34562	PASS
70	69	0.00	2	0.6	218	PASS
127	198	10	80	49.7	49661	PASS
197	198	0.00	2	0.5	474	PASS
198	198	100	100	100.0	99858	PASS
199	198	5	9	6.6	6546	PASS
275	198	10	60	26.8	26741	PASS
365	198	1	100	3.4	3353	PASS
441	443	0.01	100	83.1	14937	PASS
442	198	50	100	94.8	94669	PASS
443	442	15	24	19.0	17980	PASS