
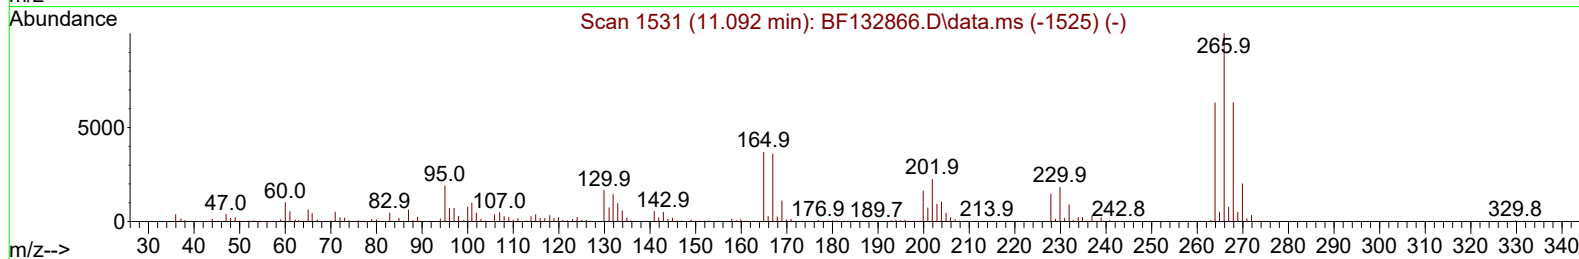
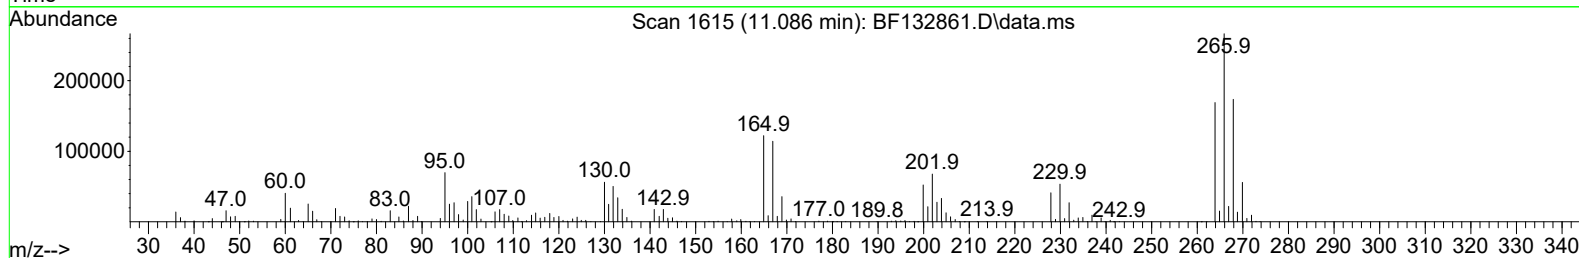


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041223\
Data File : BF132861.D
Acq On : 12 Apr 2023 14:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 08:16:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 13 05:46:34 2023
Response via : Initial Calibration

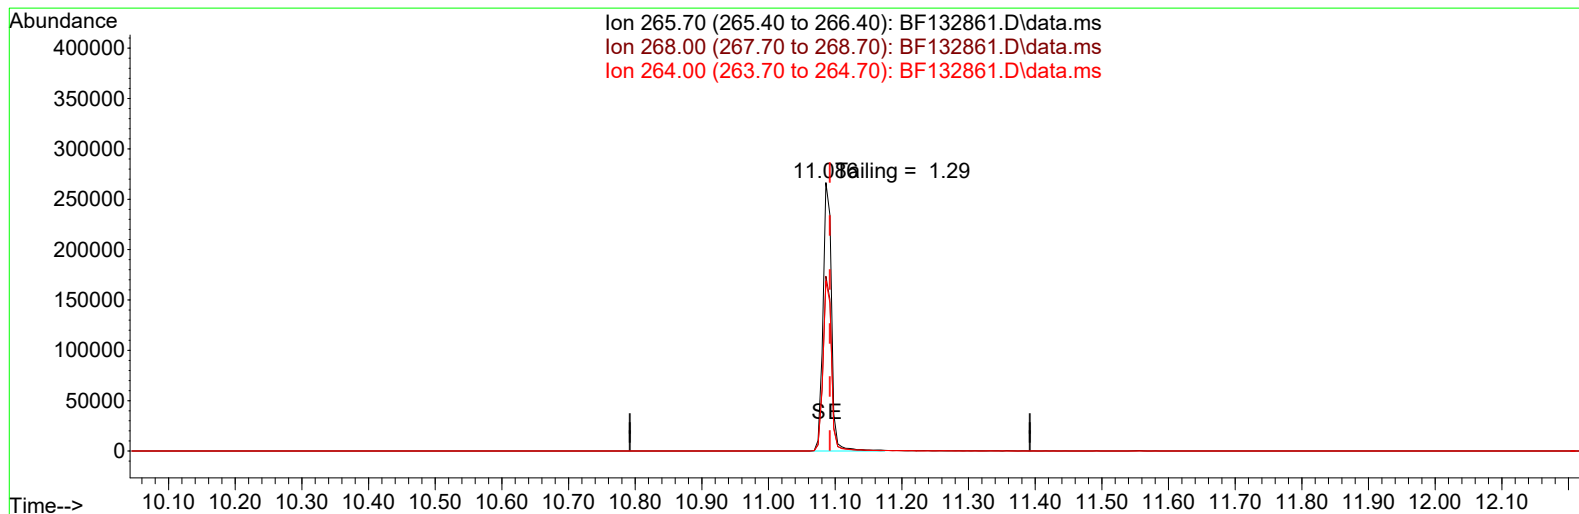

TIC: BF132861.D\data.ms

(70) Pentachlorophenol (C)




11.086min (-0.006) 78372.59 ng

response 238545

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	65.13
264.00	63.10	63.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041223\
Data File : BF132861.D
Acq On : 12 Apr 2023 14:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 08:16:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 13 05:46:34 2023
Response via : Initial Calibration

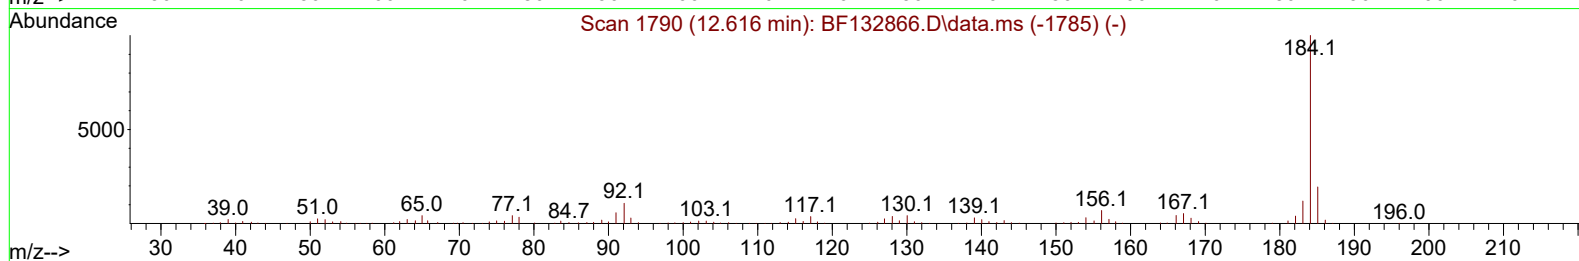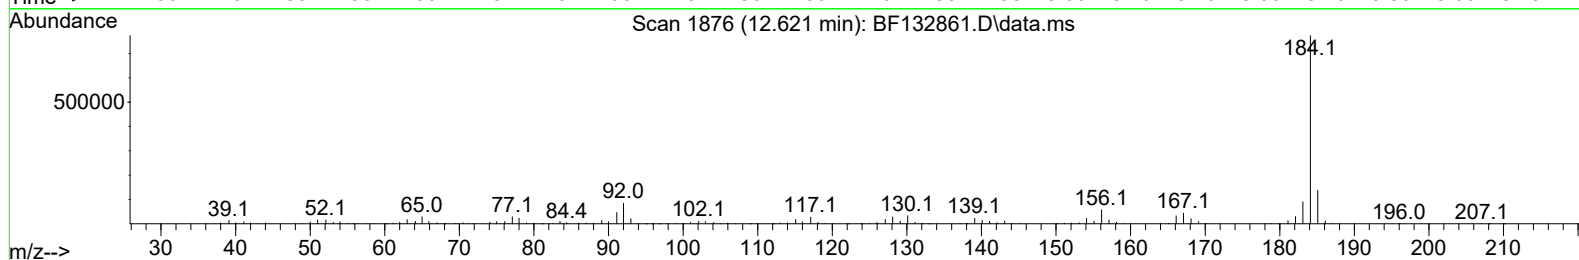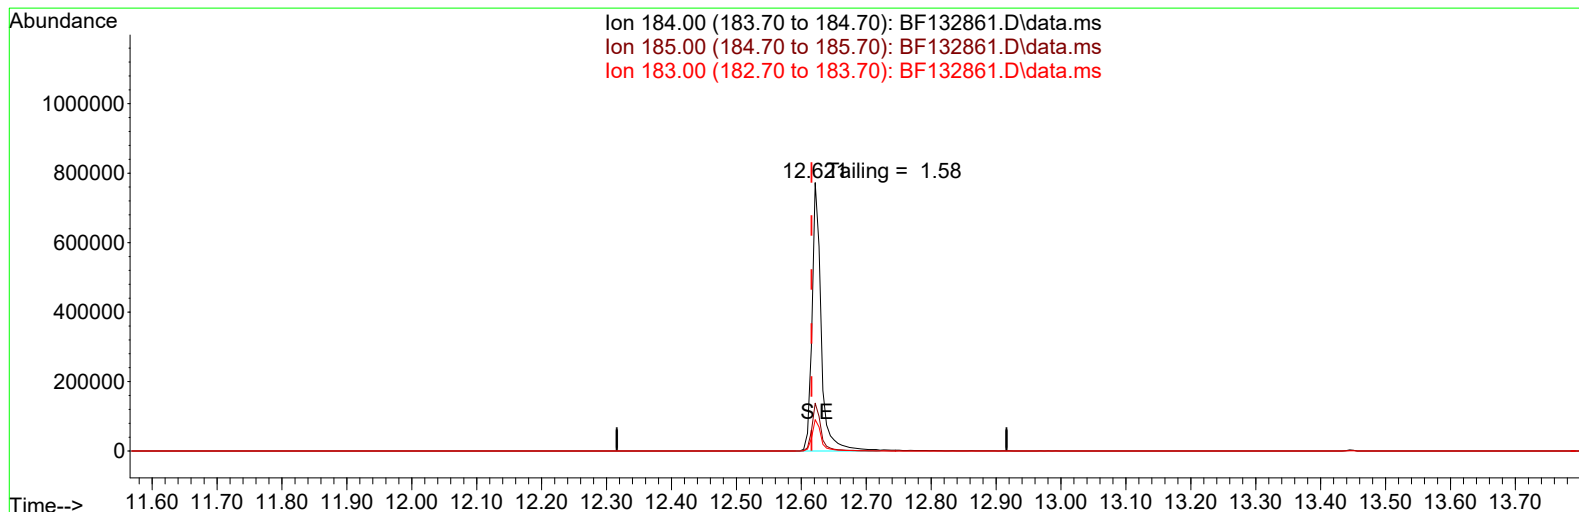

TIC: BF132861.D\data.ms

(77) Benzidine

12.621min (+ 0.005) 0.00 ng

response 766965

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.50	17.82
183.00	11.90	11.70
0.00	0.00	0.00