


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041223\
Data File : BF132861.D
Acq On : 12 Apr 2023 14:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 13 05:46:34 2023

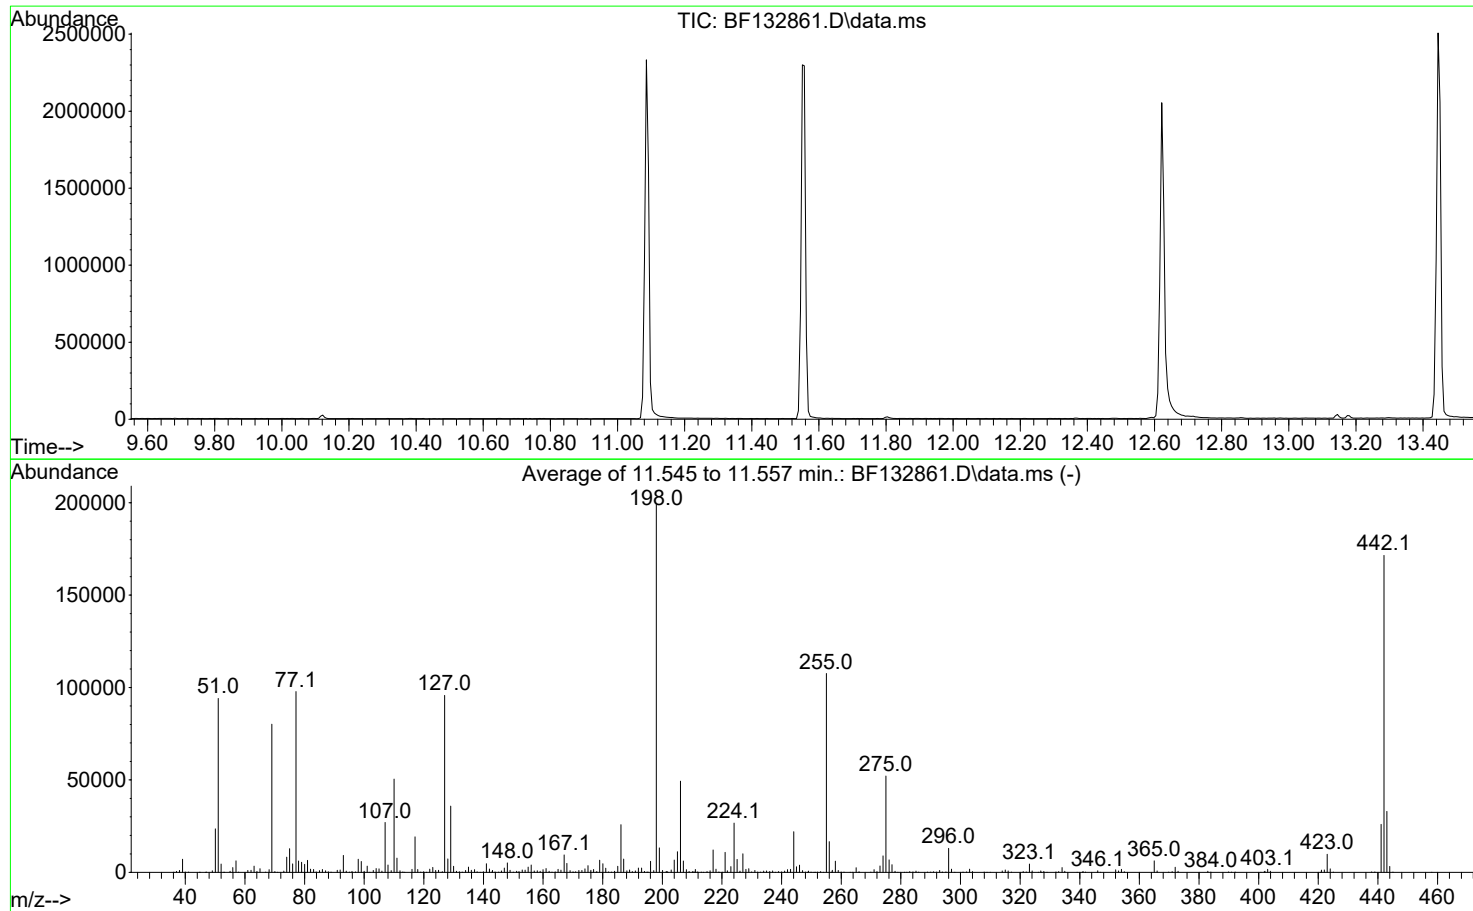




AutoFind: Scans 1693, 1694, 1695; Background Corrected with Scan 1688

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.3	94149	PASS
68	69	0.00	2	1.8	1480	PASS
69	198	0.00	100	40.3	80205	PASS
70	69	0.00	2	0.5	420	PASS
127	198	10	80	48.1	95760	PASS
197	198	0.00	2	0.5	946	PASS
198	198	100	100	100.0	199037	PASS
199	198	5	9	6.7	13283	PASS
275	198	10	60	26.2	52121	PASS
365	198	1	100	3.1	6227	PASS
441	198	0.01	100	13.1	25992	PASS
442	442	50	100	100.0	171544	PASS
443	442	15	24	19.3	33023	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041223\
Data File : BF132861.D
Acq On : 12 Apr 2023 14:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 13 08:16:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 13 05:46:34 2023
Response via : Initial Calibration

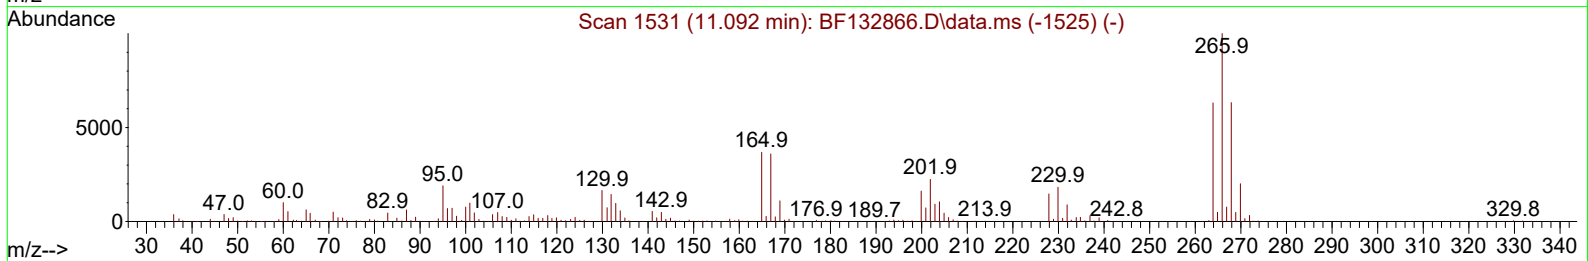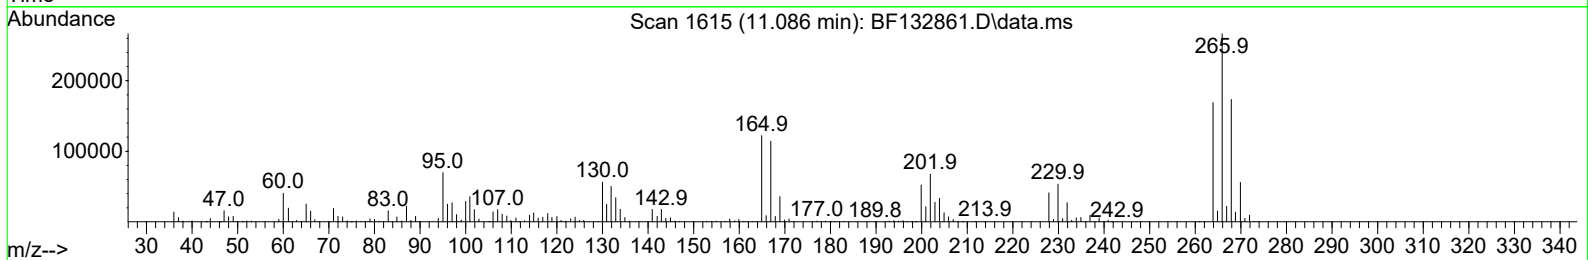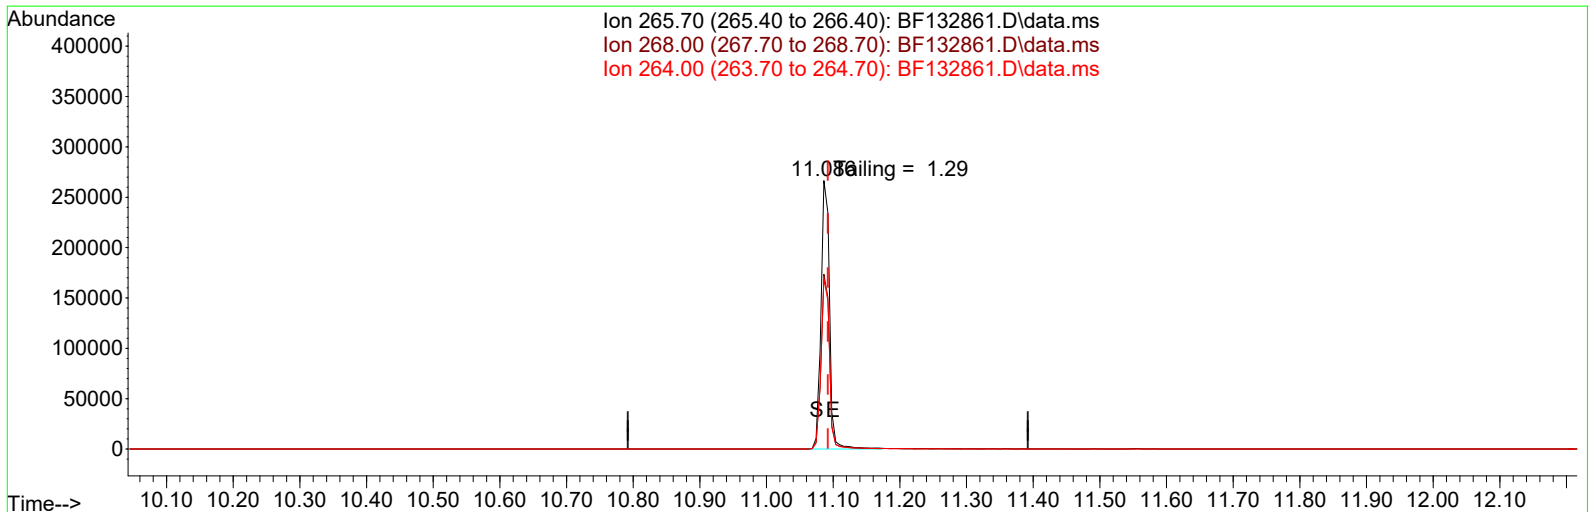

TIC: BF132861.D\data.ms

(70) Pentachlorophenol (C)

11.086min (-0.006) 78372.59 ng




response 238545

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	65.13
264.00	63.10	63.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041223\
Data File : BF132861.D
Acq On : 12 Apr 2023 14:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 13 08:16:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 13 05:46:34 2023
Response via : Initial Calibration

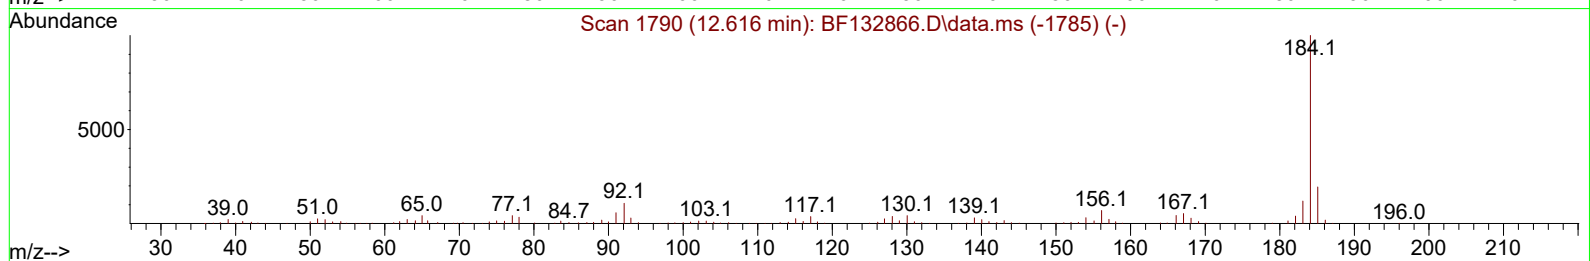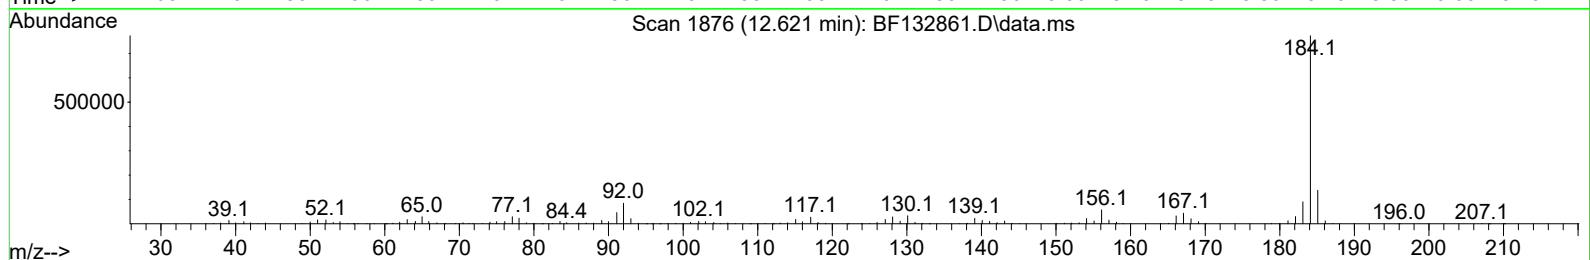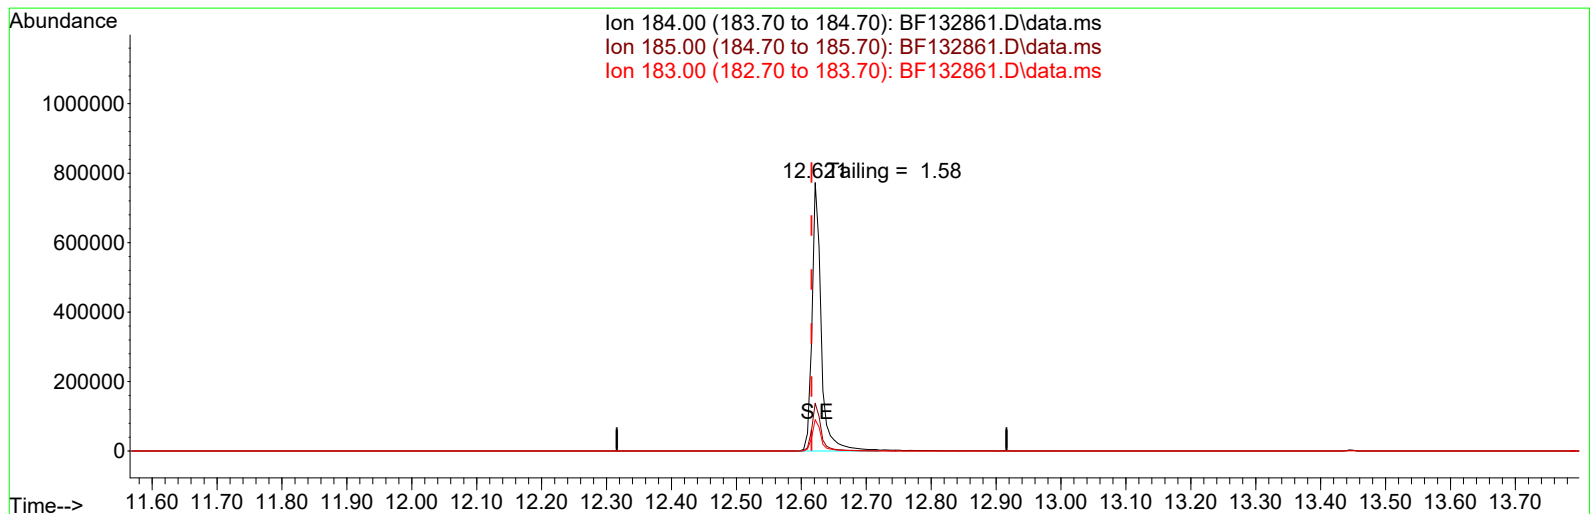

TIC: BF132861.D\data.ms

(77) Benzidine

12.621min (+ 0.005) 0.00 ng

response 766965

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.50	17.82
183.00	11.90	11.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/12/2023	BNA_F	BF132861.D
Compound Name	Response	Retention Time
DDT	293650	13.445
DDD	4803	13.145
DDE	0	12.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4803	298453	1.61

Instrument :
BNA_F
ClientSampleId :
DFTPP