
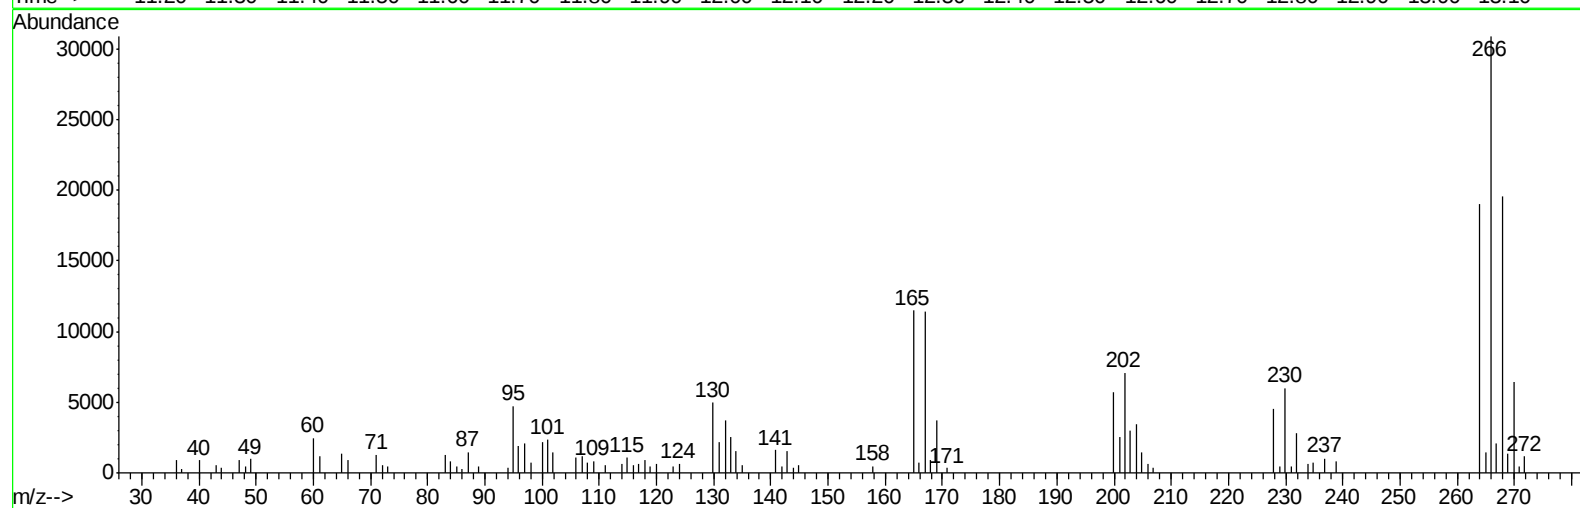


Data Path : Z:\HPCHEM1\BNA_F\Data\BF041315\
Data File : BF078459.D
Acq On : 13 Apr 2015 12:37
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 07:55:02 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 14 07:20:26 2015
Response via : Initial Calibration

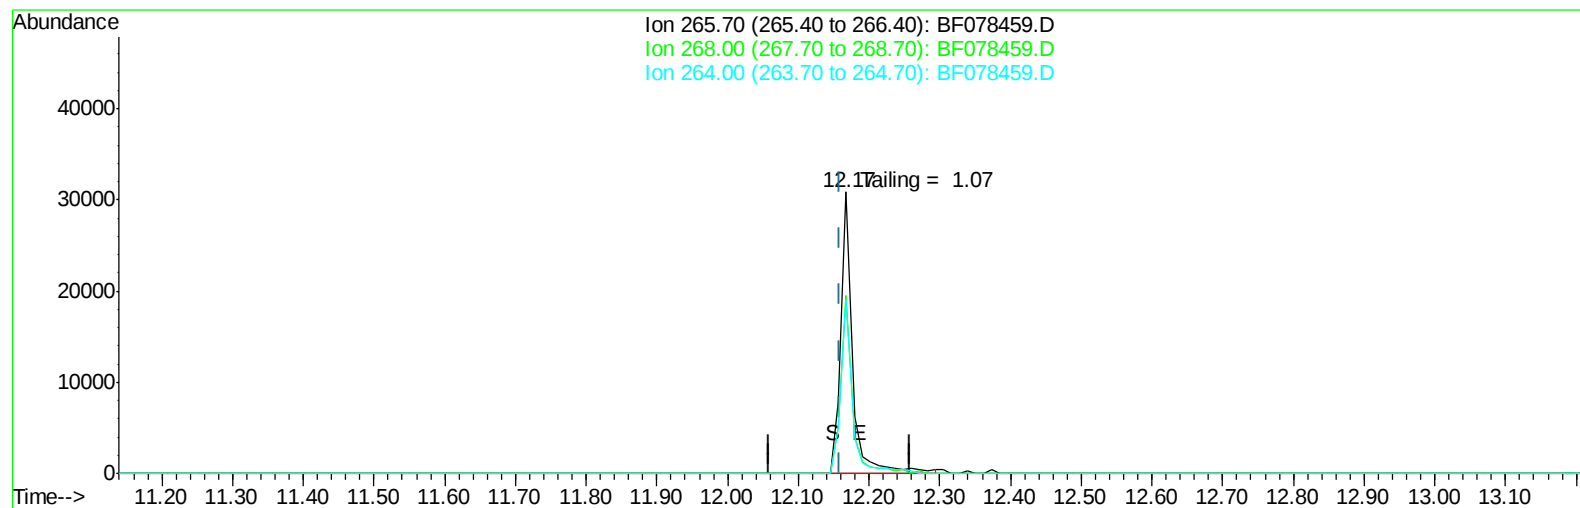

TIC: BF078459.D

(69) Pentachlorophenol (C)



12.168min (+0.008) 13849.86ng

response 33527

Ion	Exp%	Act%
265.70	100	100
268.00	62.60	63.32
264.00	62.50	61.63
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF041315\
Data File : BF078459.D
Acq On : 13 Apr 2015 12:37
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 07:55:02 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 14 07:20:26 2015
Response via : Initial Calibration

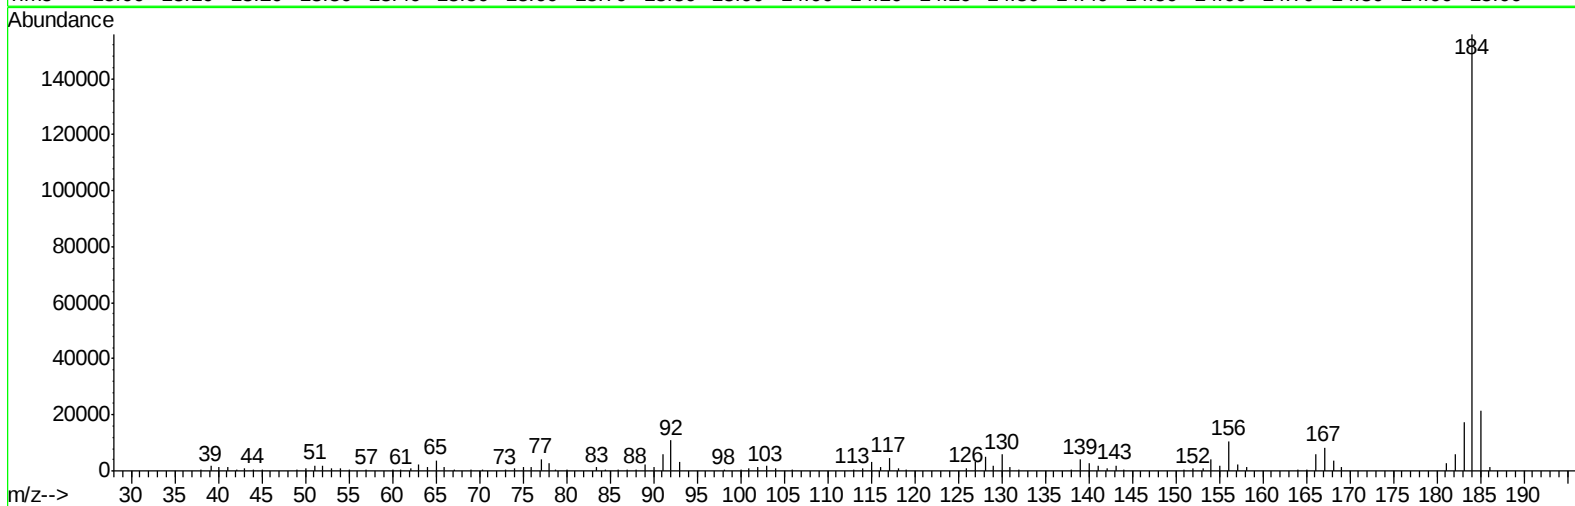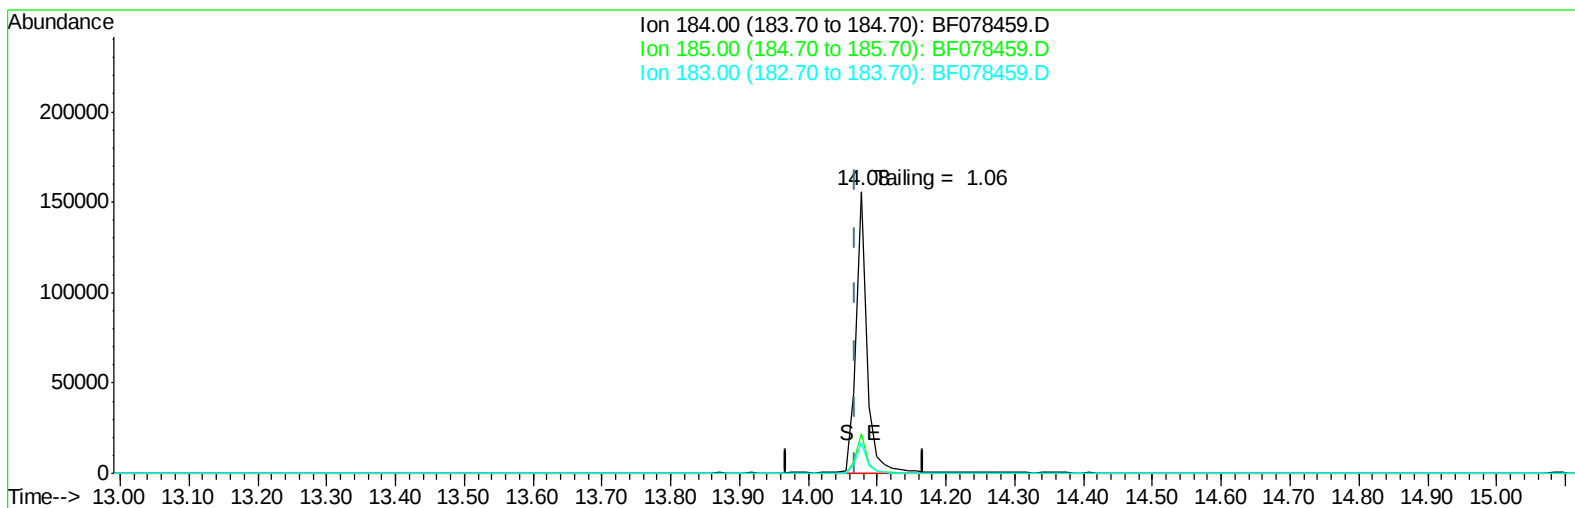

TIC: BF078459.D

(76) Benzidine

14.077min (+0.008) 6931.53ng

response 173486

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	13.91
183.00	11.90	11.03
0.00	0.00	0.00