
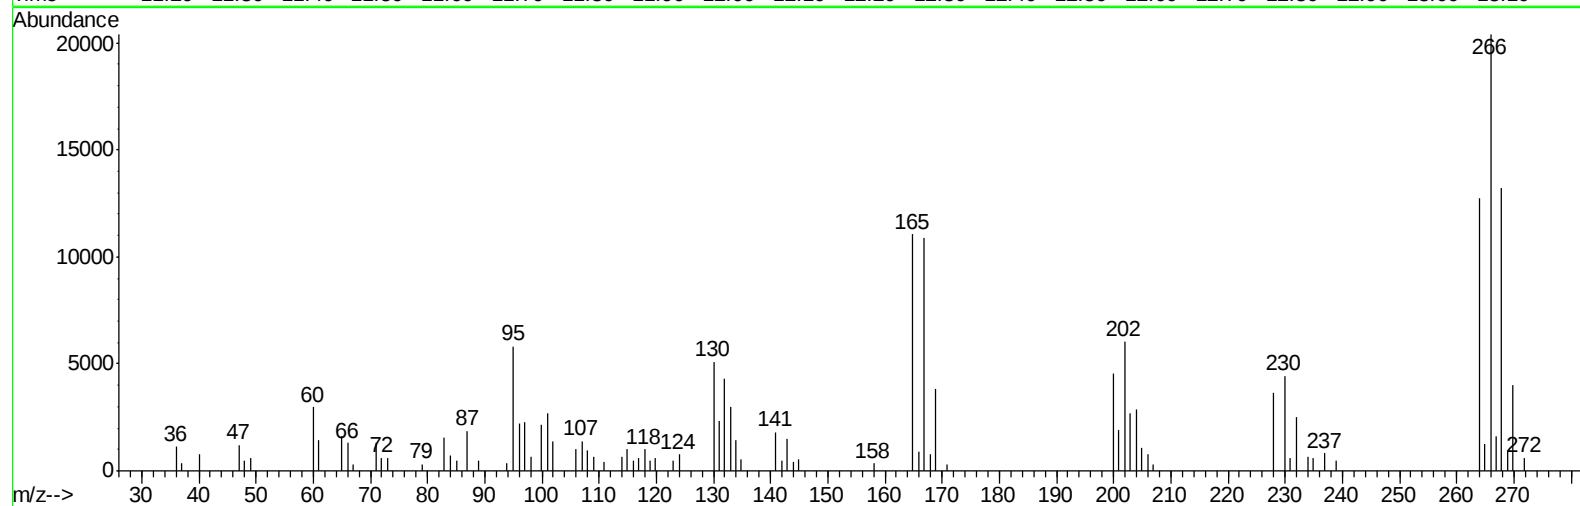


Data Path : Z:\HPCHEM1\BNA_F\Data\BF041315\
Data File : BF078480.D
Acq On : 14 Apr 2015 2:17
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 07:55:56 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 14 07:20:26 2015
Response via : Initial Calibration

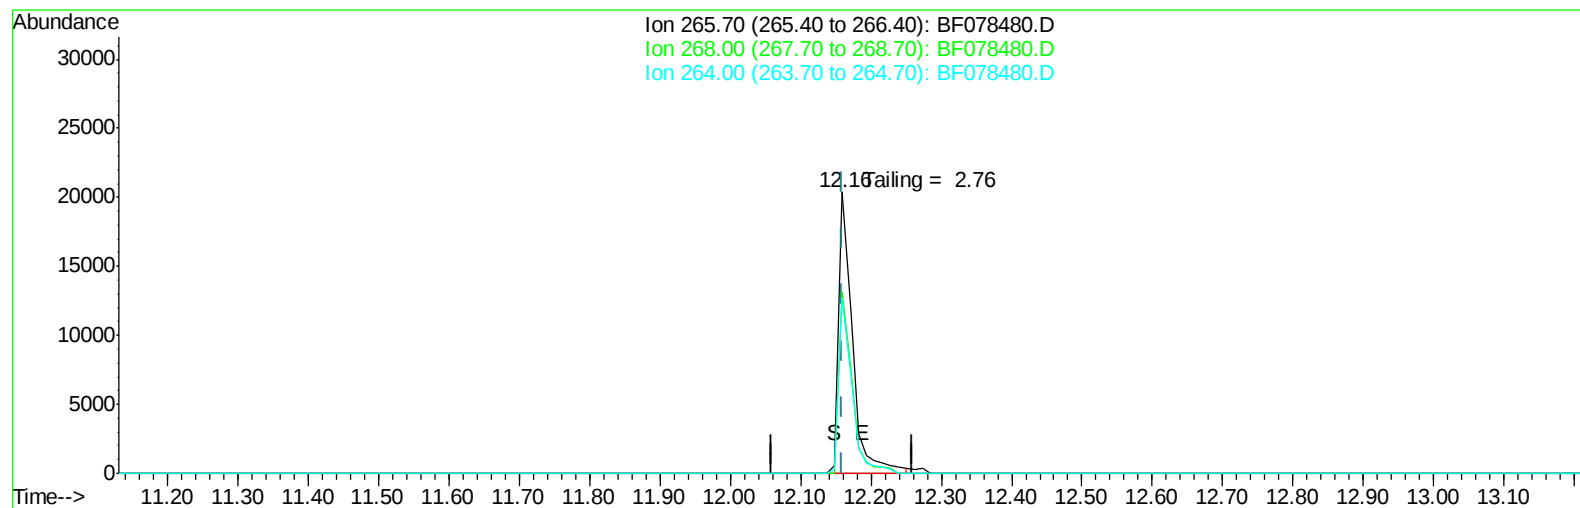

TIC: BF078480.D

(69) Pentachlorophenol (C)



12.159min (-0.000) 11672.81ng

response 26459

Ion	Exp%	Act%
265.70	100	100
268.00	62.60	64.75
264.00	62.50	62.37
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF041315\
Data File : BF078480.D
Acq On : 14 Apr 2015 2:17
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 07:55:56 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 14 07:20:26 2015
Response via : Initial Calibration

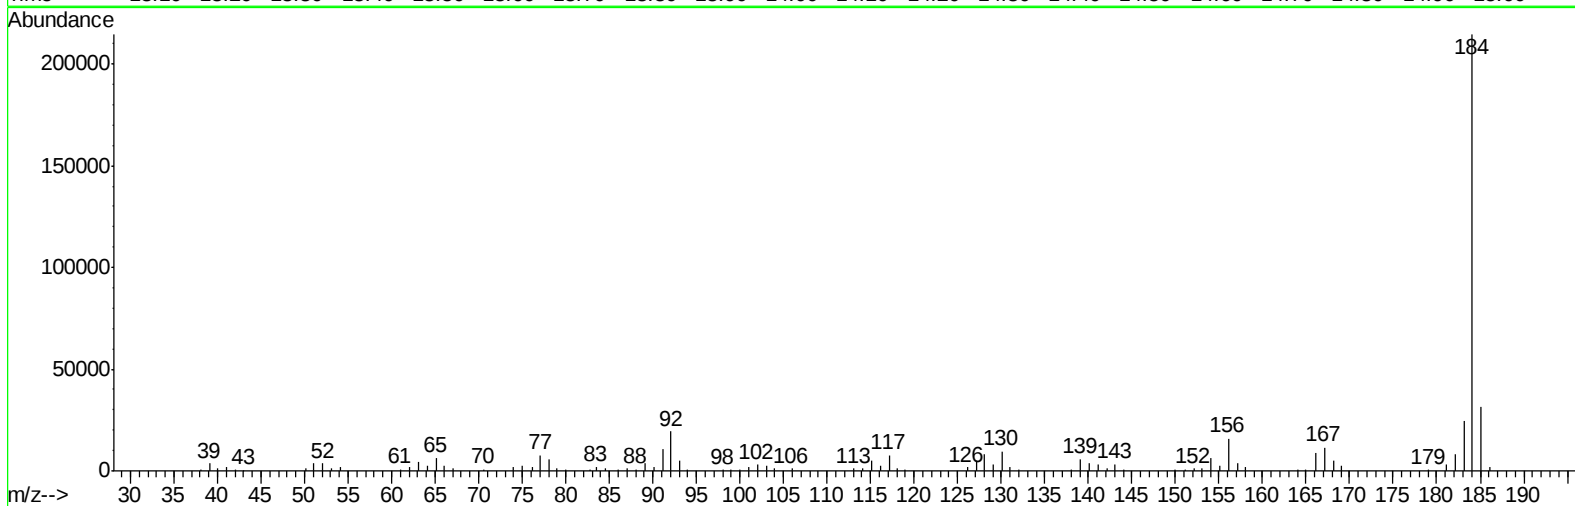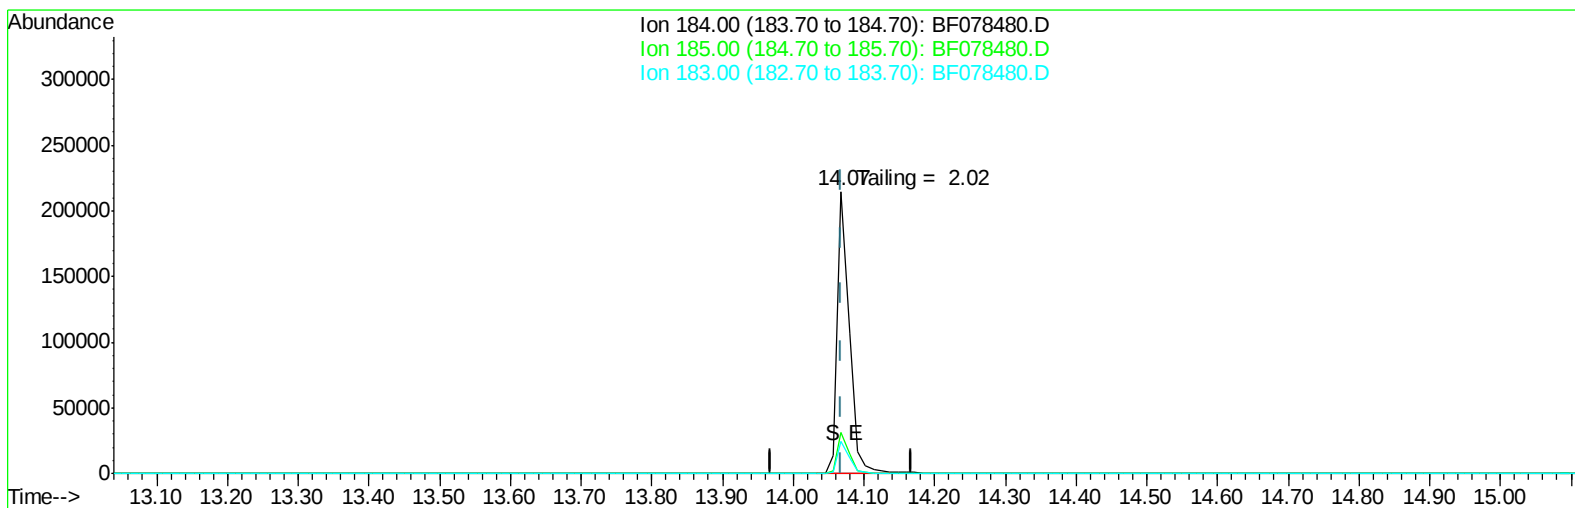

TIC: BF078480.D

(76) Benzidine

14.068min (-0.000) 18796.44ng

response 246804

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.58
183.00	11.90	11.52
0.00	0.00	0.00