

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041315\
 Data File : BF078462.D
 Acq On : 13 Apr 2015 16:13
 Operator : TP/IZ
 Sample : G1787-13
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 LS-SD06A

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.244	4	5	27	rVB3	95711	395203	10.21%	3.934%
2	1.507	27	28	35	rVV	298034	503908	13.02%	5.016%
3	1.610	35	37	81	rVB	1724957	3870525	100.00%	38.531%
4	4.490	287	289	299	rVB	34762	50803	1.31%	0.506%
5	5.084	339	341	347	rBV	383774	463867	11.98%	4.618%
6	6.422	456	458	461	rBV	347023	465786	12.03%	4.637%
7	6.536	466	468	471	rBV	394122	498654	12.88%	4.964%
8	6.833	491	494	496	rBV	137030	159499	4.12%	1.588%
9	7.016	508	510	512	rBV	349897	346212	8.94%	3.447%
10	7.530	552	555	557	rBV	330960	289458	7.48%	2.882%
11	8.410	629	632	634	rBV	194391	219758	5.68%	2.188%
12	9.759	747	750	752	rBV	527481	542766	14.02%	5.403%
13	10.559	818	820	823	rVB	198367	263562	6.81%	2.624%
14	11.542	903	906	908	rBV	325017	369361	9.54%	3.677%
15	12.388	978	980	983	rBV	294896	279714	7.23%	2.785%
16	14.377	1151	1154	1157	rBV	643037	646951	16.71%	6.440%
17	15.645	1263	1265	1268	rVB	322935	340114	8.79%	3.386%
18	17.383	1414	1417	1420	rBV	251747	339166	8.76%	3.376%


Sum of corrected areas: 10045307

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041315\
Data File : BF078462.D
Acq On : 13 Apr 2015 16:13
Operator : TP/IZ
Sample : G1787-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LS-SD06A

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

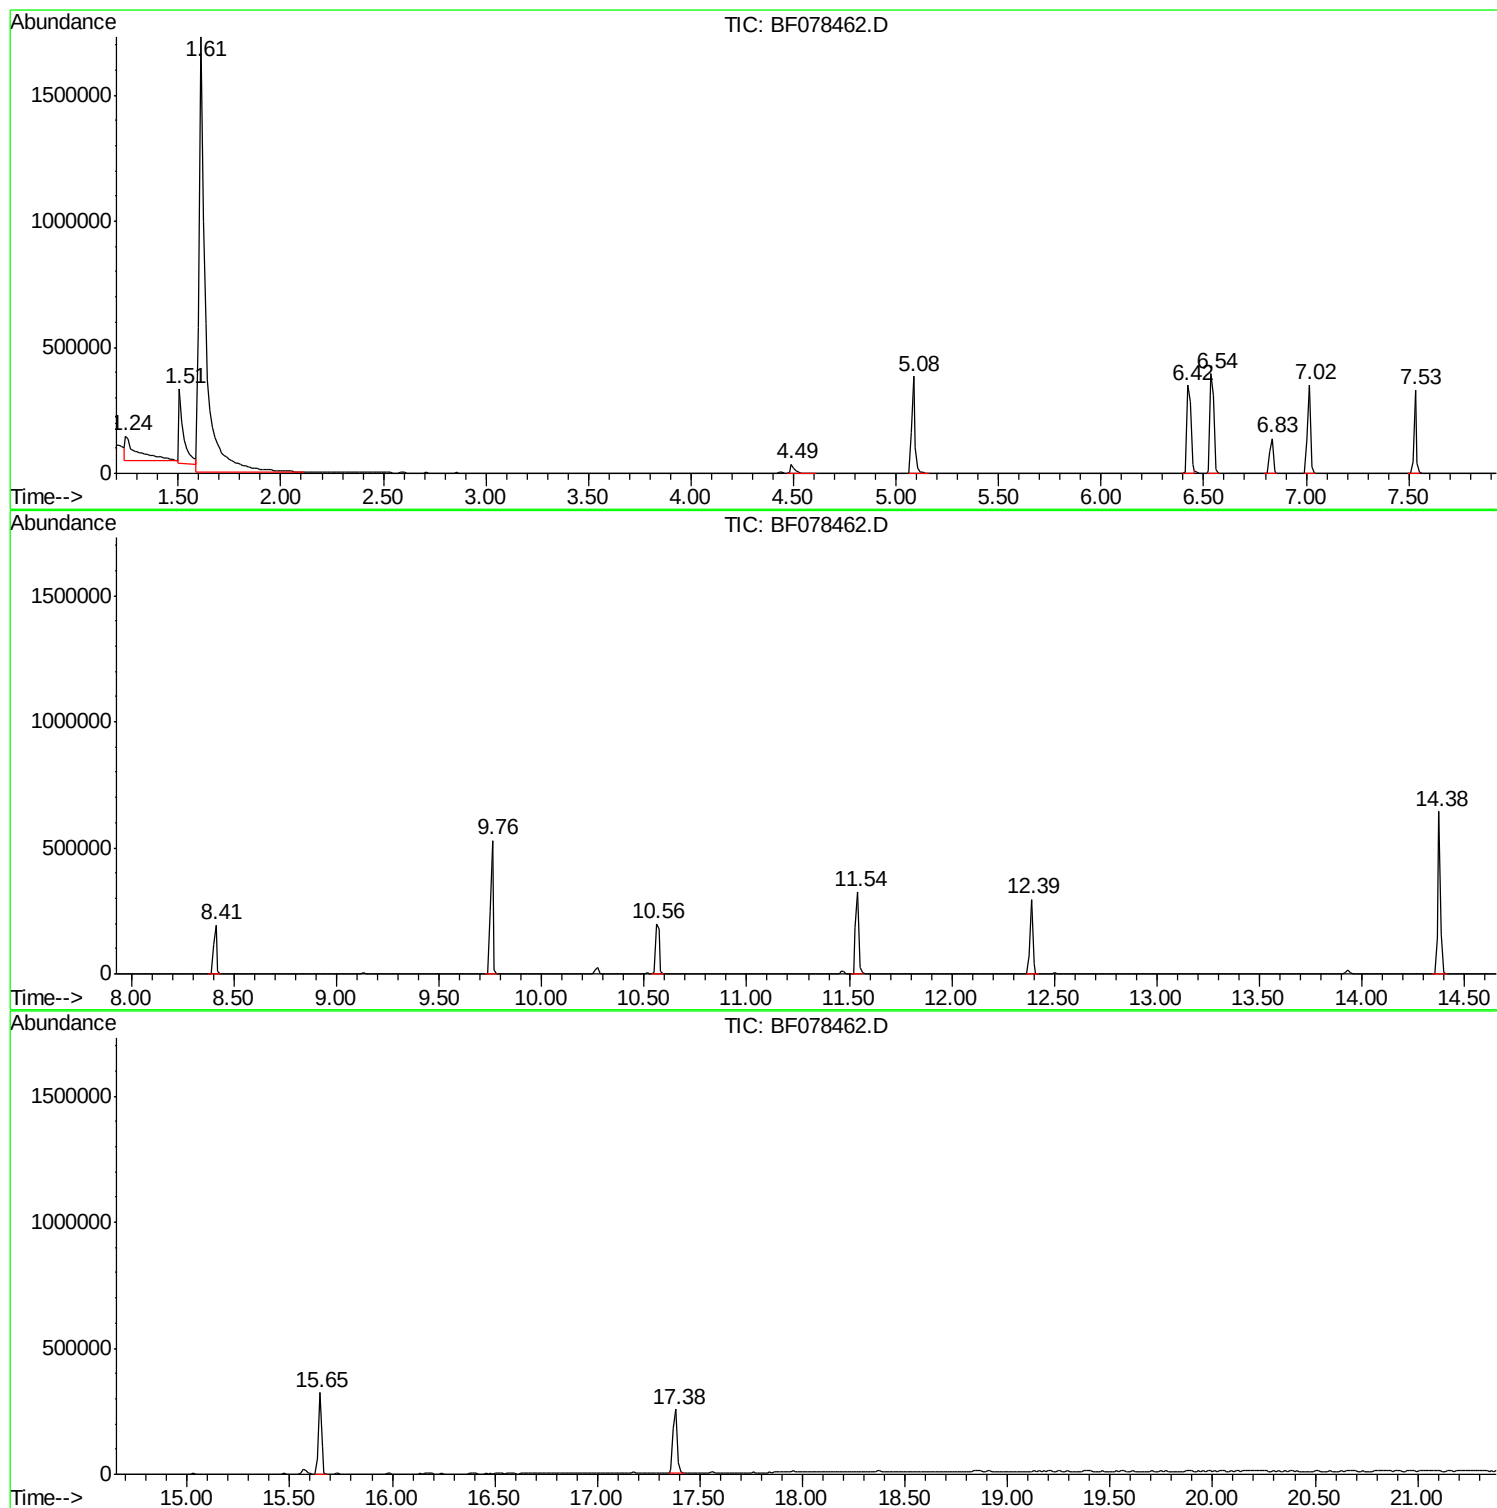

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041315\
Data File : BF078462.D
Acq On : 13 Apr 2015 16:13
Operator : TP/IZ
Sample : G1787-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LS-SD06A










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.24	49.56 ng	395203	1,4-Dichlorobenzene-d4	6.83

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2		2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3		N-Ethylformamide	73	C3H7NO	000627-45-2	9
4		1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	9
5		2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	9

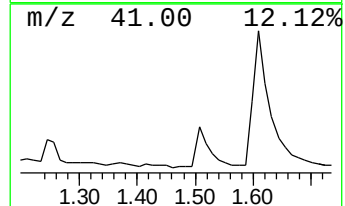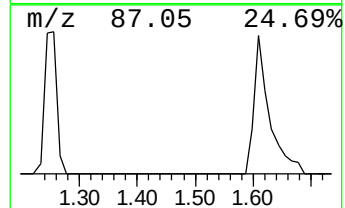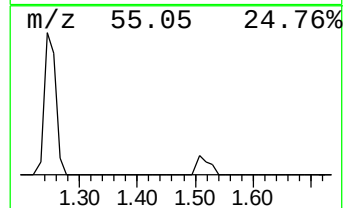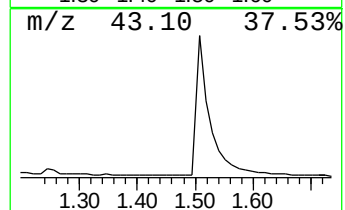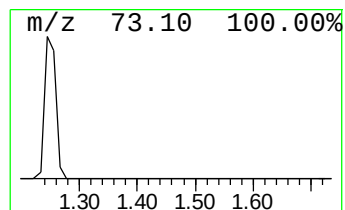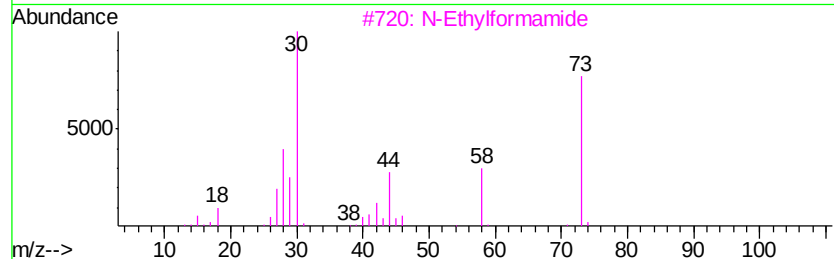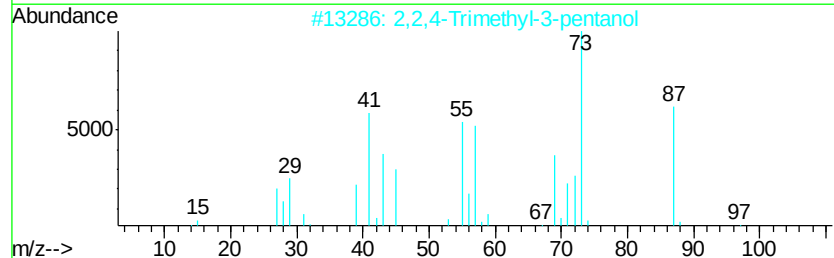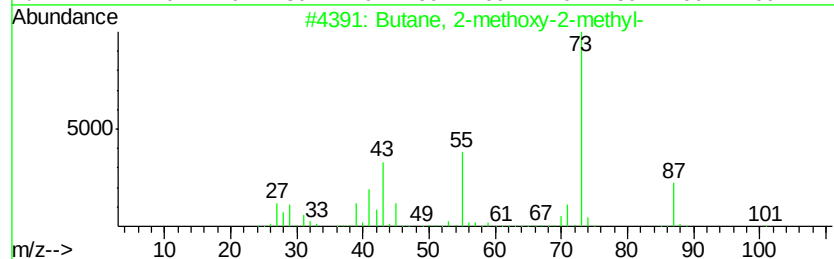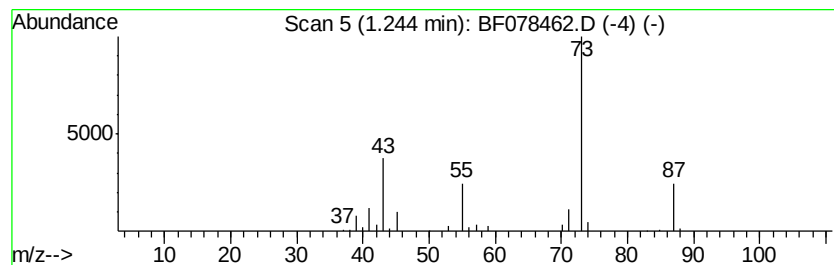

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041315\
Data File : BF078462.D
Acq On : 13 Apr 2015 16:13
Operator : TP/IZ
Sample : G1787-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LS-SD06A










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 6

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.49	6.37 ng	50803	1,4-Dichlorobenzene-d4	6.83

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	53		
2	5-Hexen-2-one	98	C6H10O	000109-49-9	9		
3	Acetone	58	C3H6O	000067-64-1	9		
4	3-Octanol	130	C8H18O	000589-98-0	9		
5	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	9		

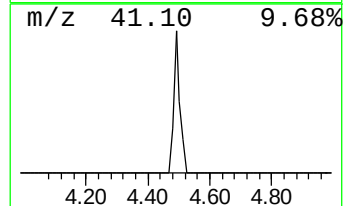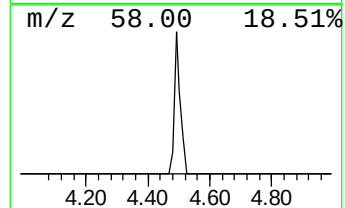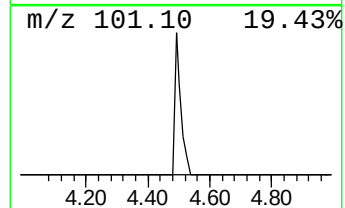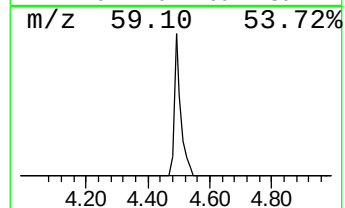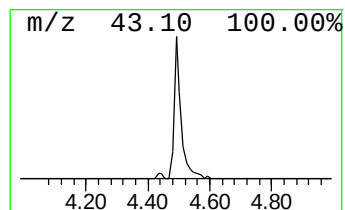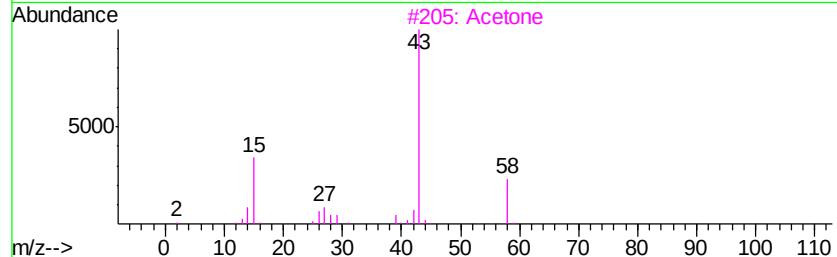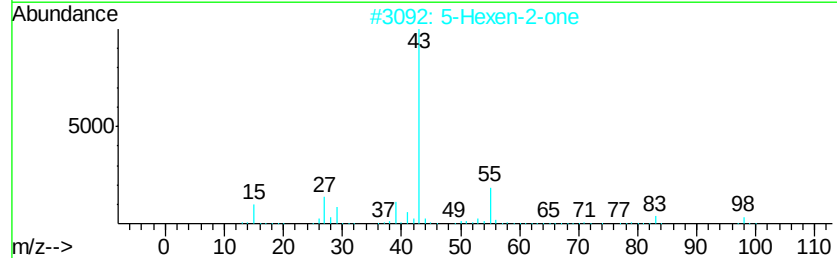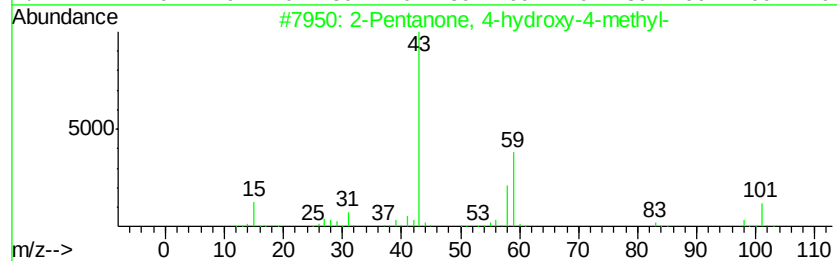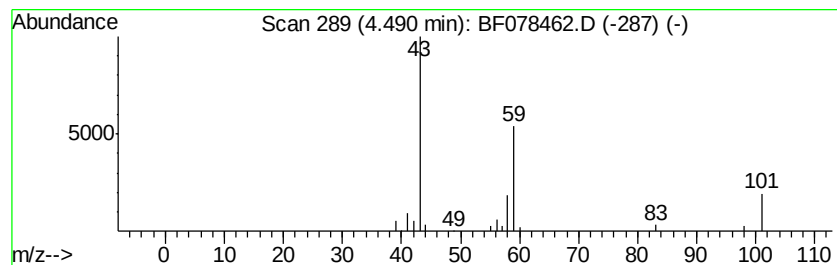

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041315\
Data File : BF078462.D
Acq On : 13 Apr 2015 16:13
Operator : TP/IZ
Sample : G1787-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LS-SD06A










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 5 unknown6.54 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.54	62.53 ng	498654	1,4-Dichlorobenzene-d4	6.83

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35	
2	5-Aminoindole	132	C8H8N2	005192-03-0	12	
3	Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10	
4	Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9	
5	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9	

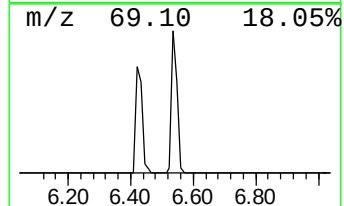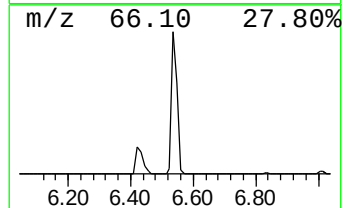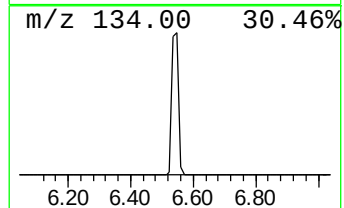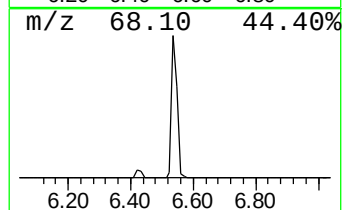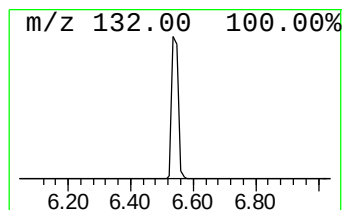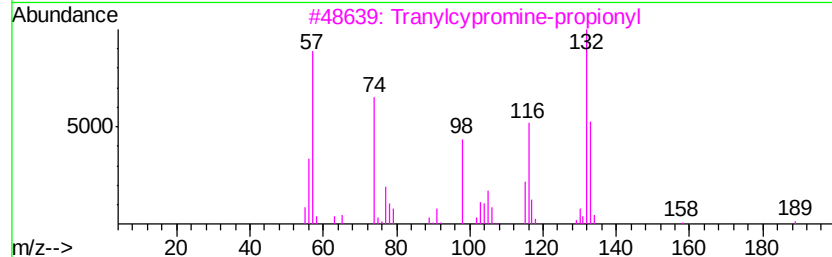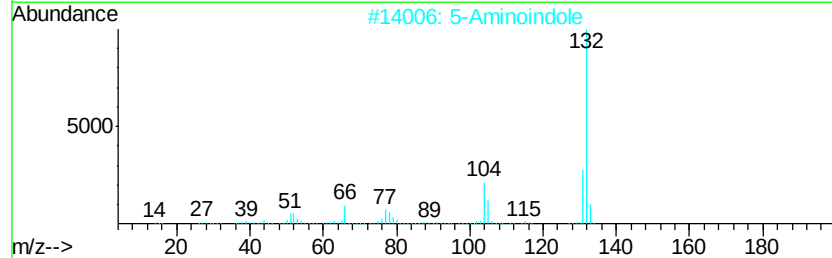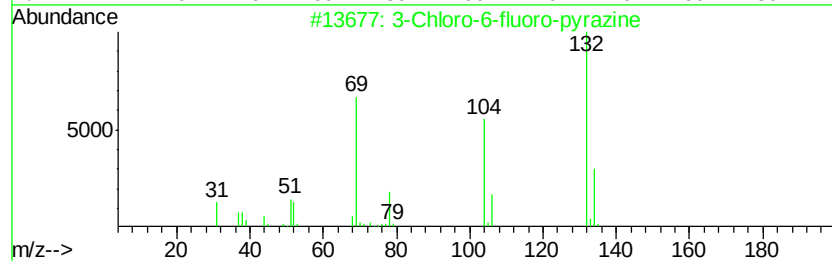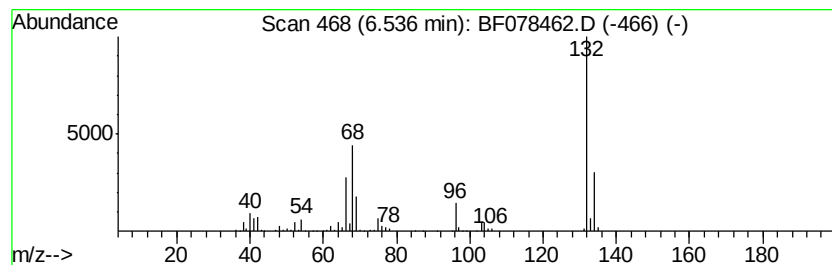

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041315\
Data File : BF078462.D
Acq On : 13 Apr 2015 16:13
Operator : TP/IZ
Sample : G1787-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LS-SD06A

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-methoxy...	1.24	49.6	ng	395203	1	6.83	159499	20.0
2-Pentanone, 4-hy...	4.49	6.4	ng	50803	1	6.83	159499	20.0
unknown6.54	6.54	62.5	ng	498654	1	6.83	159499	20.0