

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041315\
 Data File : BF078489.D
 Acq On : 14 Apr 2015 7:01
 Operator : TP/IZ
 Sample : G1787-03 5X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 LS-SD01C

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.518	27	29	35	rVB2	19778	53728	1.52%	0.787%
2	1.610	35	37	77	rVB	1612797	3535664	100.00%	51.789%
3	5.084	338	341	347	rBV	53840	67812	1.92%	0.993%
4	6.433	456	459	467	rBV	63445	76358	2.16%	1.118%
5	6.547	467	469	472	rBV	76179	84705	2.40%	1.241%
6	6.822	491	493	496	rBV	164031	223019	6.31%	3.267%
7	7.016	508	510	512	rVB	49476	57263	1.62%	0.839%
8	7.530	553	555	559	rBV	48294	48685	1.38%	0.713%
9	8.399	629	631	634	rBV	263395	325517	9.21%	4.768%
10	9.748	748	749	752	rVB	75003	84703	2.40%	1.241%
11	10.559	818	820	823	rBV	394453	388922	11.00%	5.697%
12	11.531	903	905	909	rBV2	47533	61920	1.75%	0.907%
13	12.388	977	980	981	rBV	333509	416715	11.79%	6.104%
14	13.874	1107	1110	1112	rVV	47043	46528	1.32%	0.682%
15	14.148	1131	1134	1136	rVB	44222	46514	1.32%	0.681%
16	14.365	1151	1153	1156	rVB	69968	88500	2.50%	1.296%
17	15.634	1261	1264	1266	rBV	480470	522425	14.78%	7.652%
18	15.714	1269	1271	1273	rVB	36641	43328	1.23%	0.635%
19	16.045	1298	1300	1302	rBV	33998	40958	1.16%	0.600%
20	16.891	1372	1374	1379	rBV	23650	58547	1.66%	0.858%
21	17.326	1409	1412	1417	rVV	367656	514084	14.54%	7.530%
22	18.617	1522	1525	1530	rVB4	20988	41208	1.17%	0.604%


Sum of corrected areas: 6827103

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041315\
Data File : BF078489.D
Acq On : 14 Apr 2015 7:01
Operator : TP/IZ
Sample : G1787-03 5X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LS-SD01C

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

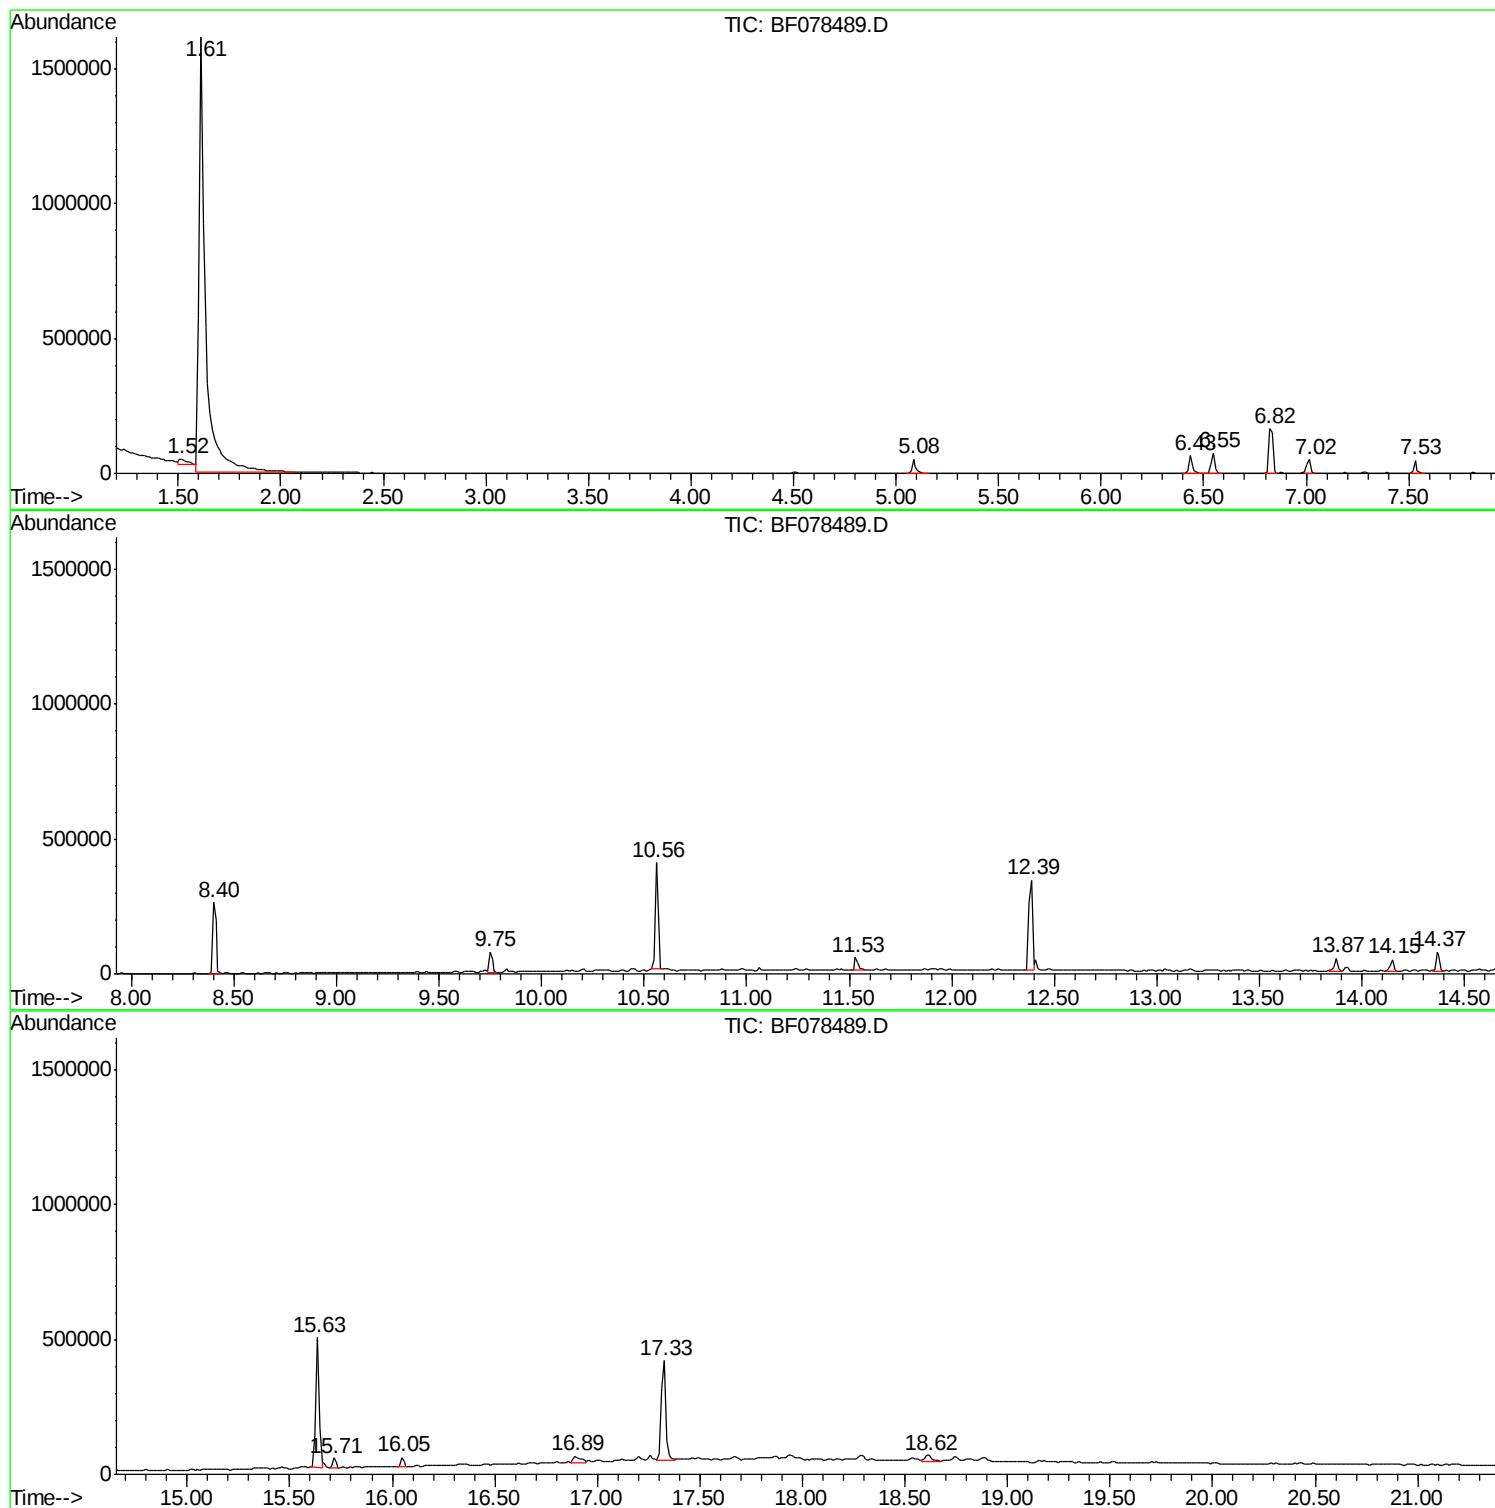

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041315\
Data File : BF078489.D
Acq On : 14 Apr 2015 7:01
Operator : TP/IZ
Sample : G1787-03 5X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LS-SD01C










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 unknown6.55 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.55	7.60 ng	84705	1,4-Dichlorobenzene-d4	6.83

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	17
3		Amphetaminil	250	C17H18N2	017590-01-1	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	10
5		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9

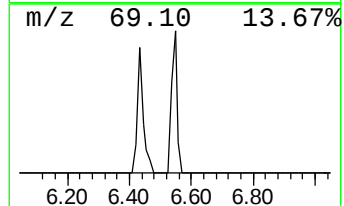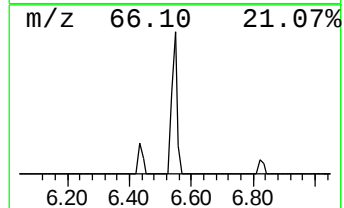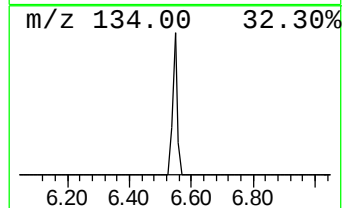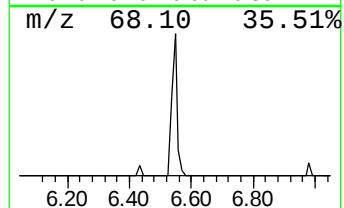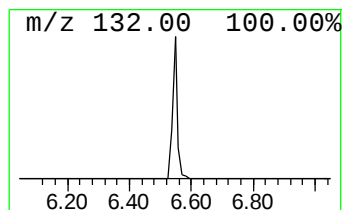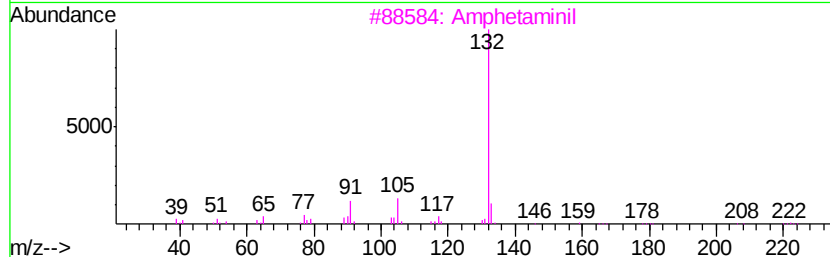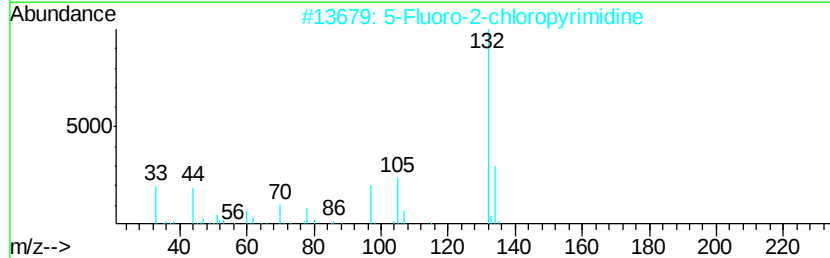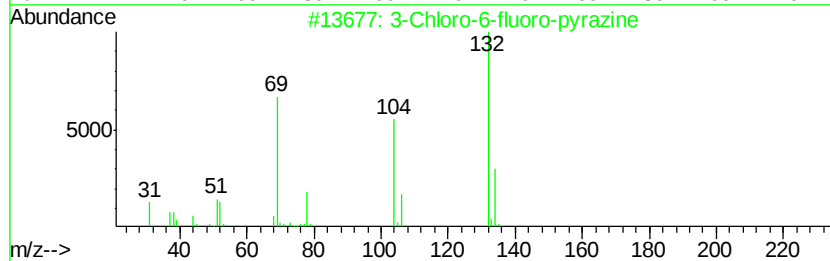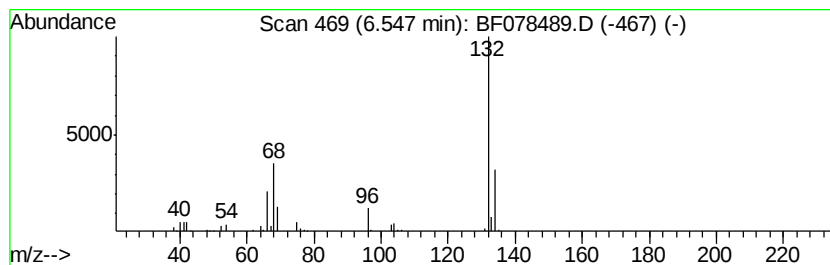

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041315\
Data File : BF078489.D
Acq On : 14 Apr 2015 7:01
Operator : TP/IZ
Sample : G1787-03 5X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LS-SD01C

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.55	6.55	7.6	ng	84705	1	6.83	223019	20.0