


Data Path : Z:\HPCHEM1\BNA_F\Data\BF041315\
 Data File : BF078480.D
 Acq On : 14 Apr 2015 2:17
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 31 14:58:34 2015

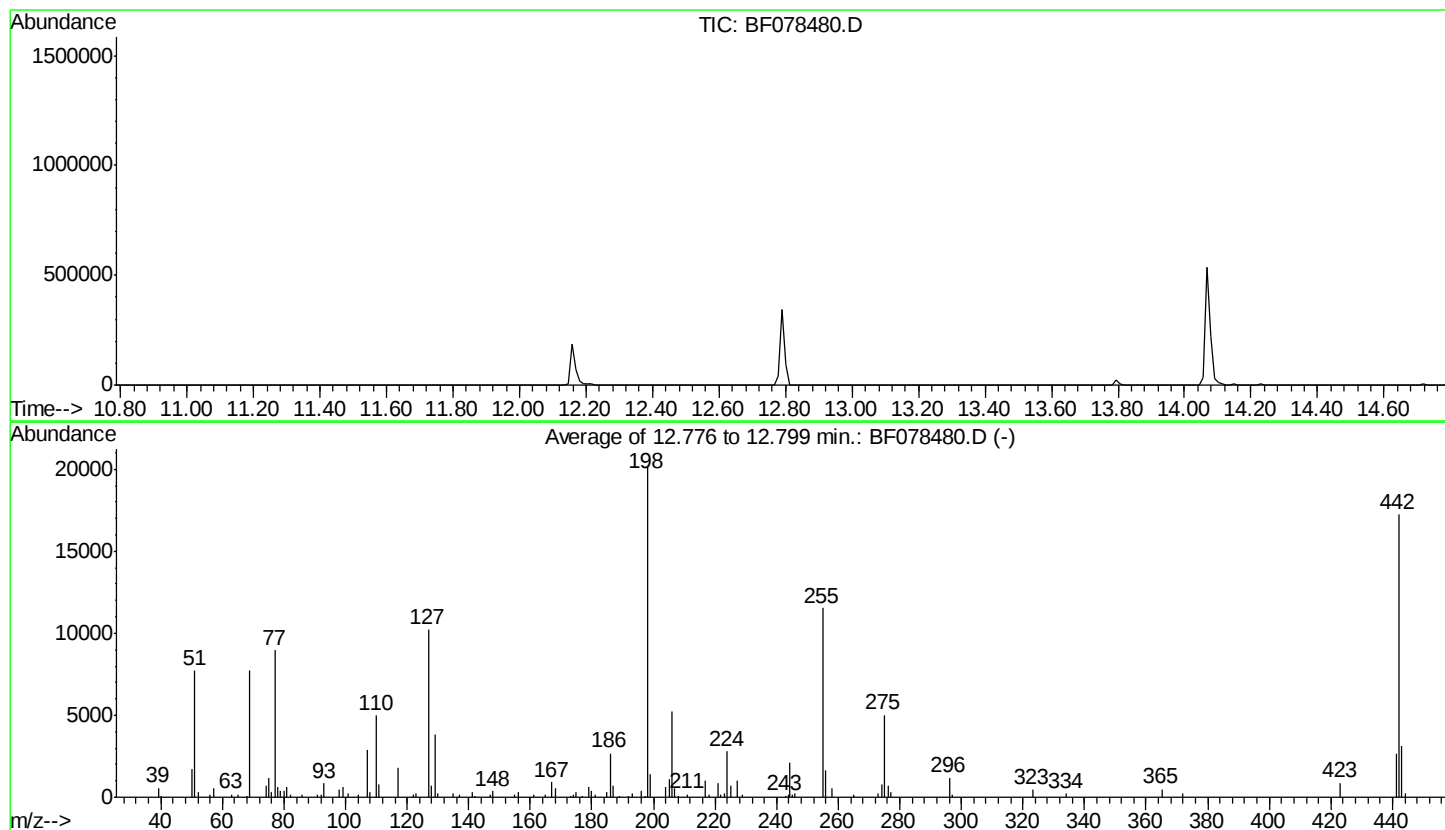

AutoFind: Scans 1014, 1015, 1016; Background Corrected with Scan 1011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	7708	PASS
68	69	0.00	2	1.3	103	PASS
69	198	0.00	100	38.1	7696	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.5	10207	PASS
197	198	0.00	2	0.5	100	PASS
198	198	100	100	100.0	20213	PASS
199	198	5	9	7.0	1412	PASS
275	198	10	60	24.9	5026	PASS
365	198	1	100	2.5	505	PASS
441	442	0.01	24	15.3	2627	PASS
442	198	50	100	85.2	17226	PASS
443	442	15	24	18.2	3140	PASS