

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041317\
 Data File : BF094391.D
 Acq On : 13 Apr 2017 15:19
 Operator : SJ/MA
 Sample : PB98215BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Apr 14 00:45:20 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 20 17:43:27 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ng	-8.05
21) Naphthalene-d8	0.00	136	0	0.00	ng	-10.85
38) Acenaphthene-d10	0.00	164	0	0.00	ng	-14.66
63) Phenanthrene-d10	0.00	188	0	0.00	ng	-17.39
75) Chrysene-d12	0.00	240	0	0.00	ng	-21.64
86) Perylene-d12	0.00	264	0	0.00	ng	-24.82
System Monitoring Compounds						
5) 2-Fluorophenol	5.79	112	135	0.00	ng	0.17
7) Phenol-d6	0.00	99	0	0.00	ng	
23) Nitrobenzene-d5	9.42	82	26814	0.00	ng	0.22
41) 2,4,6-Tribromophenol	0.00	330	0	0.00	ng	
44) 2-Fluorobiphenyl	13.23	172	5042	0.00	ng	-0.05
78) Terphenyl-d14	0.00	244	0	0.00	ng	


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041317\
Data File : BF094391.D
Acq On : 13 Apr 2017 15:19
Operator : SJ/MA
Sample : PB98215BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Apr 14 00:45:20 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 20 17:43:27 2017
Response via : Initial Calibration

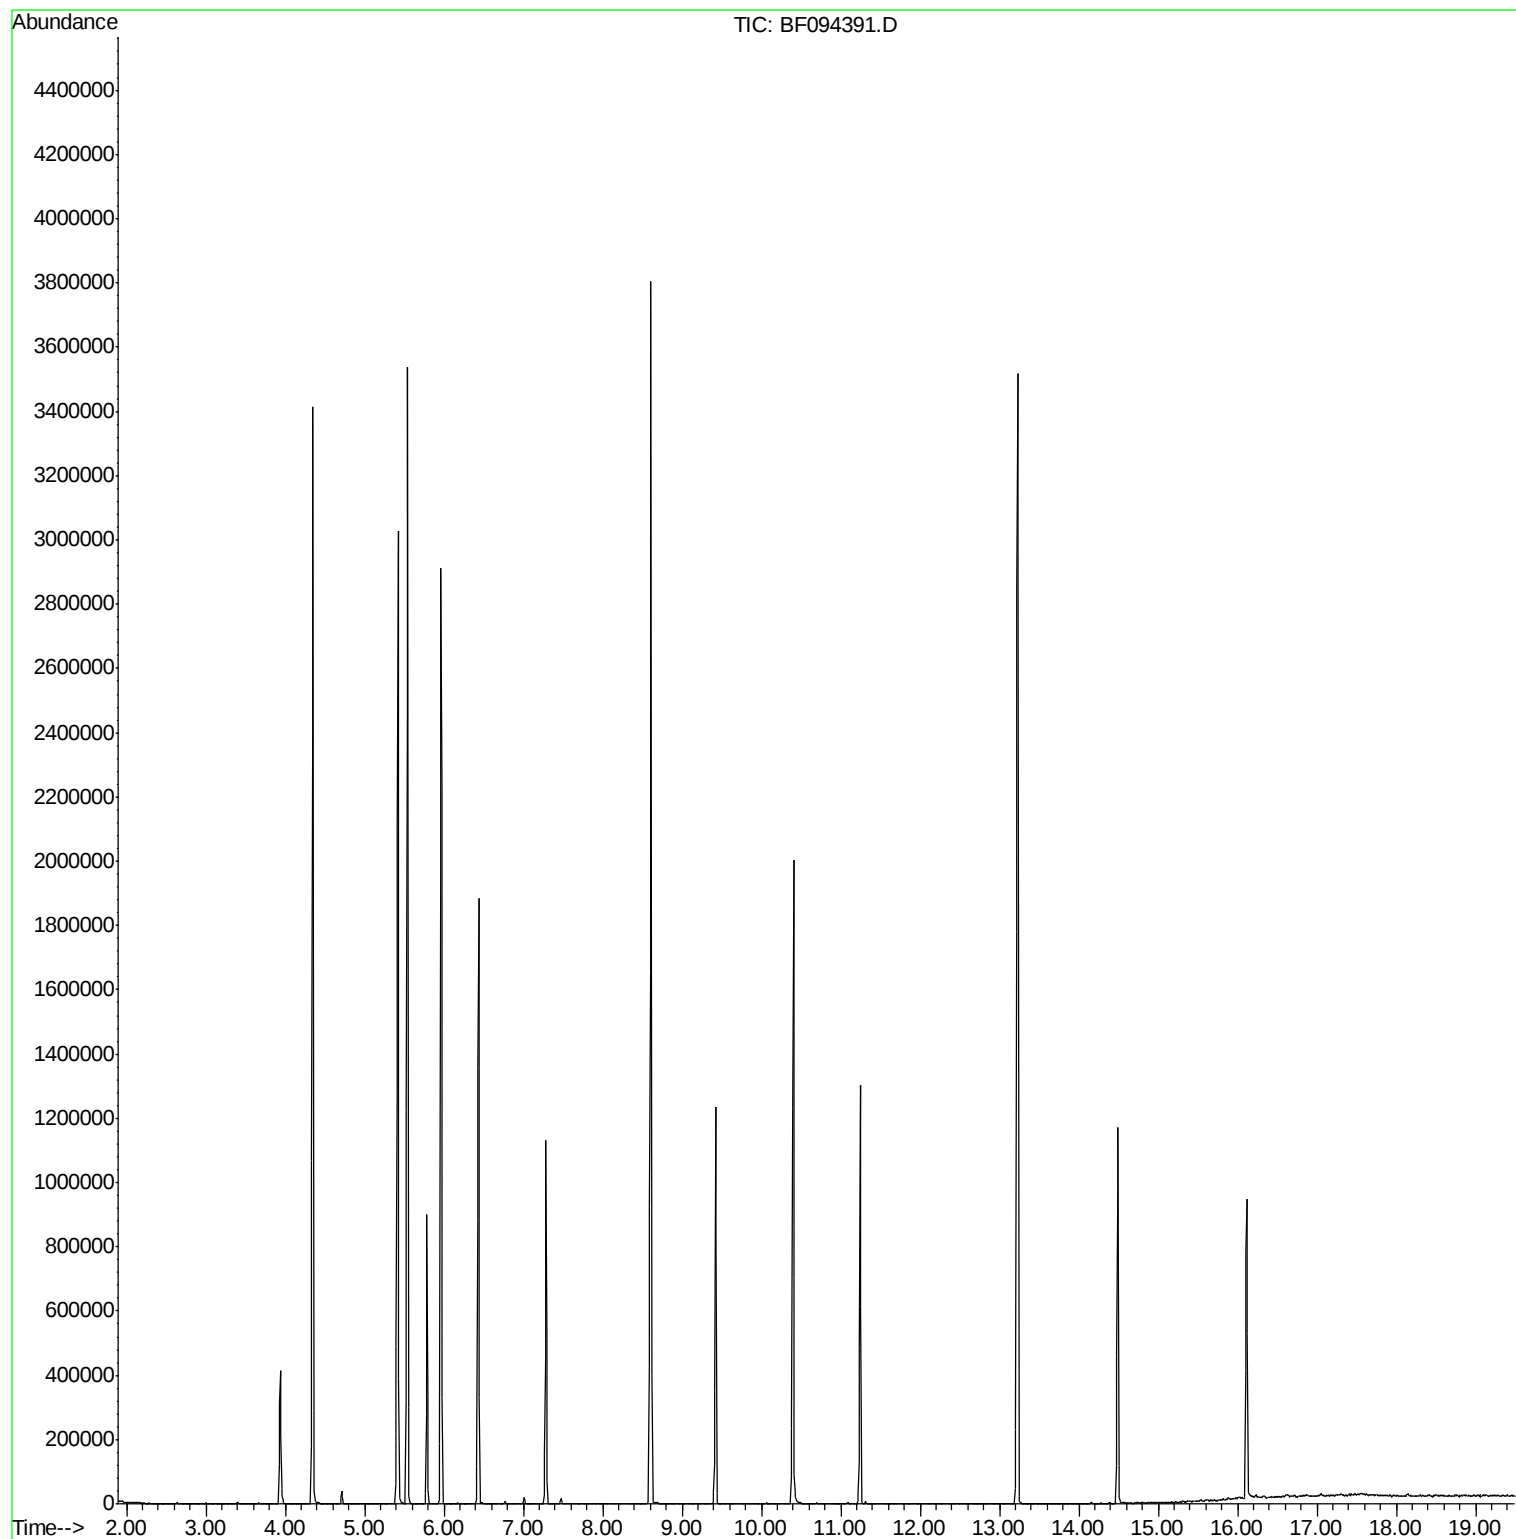

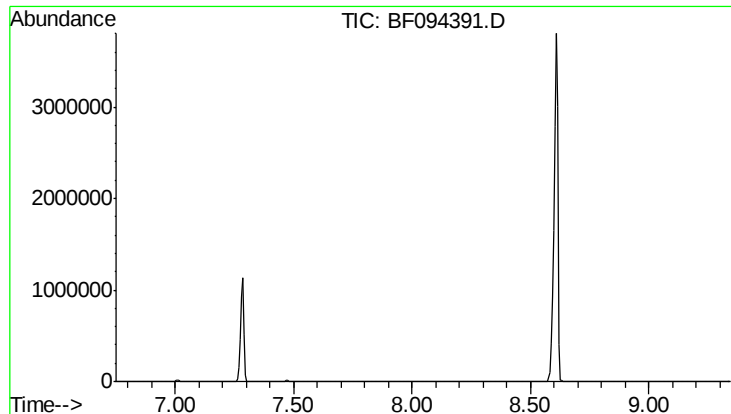

#1

1,4-Dichlorobenzene-d4

Concen: 0.00 ng

Expected RT: 8.05 min

Lab File: BF094391.D

Acq: 13 Apr 2017 15:19

Instrument :

BNA_F

ClientSampleId :



Tot Ion: 152

Sig Exp Ratio

152 100

150 142.5

115 60.1

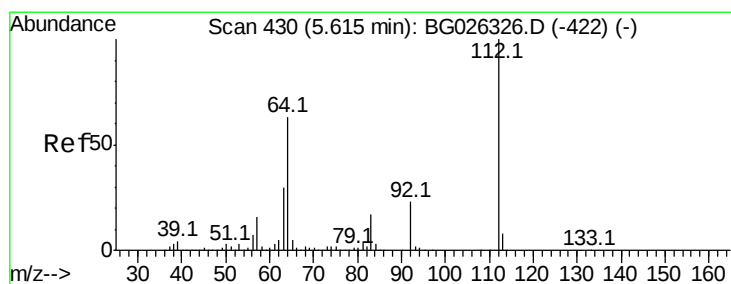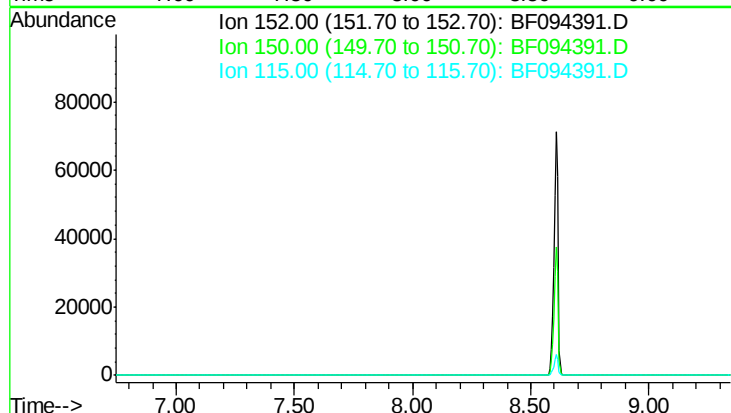

#5

2-Fluorophenol

Concen: 0.00 ng

RT: 5.79 min Scan# 663

Delta R.T. 0.17 min

Lab File: BF094391.D

Acq: 13 Apr 2017 15:19




Tgt Ion:112 Resp: 135


Ion Ratio Lower Upper

112 100

64 546.5 61.8 92.6#

63 789.3 37.2 55.8#

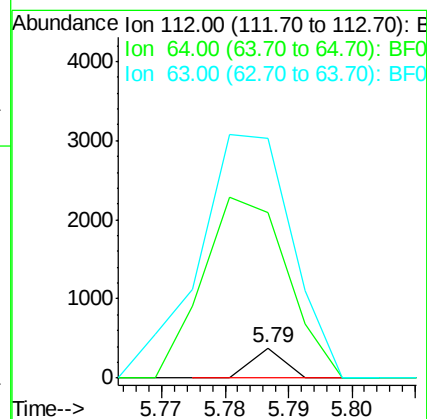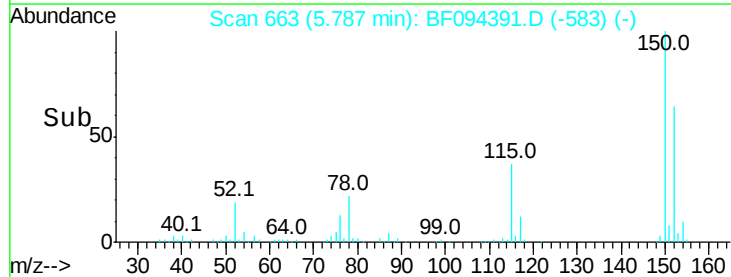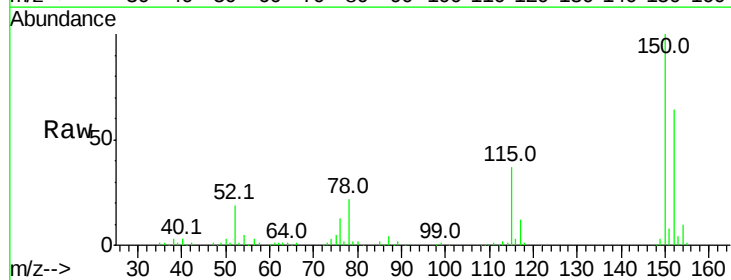

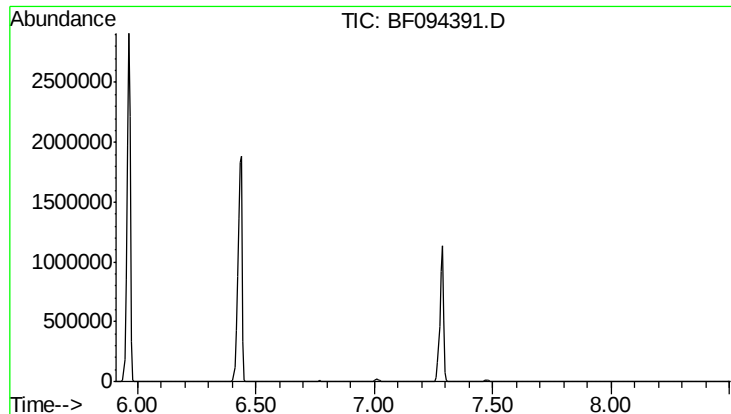

#7

Phenol-d6

Concen: 0.00 ng

Expected RT: 7.21 min

Lab File: BF094391.D

Acq: 13 Apr 2017 15:19

Tot Ion: 99

Sig Exp Ratio

99 100



42 25.6

71 47.0

Instrument :

BNA_F

ClientSampleId :

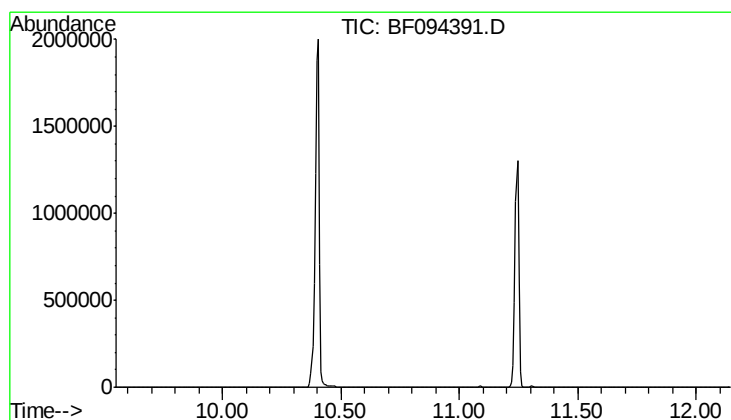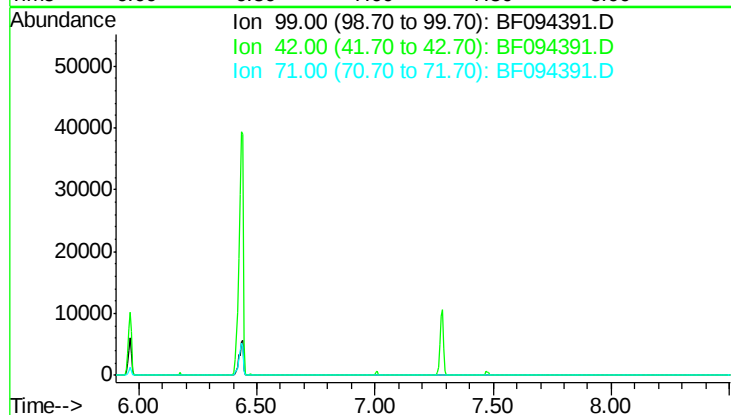

#21

Naphthalene-d8

Concen: 0.00 ng

Expected RT: 10.85 min

Lab File: BF094391.D

Acq: 13 Apr 2017 15:19

Tgt Ion: 136


Sig Exp Ratio


136 100

137 11.1

54 11.6

68 6.4

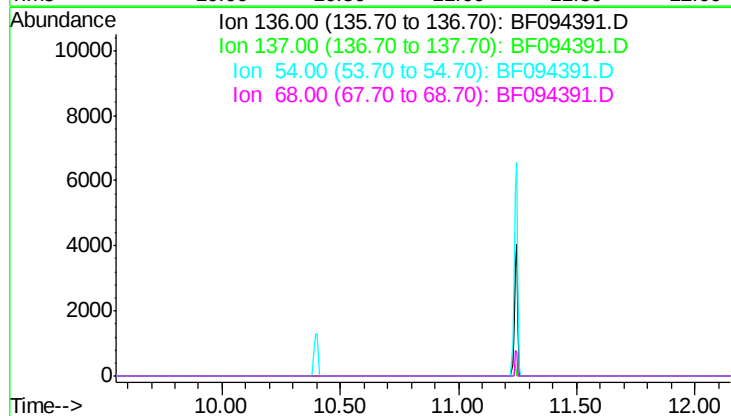

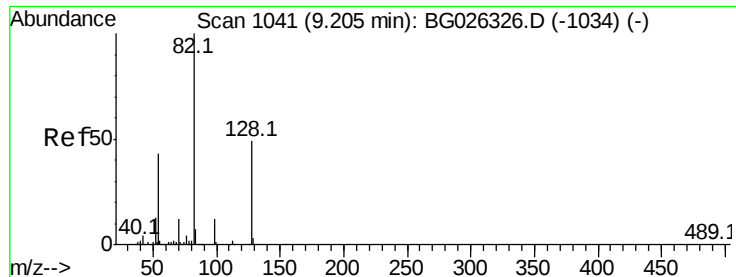

#23

Nitrobenzene-d5

Concen: 0.00 ng

RT: 9.42 min Scan# 1281

Delta R.T. 0.22 min

Lab File: BF094391.D

Acq: 13 Apr 2017 15:19

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 26814

Ion Ratio Lower Upper

82 100

128 0.0 26.4 39.6#




54 55.0 49.4 74.2

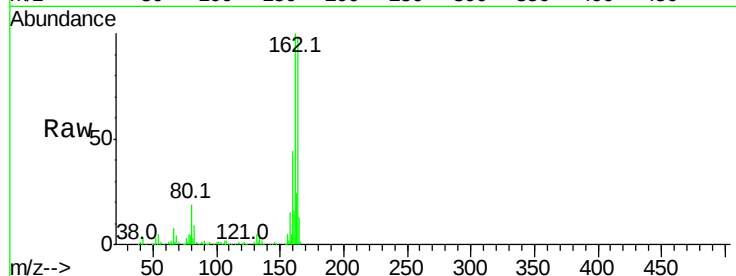

Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): BF0

Ion 54.00 (53.70 to 54.70): BF0

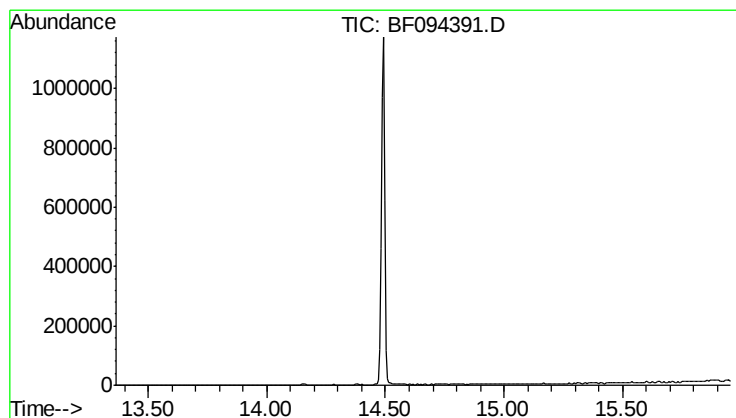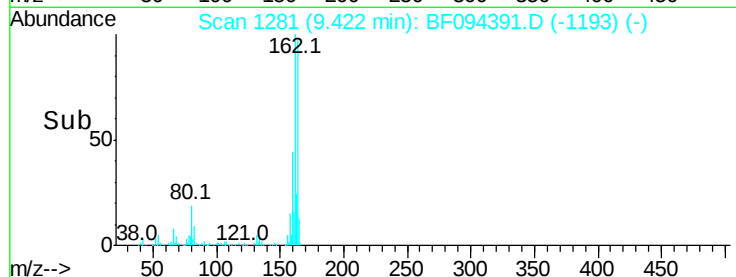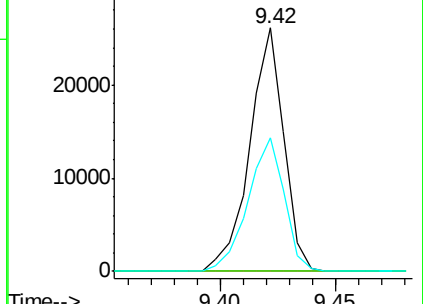

#38

Acenaphthene-d10

Concen: 0.00 ng

Expected RT: 14.66 min

Lab File: BF094391.D

Acq: 13 Apr 2017 15:19


Tgt Ion: 164


Sig Exp Ratio

164 100

162 106.4

160 43.4


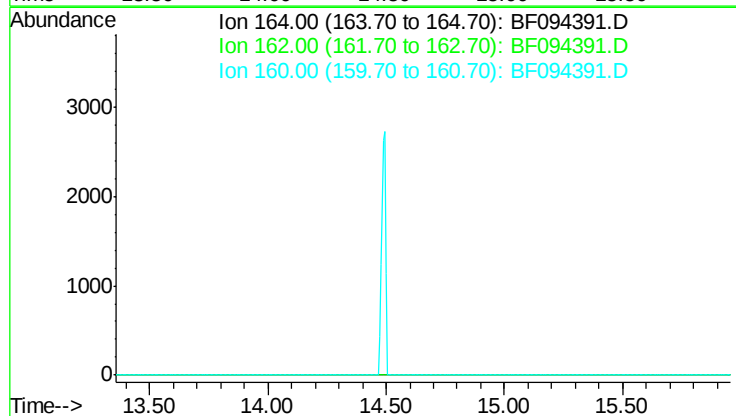


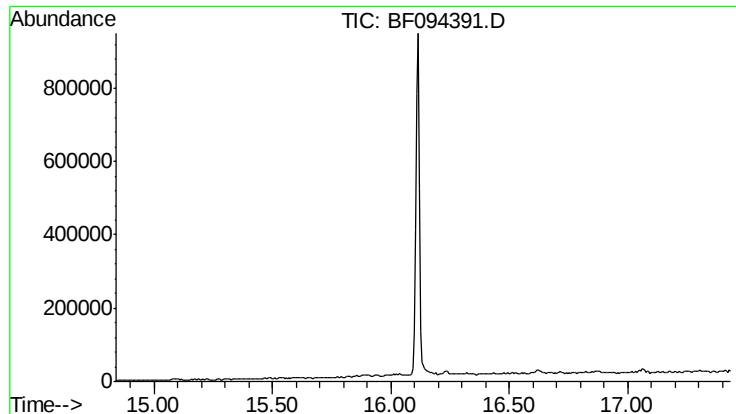

#41
 2,4,6-Tribromophenol
 Concen: 0.00 ng
 Expected RT: 16.14 min
 Lab File: BF094391.D
 Acq: 13 Apr 2017 15:19




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion: 330
 Sig Exp Ratio
 330 100
 332 96.6
 141 40.1

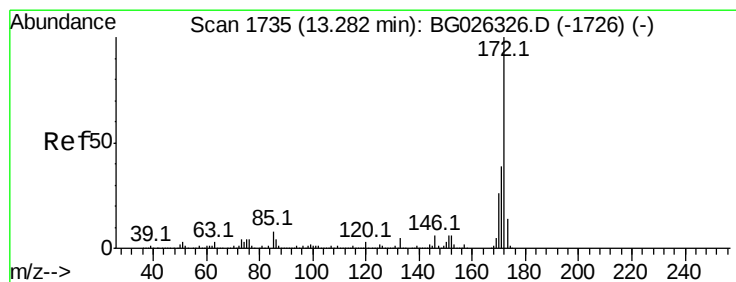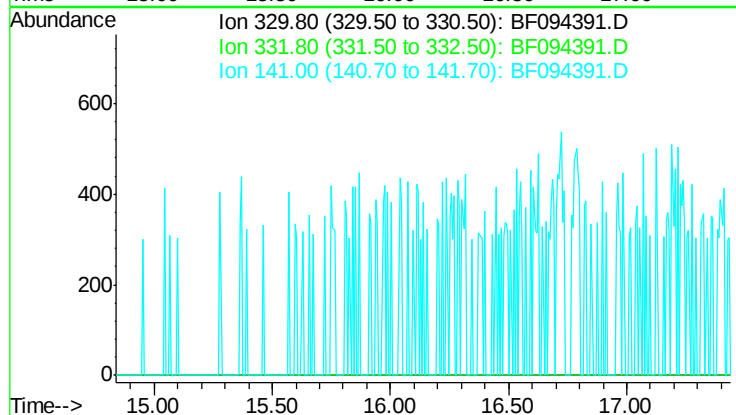

#44
 2-Fluorobiphenyl
 Concen: 0.00 ng
 RT: 13.23 min Scan# 1928
 Delta R.T. -0.05 min
 Lab File: BF094391.D
 Acq: 13 Apr 2017 15:19

Tgt Ion:172 Resp: 5042
 Ion Ratio Lower Upper
 172 100
 171 53.1 32.2 48.2#
 170 270.3 21.8 32.6#

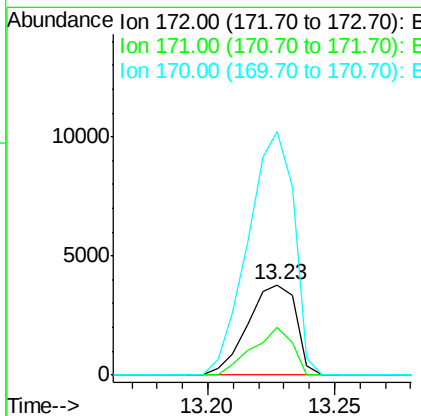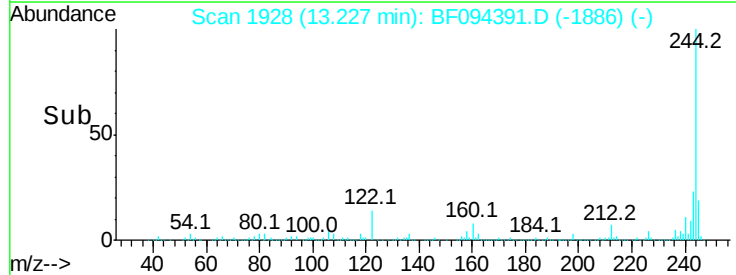
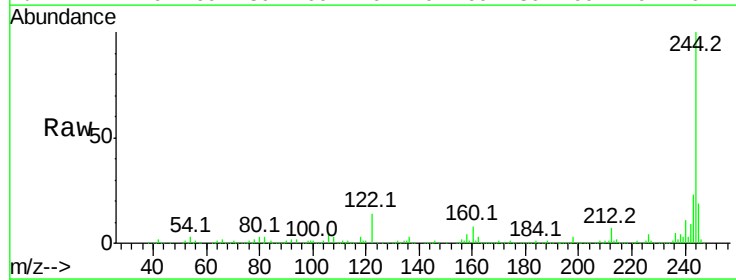


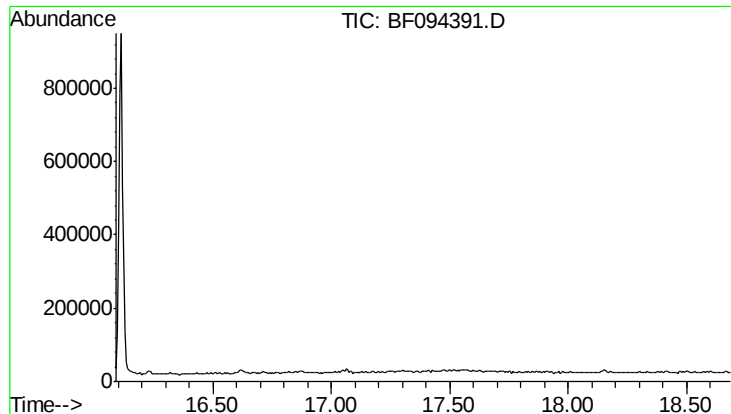

#63
 Phenanthrene-d10
 Concen: 0.00 ng
 Expected RT: 17.39 min
 Lab File: BF094391.D
 Acq: 13 Apr 2017 15:19


Instrument :
 BNA_F
 ClientSampleId :


Tot Ion: 188
 Sig Exp Ratio
 188 100
 94 7.3
 80 9.4

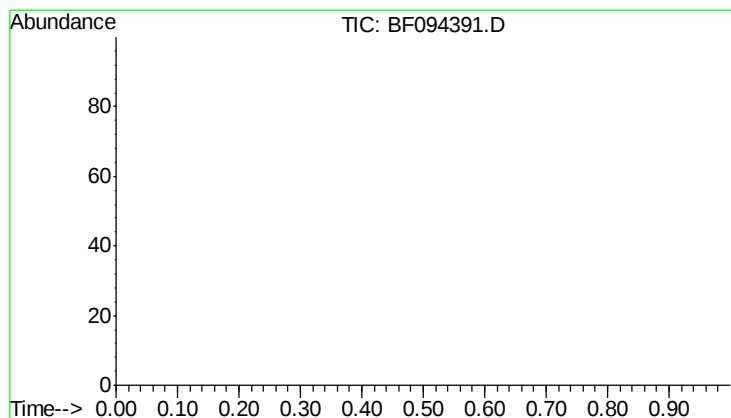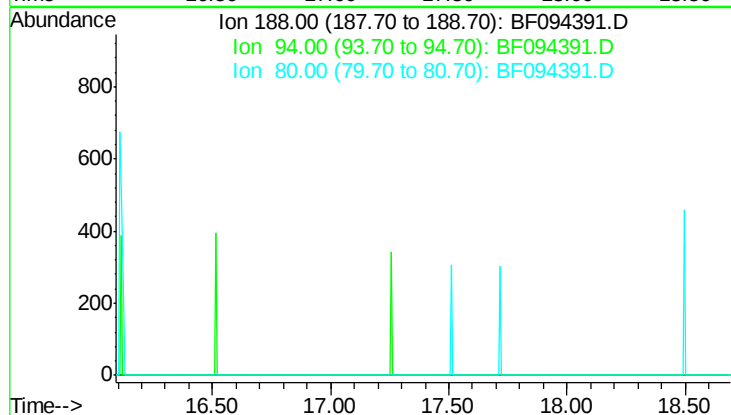

#75
 Chrysene-d12
 Concen: 0.00 ng
 Expected RT: 21.64 min
 Lab File: BF094391.D
 Acq: 13 Apr 2017 15:19

Tgt Ion: 240
 Sig Exp Ratio
 240 100
 120 7.1
 236 27.8


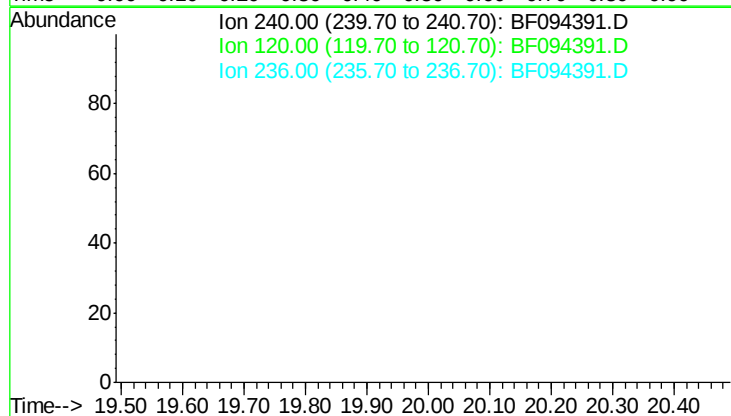


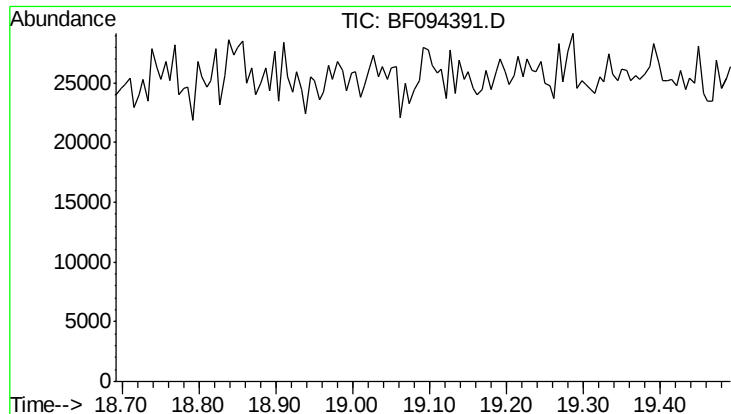

#78
 Terphenyl-d14
 Concen: 0.00 ng
 Expected RT: 19.99 min
 Lab File: BF094391.D
 Acq: 13 Apr 2017 15:19

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion: 244
 Sig Exp Ratio
 244 100
 212 12.5
 122 10.7

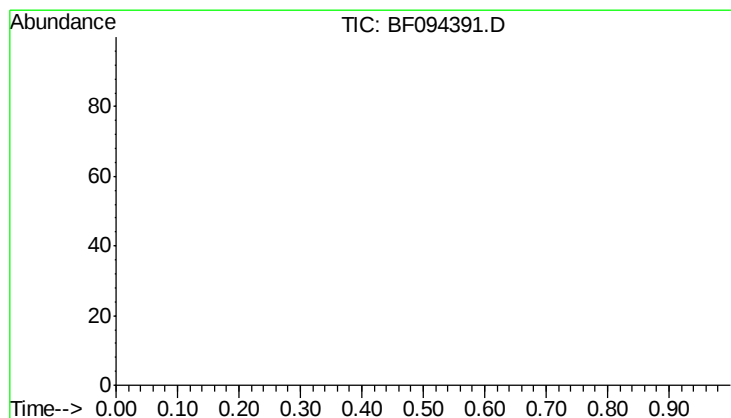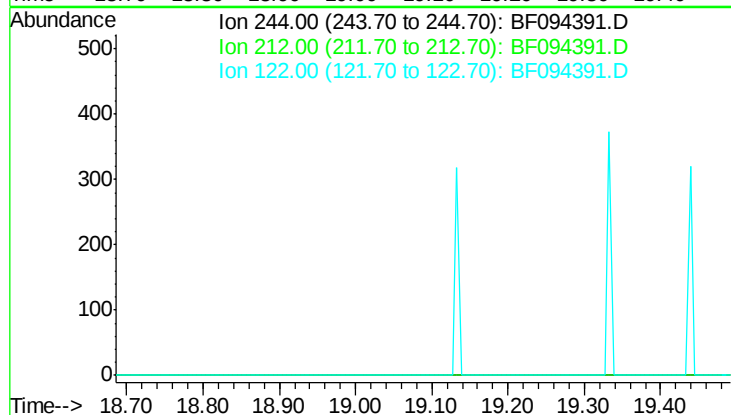

#86
 Perylene-d12
 Concen: 0.00 ng
 Expected RT: 24.82 min
 Lab File: BF094391.D
 Acq: 13 Apr 2017 15:19

Tgt Ion: 264
 Sig Exp Ratio
 264 100
 260 27.3
 265 22.8

