
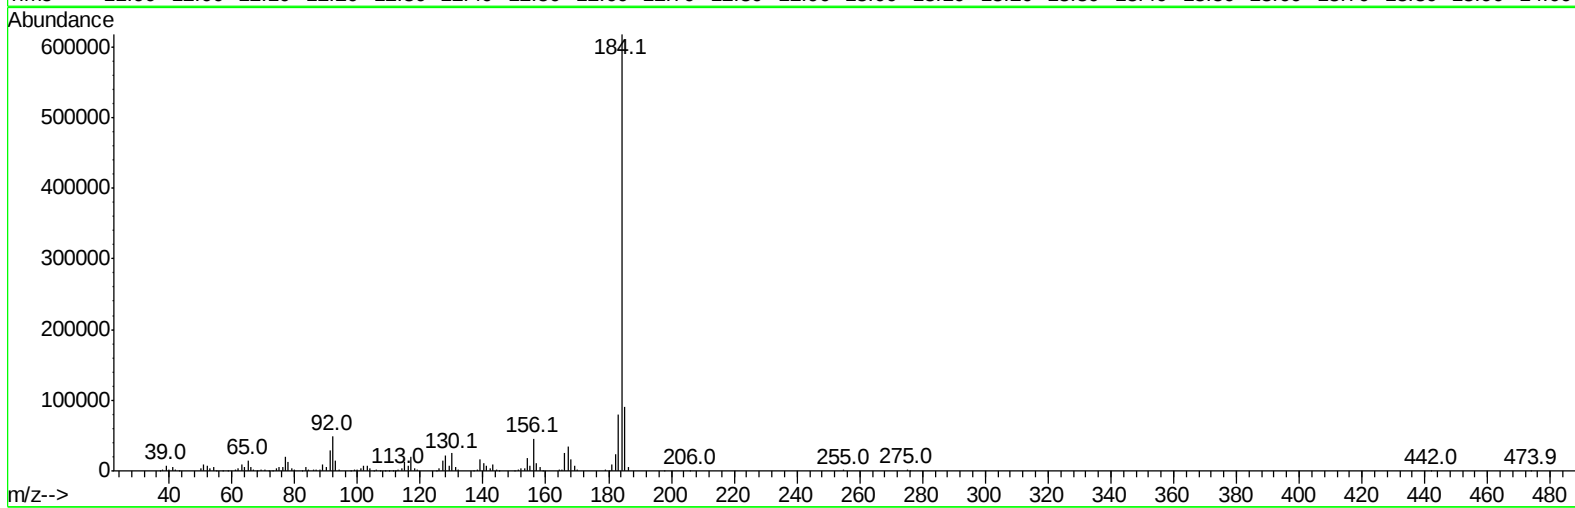


Data Path : Z:\HPCHEM1\BNA F\DATA\BF041317\
Data File : BF094388.D
Acq On : 13 Apr 2017 13:44
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 04:49:01 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 14 01:21:26 2017
Response via : Initial Calibration

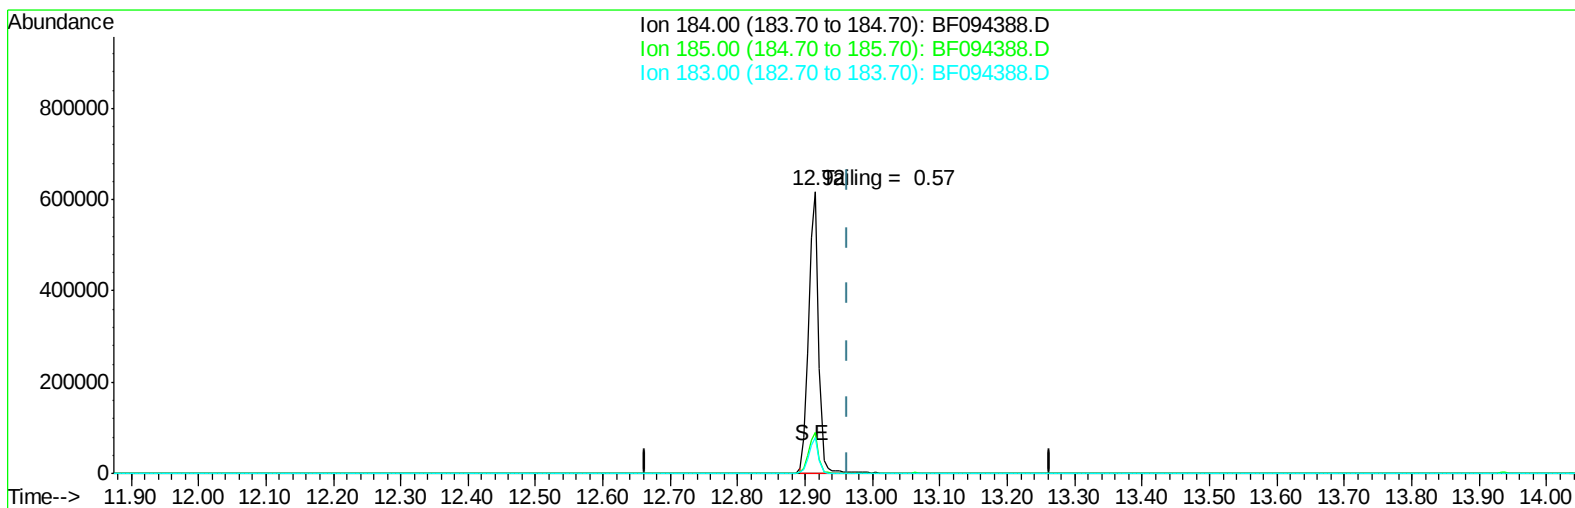

TIC: BF094388.D

(76) Benzidine



12.916min (-0.047) 0.00ng

response 635899

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.75#
183.00	12.20	12.81
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041317\
Data File : BF094388.D
Acq On : 13 Apr 2017 13:44
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 04:49:01 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 14 01:21:26 2017
Response via : Initial Calibration

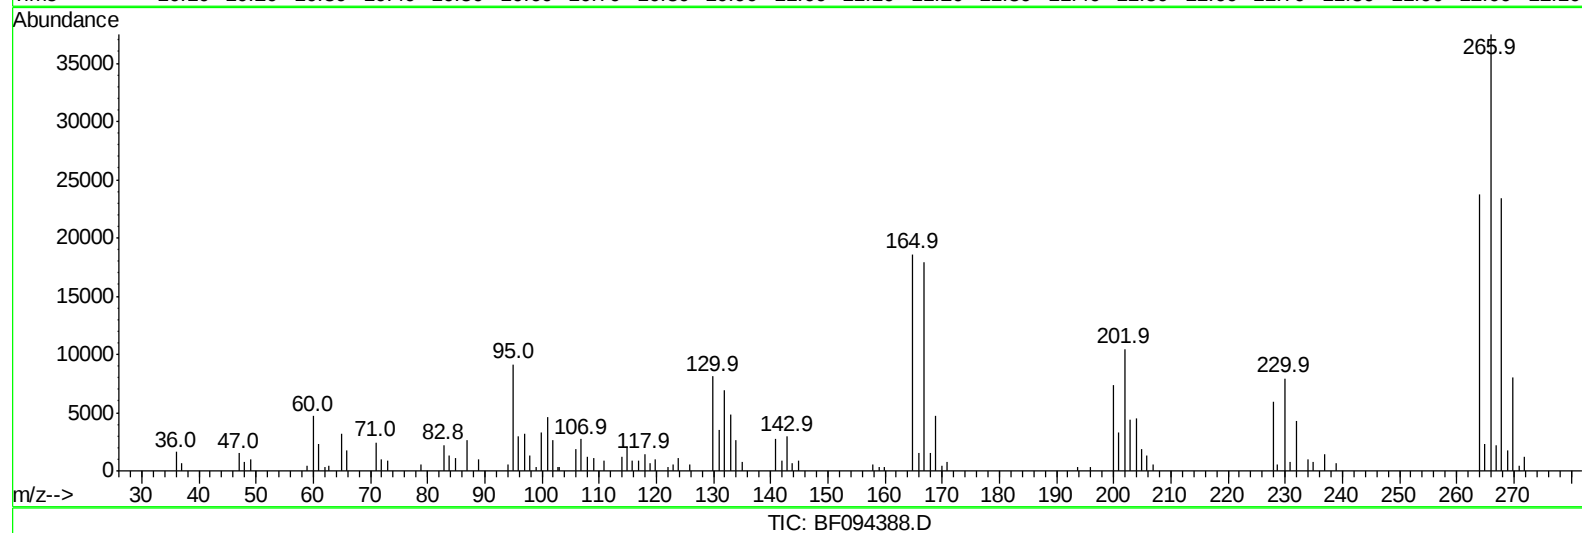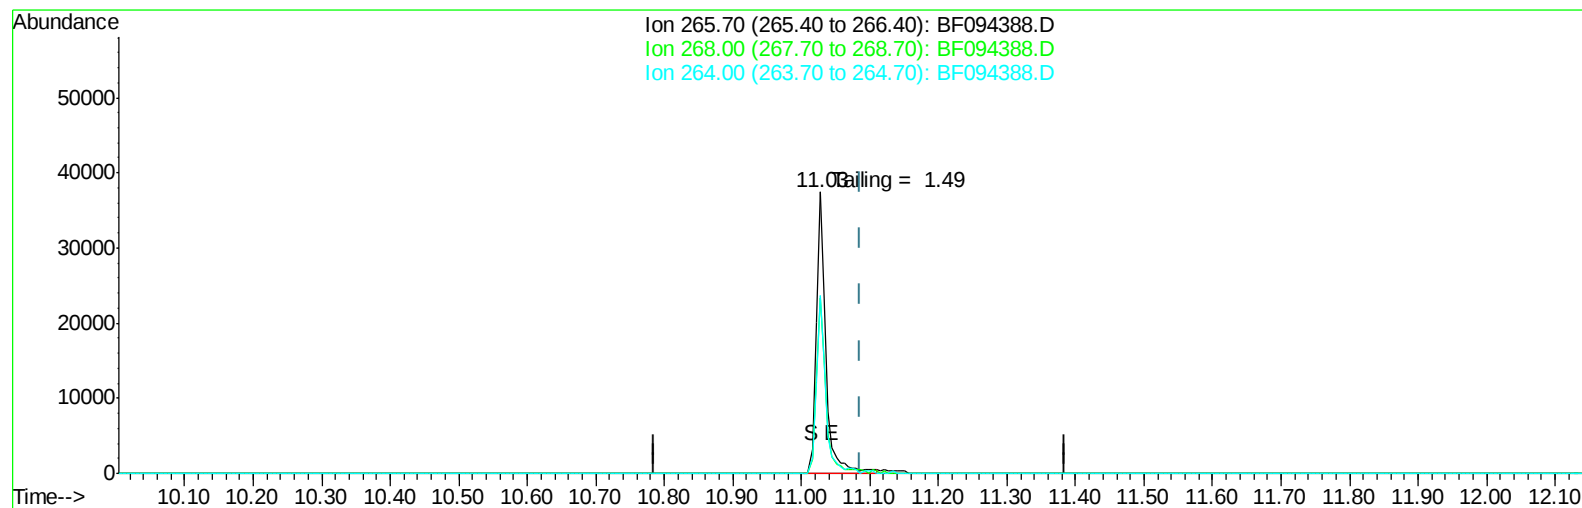

TIC: BF094388.D

(69) Pentachlorophenol (C)

11.027min (-0.059) 0.00ng

response 36829

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.37
264.00	64.60	63.29
0.00	0.00	0.00