
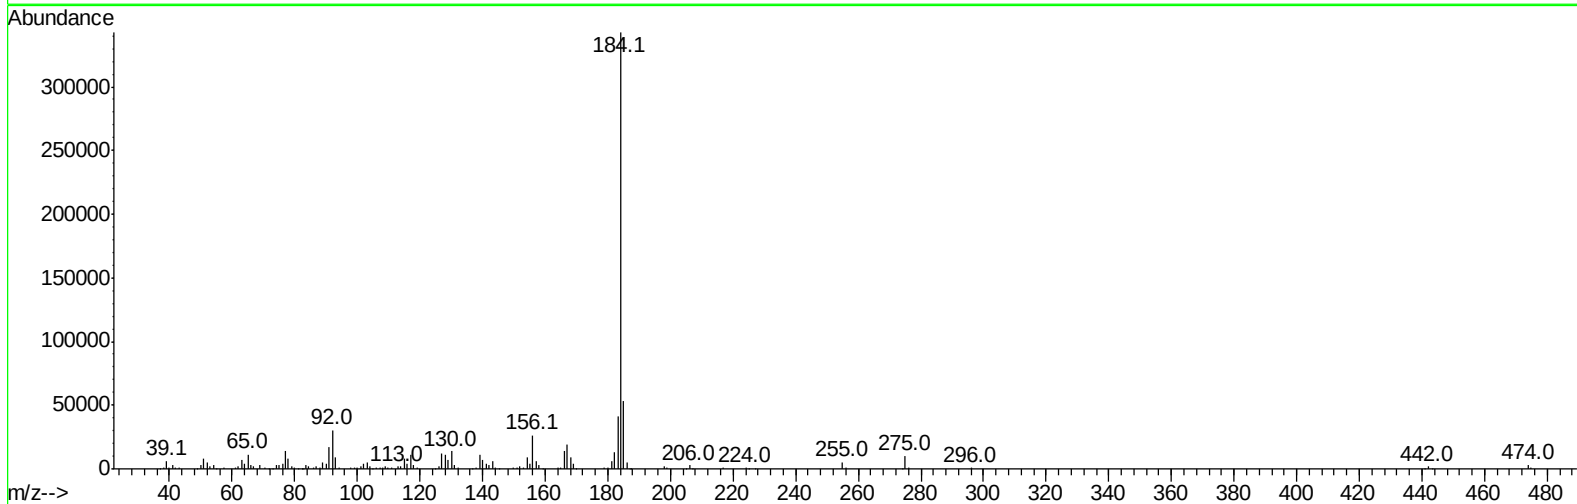


Data Path : Z:\HPCHEM1\BNA F\DATA\BF041317\
Data File : BF094413.D
Acq On : 14 Apr 2017 2:35
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 04:53:13 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 14 01:21:26 2017
Response via : Initial Calibration

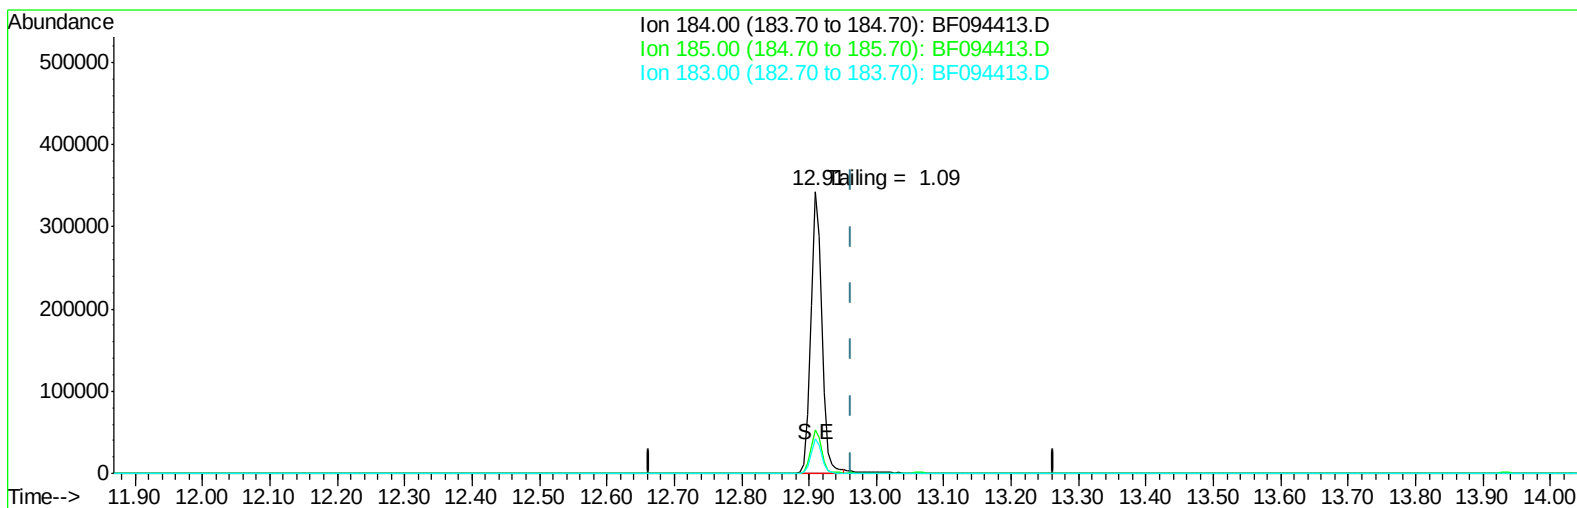

TIC: BF094413.D

(76) Benzidine



12.910min (-0.053) 0.00ng

response 385476

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	15.53
183.00	12.20	12.07
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041317\
Data File : BF094413.D
Acq On : 14 Apr 2017 2:35
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 04:53:13 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 14 01:21:26 2017
Response via : Initial Calibration

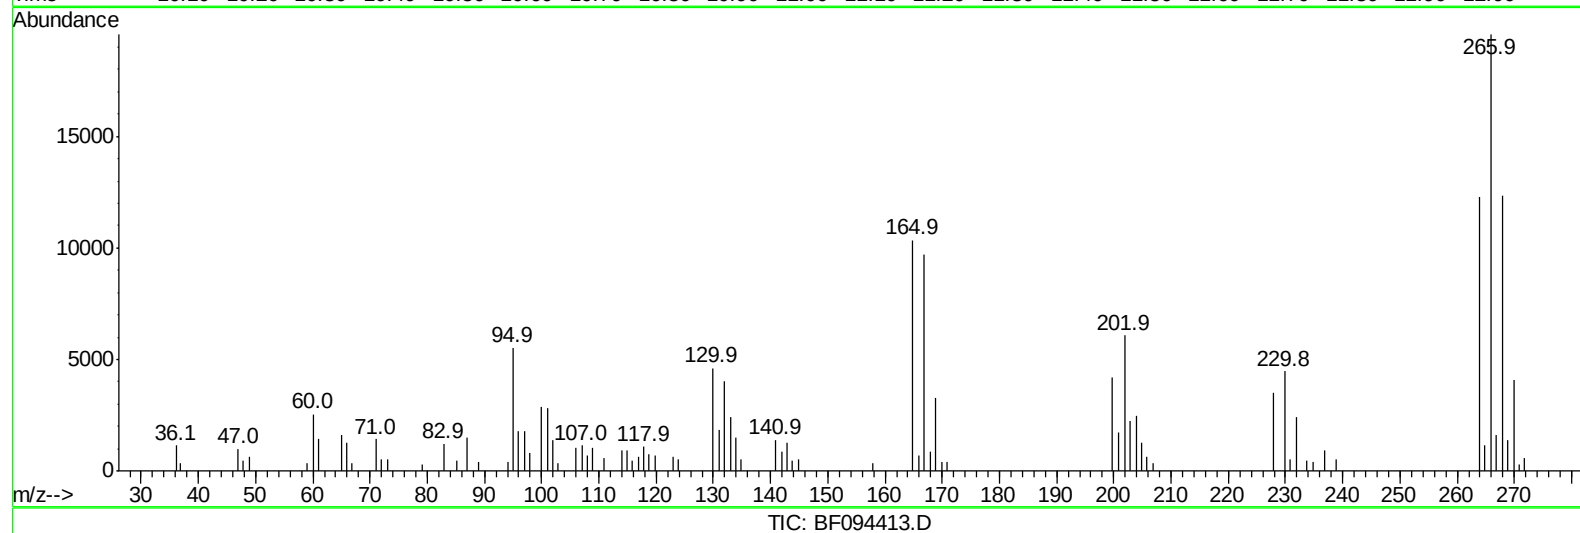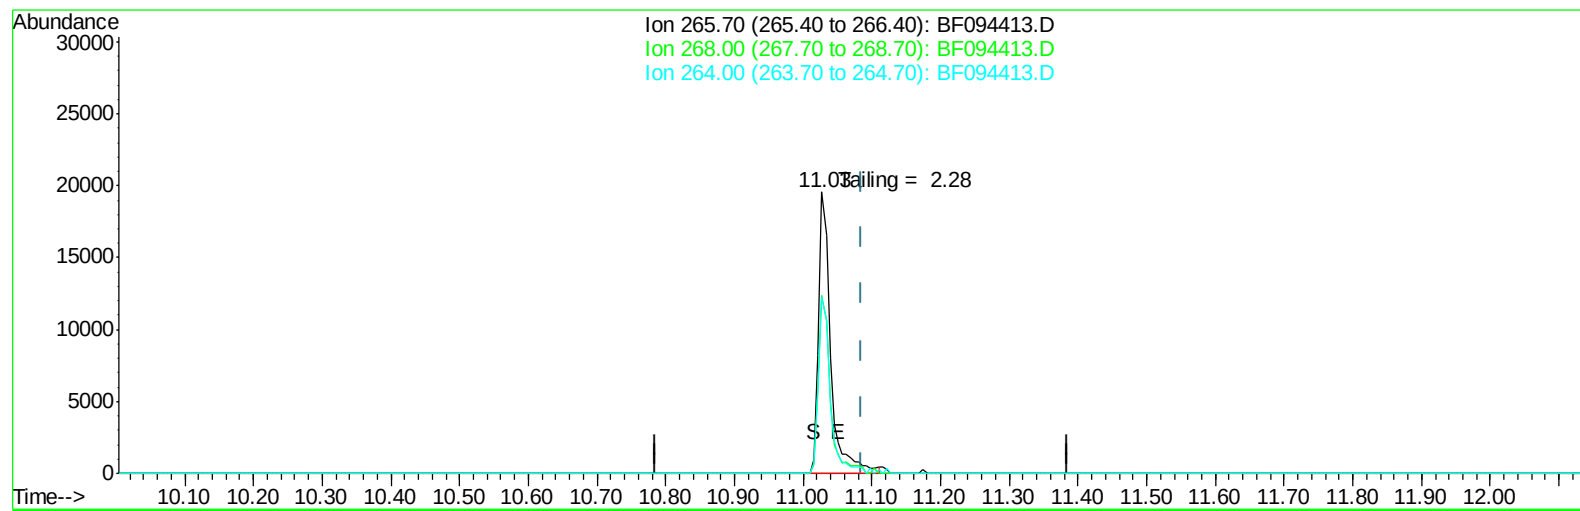

TIC: BF094413.D

(69) Pentachlorophenol (C)

11.028min (-0.059) 0.00ng m

response 23461

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.17
264.00	64.60	62.73
0.00	0.00	0.00