


Data Path : Z:\HPCHEM1\BNA F\Data\BF041317\
 Data File : BF094388.D
 Acq On : 13 Apr 2017 13:44
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 14 01:21:26 2017

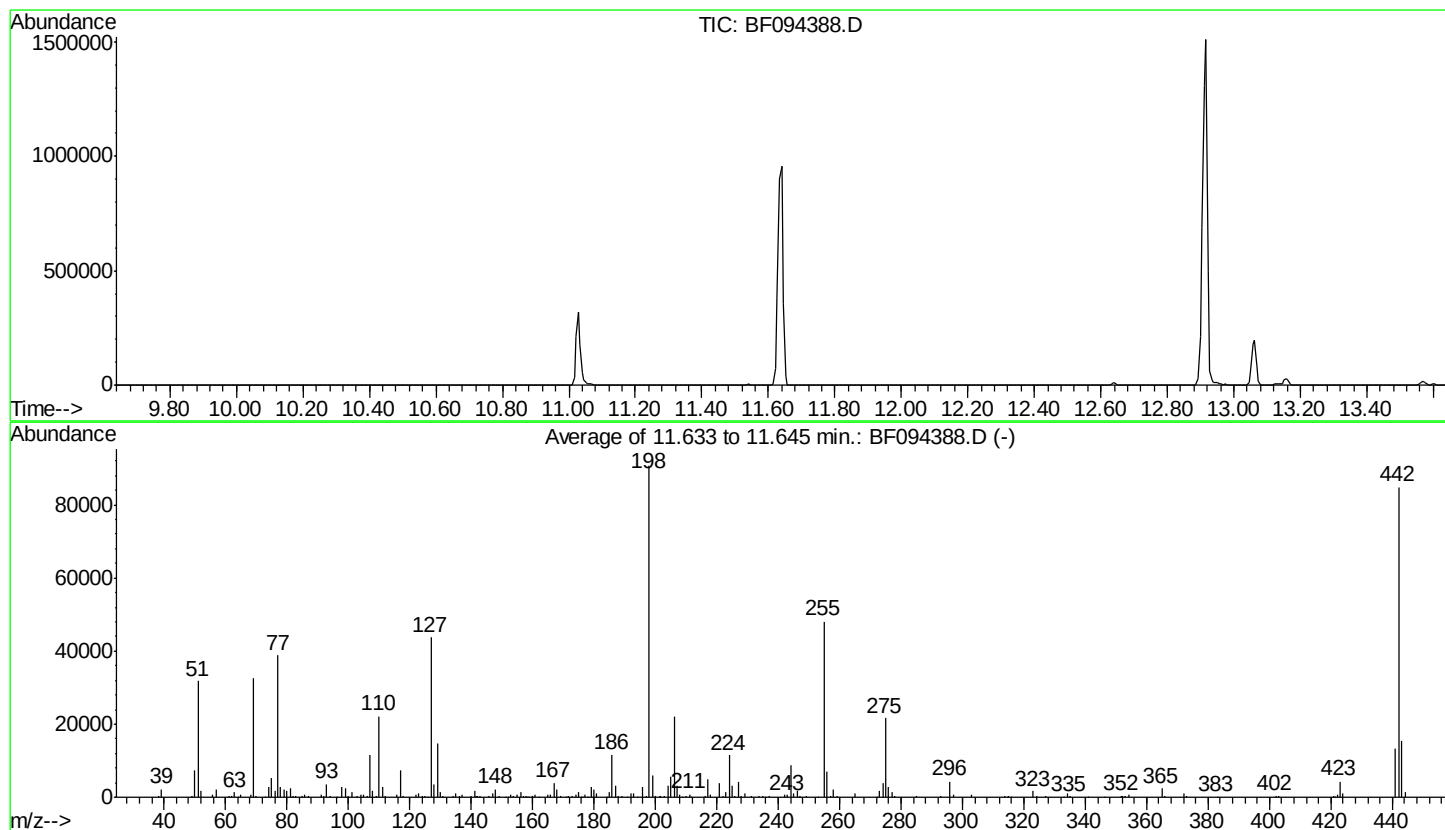

AutoFind: Scans 1657, 1658, 1659; Background Corrected with Scan 1650

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	31806	PASS
68	69	0.00	2	1.7	554	PASS
69	198	0.00	100	35.8	32457	PASS
70	69	0.00	2	0.6	204	PASS
127	198	10	80	48.2	43712	PASS
197	198	0.00	2	0.5	480	PASS
198	198	100	100	100.0	90722	PASS
199	198	5	9	6.6	5985	PASS
275	198	10	60	23.8	21609	PASS
365	198	1	100	2.6	2366	PASS
441	442	0.01	24	15.5	13173	PASS
442	198	50	100	93.5	84850	PASS
443	442	15	24	18.2	15465	PASS