


Data Path : Z:\HPCHEM1\BNA F\Data\BF041317\
 Data File : BF094413.D
 Acq On : 14 Apr 2017 2:35
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 14 01:21:26 2017

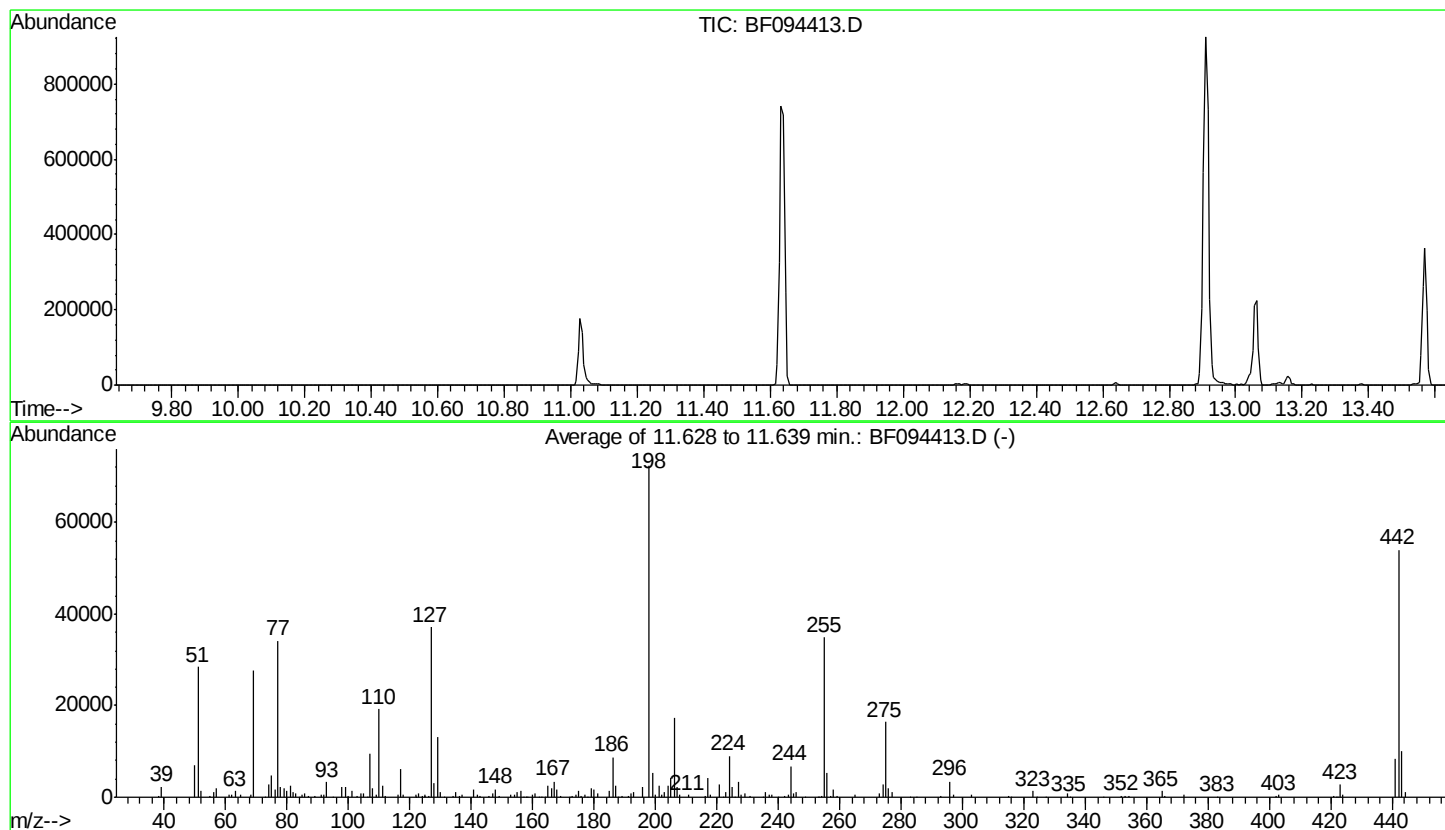

AutoFind: Scans 1656, 1657, 1658; Background Corrected with Scan 1651

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	28400	PASS
68	69	0.00	2	1.6	437	PASS
69	198	0.00	100	38.2	27642	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.3	37160	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	72384	PASS
199	198	5	9	7.2	5207	PASS
275	198	10	60	22.7	16456	PASS
365	198	1	100	1.9	1372	PASS
441	442	0.01	24	15.8	8522	PASS
442	198	50	100	74.5	53962	PASS
443	442	15	24	18.9	10184	PASS