

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041318\
 Data File : BF104518.D
 Acq On : 14 Apr 2018 11:06
 Operator : JU/SJ
 Sample : J2368-12
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Apr 16 00:42:36 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 13 17:38:31 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.81	152	149606	20.00	ng	0.00
21) Naphthalene-d8	8.09	136	596333	20.00	ng	0.00
38) Acenaphthene-d10	9.85	164	249369	20.00	ng	-0.01
63) Phenanthrene-d10	11.33	188	344057	20.00	ng	-0.01
75) Chrysene-d12	13.98	240	227461	20.00	ng	-0.01
86) Perylene-d12	15.44	264	179510	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.42	112	404466	41.34	ng	0.00
7) Phenol-d6	6.44	99	308083	25.63	ng	0.00
23) Nitrobenzene-d5	7.37	82	937662	102.67	ng	0.00
41) 2,4,6-Tribromophenol	10.64	330	198875	76.88	ng	0.00
44) 2-Fluorobiphenyl	9.17	172	1491042	94.46	ng	0.00
78) Terphenyl-d14	12.93	244	961832	96.40	ng	0.00
Target Compounds						
9) Benzaldehyde	6.44	77	579	Below Cal	#	1
19) n-Nitroso-di-n-propylamine	7.37	70	124481	15.846 ng	#	73
25) Isophorone	7.37	82	937655	48.553 ng	#	64
49) Dimethylphthalate	9.56	163	125829	6.399 ng		99
56) 2,4-Dinitrotoluene	9.85	165	30564	6.404 ng	#	23
64) 4,6-Dinitro-2-methylphenol	10.63	198	290	7.494 ng	#	1
66) 4-Bromophenyl-phenylether	10.64	248	11948	3.265 ng	#	1
76) Benzydine	12.93	184	12413	Below Cal	#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041318\
Data File : BF104518.D
Acq On : 14 Apr 2018 11:06
Operator : JU/SJ
Sample : J2368-12
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Apr 16 00:42:36 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 13 17:38:31 2018
Response via : Initial Calibration

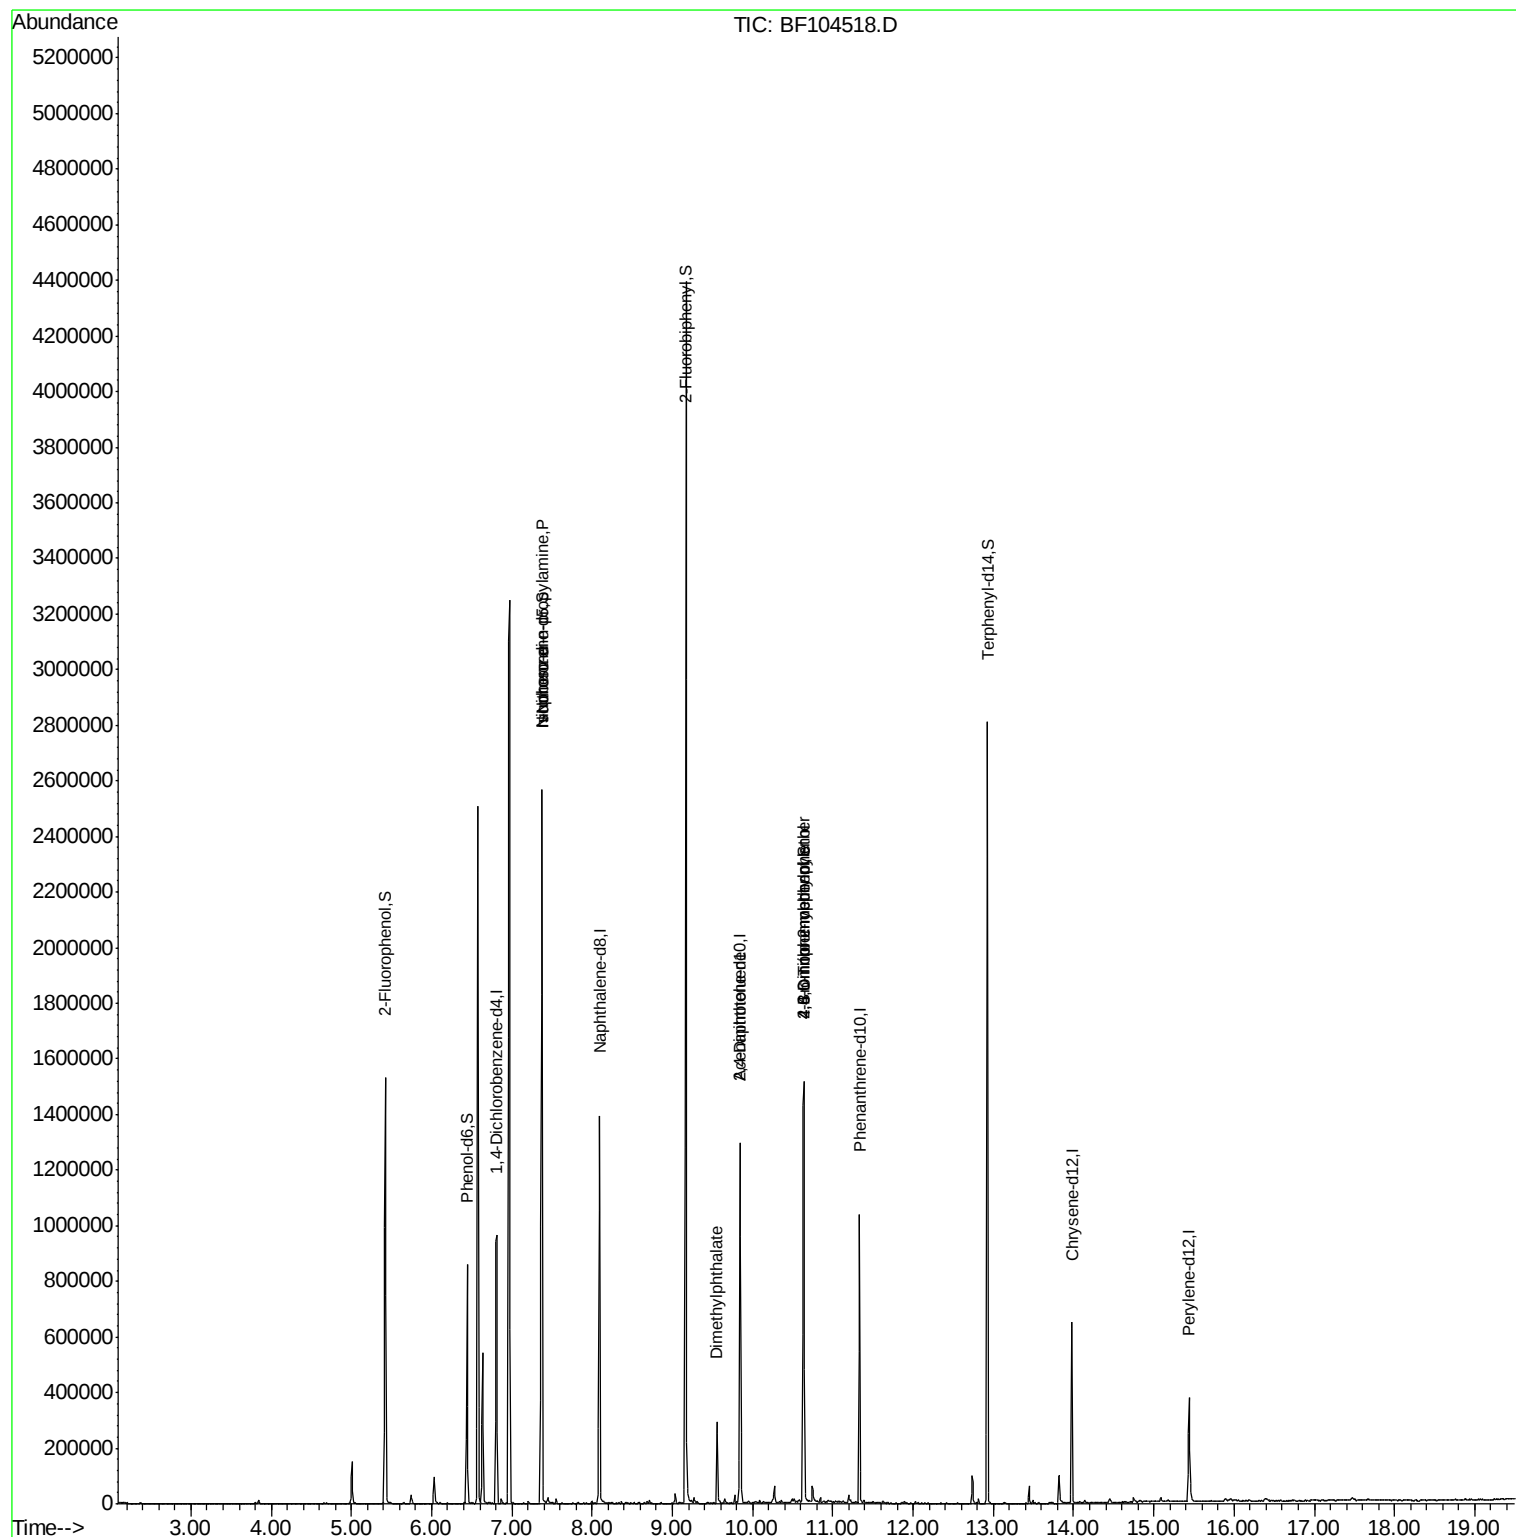

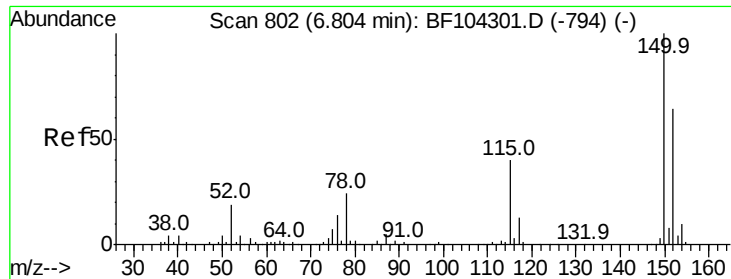


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.81 min Scan# 803
Delta R.T. -0.00 min
Lab File: BF104518.D
Acq: 14 Apr 2018 11:06

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 149606
Ion Ratio Lower Upper
152 100
150 154.6 124.6 186.8
115 60.1 50.1 75.1

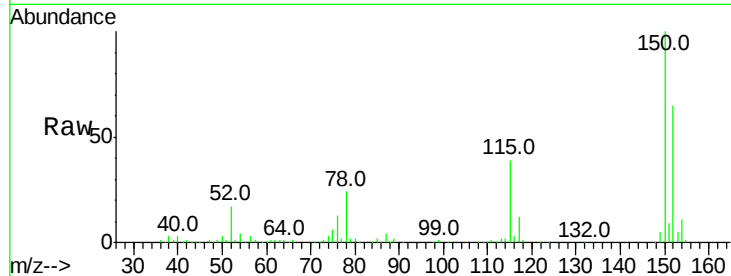


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

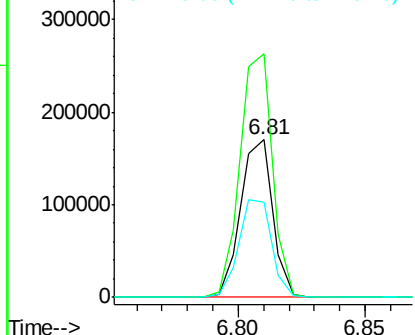



#5

2-Fluorophenol
Concen: 41.339 ng
RT: 5.42 min Scan# 567
Delta R.T. -0.00 min
Lab File: BF104518.D
Acq: 14 Apr 2018 11:06

Tgt Ion:112 Resp: 404466
Ion Ratio Lower Upper
112 100
64 55.1 47.9 71.9
63 27.9 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

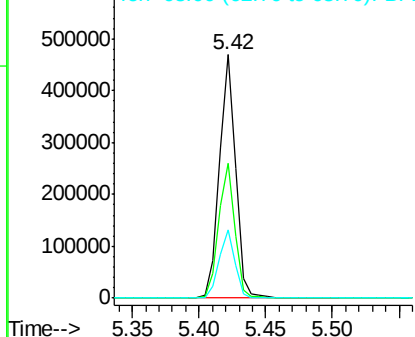



#7

Phenol-d6

Concen: 25.627 ng

RT: 6.44 min Scan# 740

Delta R.T. -0.01 min

Lab File: BF104518.D

Acq: 14 Apr 2018 11:06

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 99 Resp: 308083

Ion Ratio Lower Upper

99 100

42 14.5 14.5 21.7

71 30.6 25.4 38.0

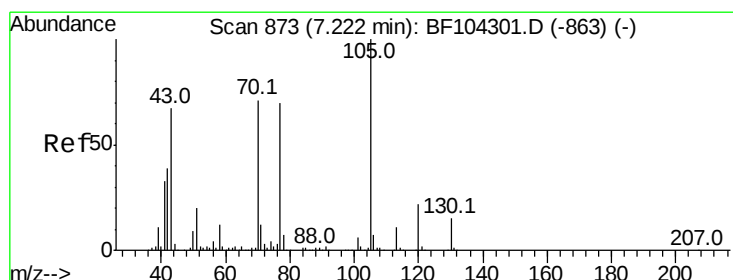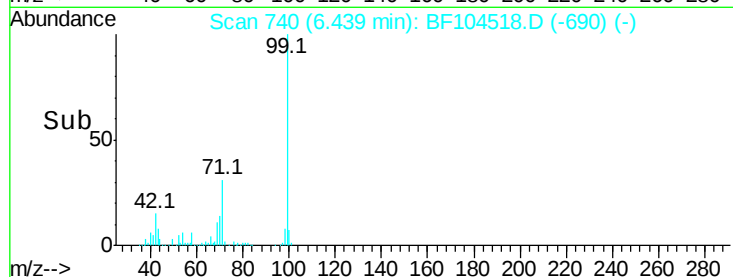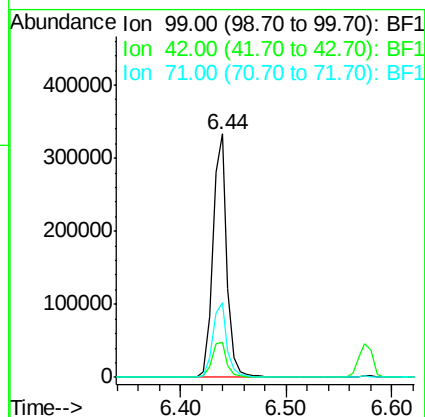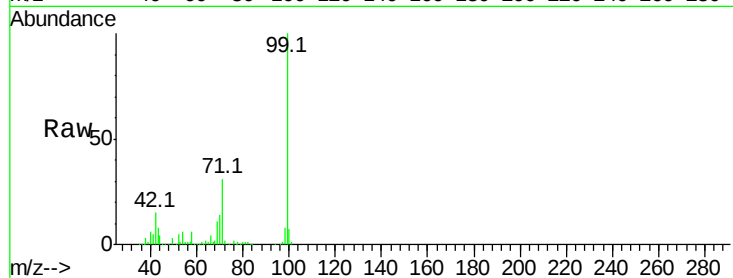

#19

n-Nitroso-di-n-propylamine

Concen: 15.846 ng

RT: 7.37 min Scan# 899

Delta R.T. 0.15 min

Lab File: BF104518.D

Acq: 14 Apr 2018 11:06

Tgt Ion: 70 Resp: 124481




Ion Ratio Lower Upper


70 100

42 42.7 47.5 71.3#

101 0.0 7.4 11.2#

130 2.1 16.6 25.0#


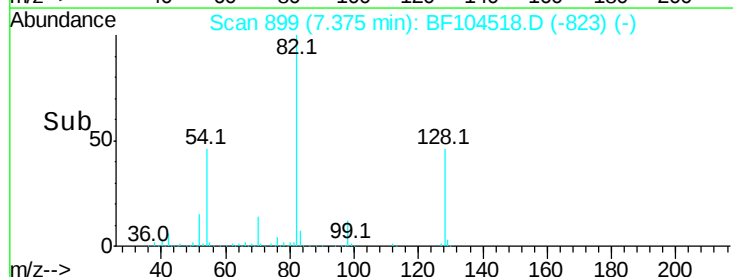
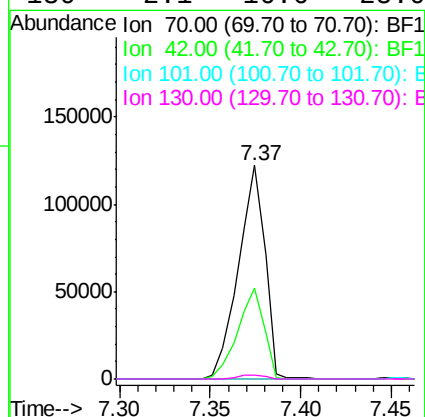
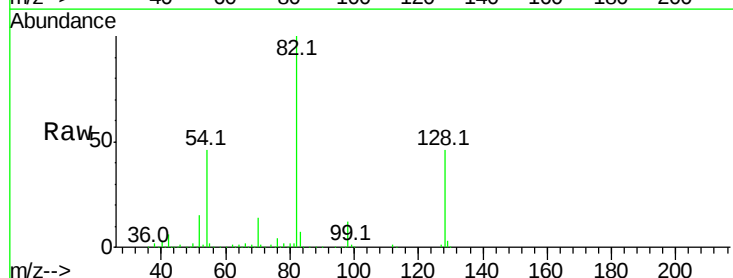


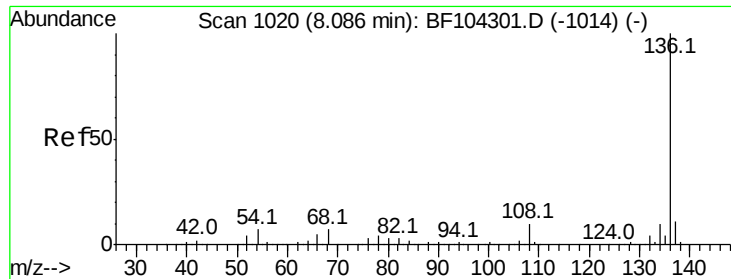

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.09 min Scan# 1021
Delta R.T. -0.01 min
Lab File: BF104518.D
Acq: 14 Apr 2018 11:06




Instrument :
BNA_F
ClientSampleId :


Tot Ion:	136	Resp:	596333
Ion	Ratio	Lower	Upper
136	100		
137	10.8	8.9	13.3
54	6.8	6.6	9.8
68	5.9	5.0	7.4

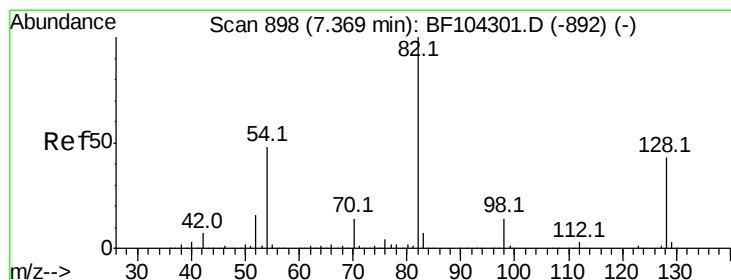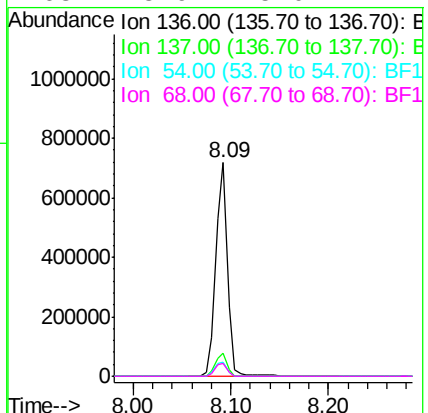

#23
Nitrobenzene-d5
Concen: 102.673 ng
RT: 7.37 min Scan# 899
Delta R.T. -0.01 min
Lab File: BF104518.D
Acq: 14 Apr 2018 11:06

Tgt Ion:	82	Resp:	937662
Ion	Ratio	Lower	Upper
82	100		
128	46.2	36.1	54.1
54	46.1	41.4	62.2

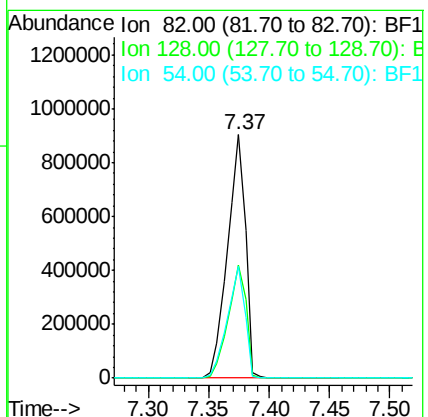

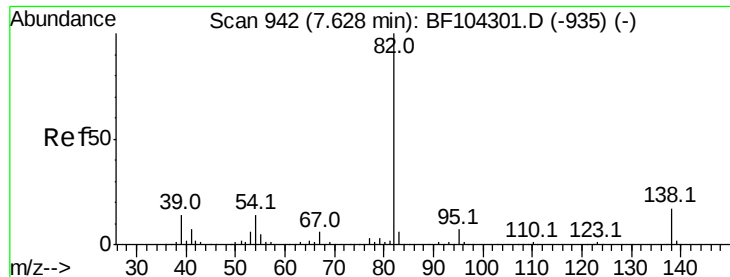

#25

Isophorone

Concen: 48.553 ng

RT: 7.37 min Scan# 899

Delta R.T. -0.26 min

Lab File: BF104518.D

Acq: 14 Apr 2018 11:06

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 937655

Ion Ratio Lower Upper

82 100

95 0.0 5.2 7.8#




138 0.0 14.9 22.3#

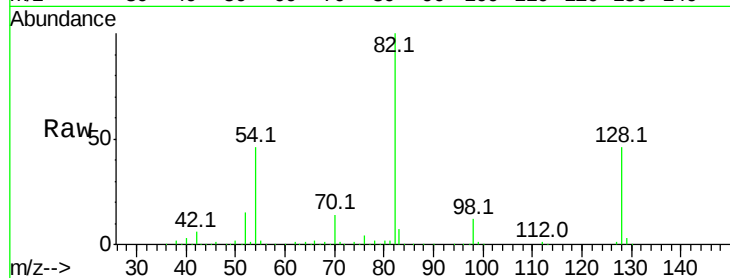

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

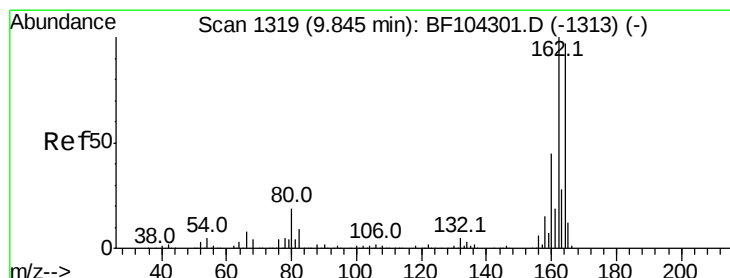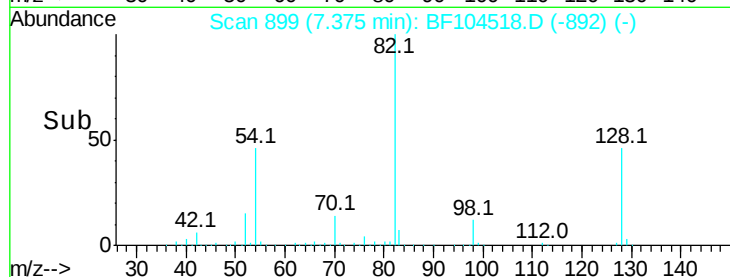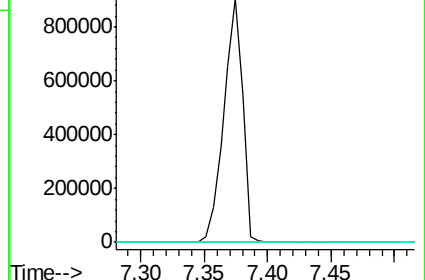

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.85 min Scan# 1319

Delta R.T. -0.01 min

Lab File: BF104518.D

Acq: 14 Apr 2018 11:06


Tgt Ion:164 Resp: 249369

Ion Ratio Lower Upper

164 100

162 103.9 86.1 129.1



160 46.5 38.3 57.5

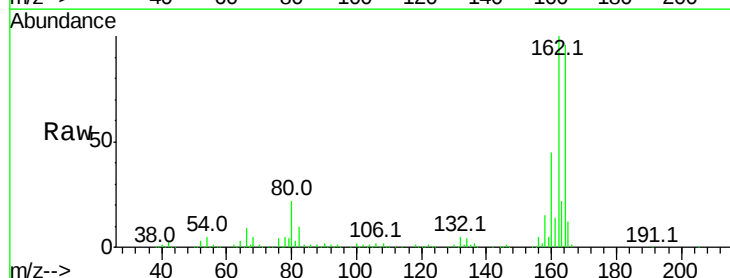


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

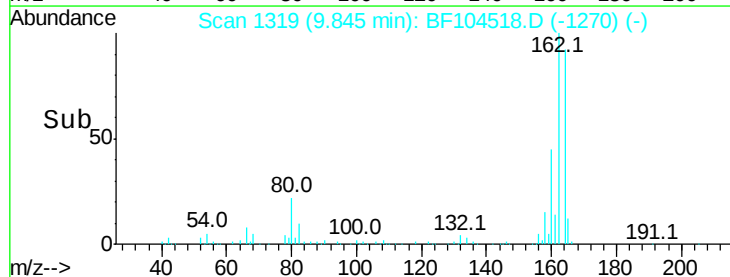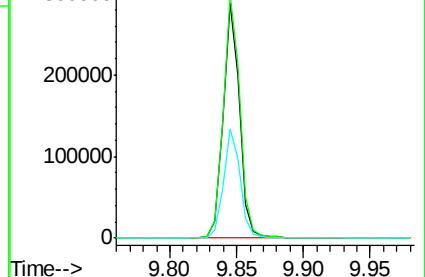







#41
 2,4,6-Tribromophenol
 Concen: 76.882 ng
 RT: 10.64 min Scan# 1454
 Delta R.T. -0.01 min
 Lab File: BF104518.D
 Acq: 14 Apr 2018 11:06

Instrument :
 BNA_F
 ClientSampled :

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.5	77.0	115.6
141	34.2	29.9	44.9

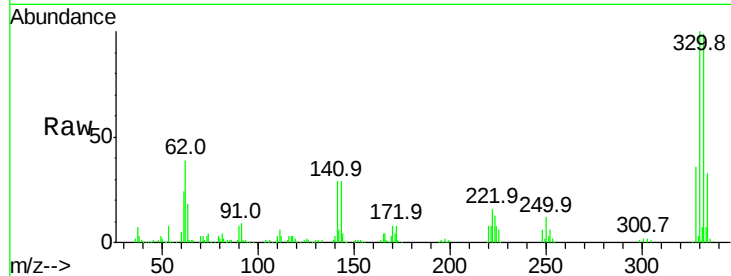


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

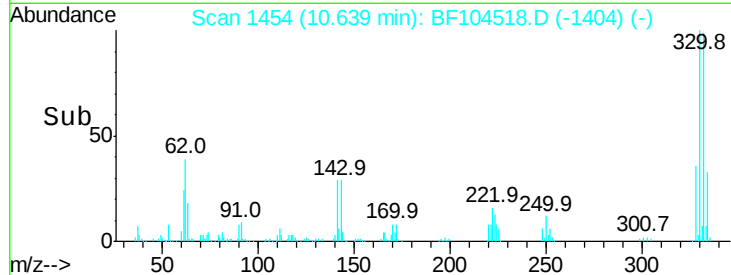
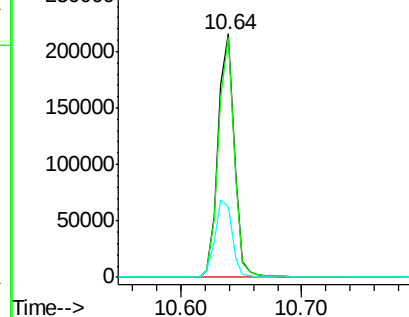



#44
 2-Fluorobiphenyl
 Concen: 94.457 ng
 RT: 9.17 min Scan# 1204
 Delta R.T. -0.01 min
 Lab File: BF104518.D
 Acq: 14 Apr 2018 11:06

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.5	29.7	44.5
170	24.1	19.6	29.4

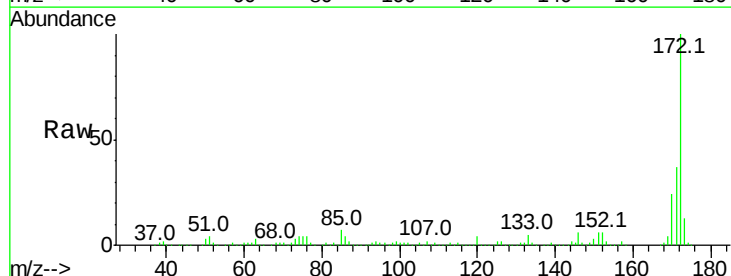

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

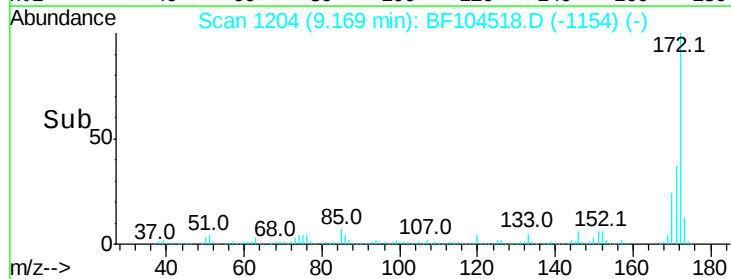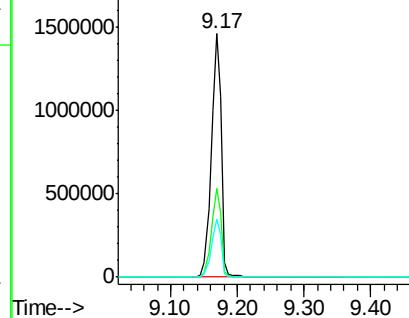



#49

Dimethylphthalate

Concen: 6.399 ng

RT: 9.56 min Scan# 1270

Delta R.T. -0.02 min

Lab File: BF104518.D

Acq: 14 Apr 2018 11:06

Instrument :

BNA_F

ClientSampleId :


Tot Ion:163 Resp: 125829

Ion Ratio Lower Upper

163 100

194 3.3 2.7 4.1




164 9.9 8.2 12.2



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

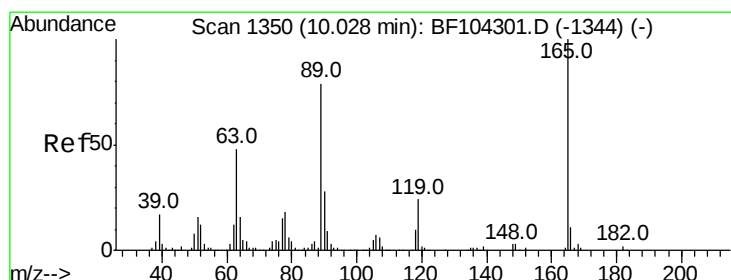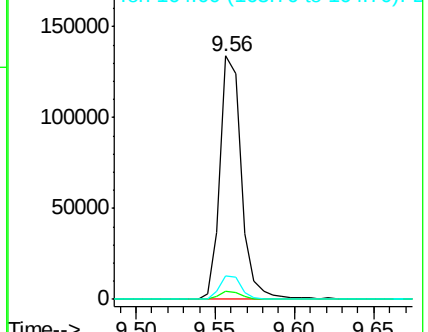

#56

2,4-Dinitrotoluene

Concen: 6.404 ng

RT: 9.85 min Scan# 1319

Delta R.T. -0.20 min

Lab File: BF104518.D

Acq: 14 Apr 2018 11:06

Tgt Ion:165 Resp: 30564


Ion Ratio Lower Upper

165 100

63 1.1 36.4 54.6#

89 1.2 57.8 86.6#

182 0.0 1.6 2.4#






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E




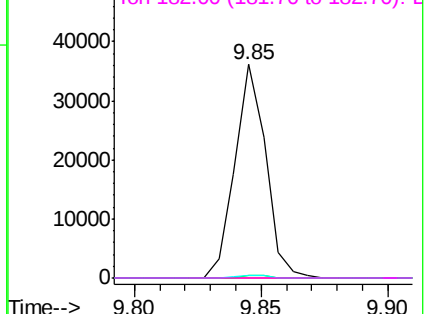


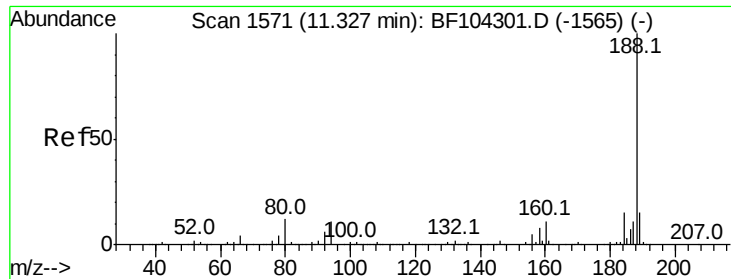

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.33 min Scan# 1572
Delta R.T. -0.01 min
Lab File: BF104518.D
Acq: 14 Apr 2018 11:06




Instrument :
BNA_F
ClientSampled :


Tot Ion:188 Resp: 344057
Ion Ratio Lower Upper
188 100
94 11.6 8.5 12.7
80 11.7 9.2 13.8

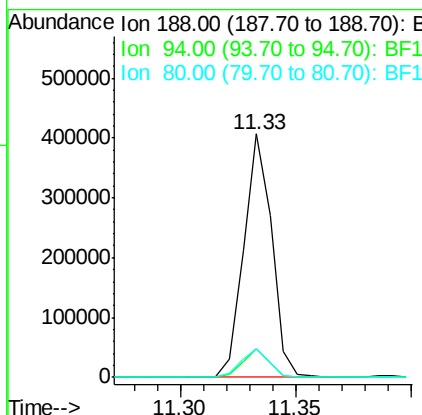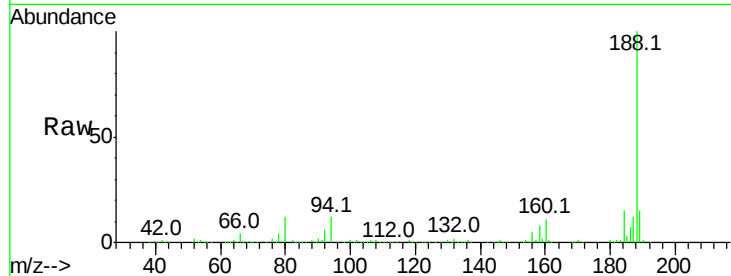

#64
4,6-Dinitro-2-methylphenol
Concen: 7.494 ng
RT: 10.63 min Scan# 1453
Delta R.T. 0.18 min
Lab File: BF104518.D
Acq: 14 Apr 2018 11:06

Tgt Ion:198 Resp: 290
Ion Ratio Lower Upper
198 100
51 159.1 37.7 77.7#
105 242.7 36.3 76.3#

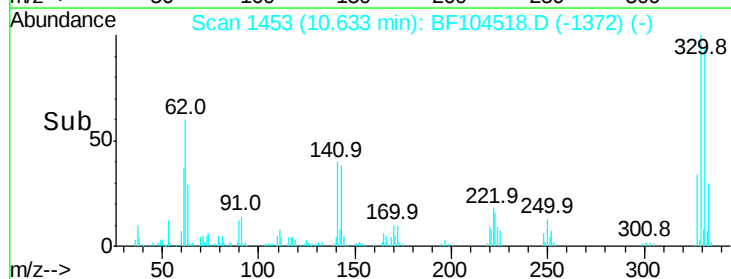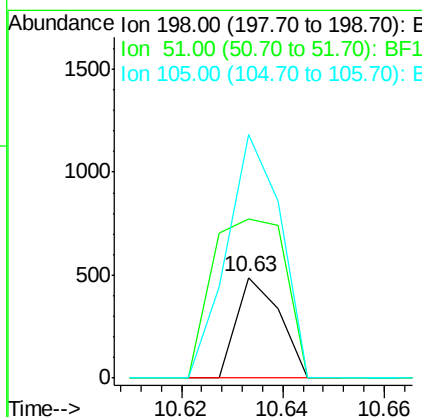


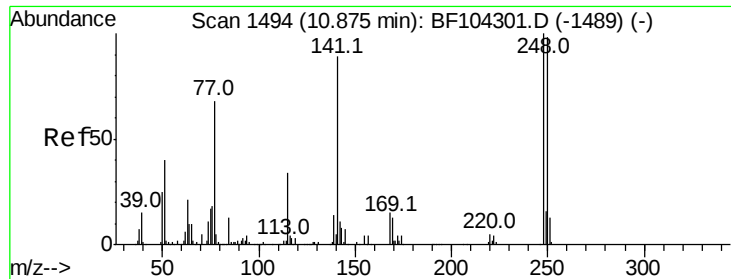




#66
 4-Bromophenyl-phenylether
 Concen: 3.265 ng
 RT: 10.64 min Scan# 1454
 Delta R.T. -0.25 min
 Lab File: BF104518.D
 Acq: 14 Apr 2018 11:06

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:248 Resp: 11948
 Ion Ratio Lower Upper
 248 100
 250 193.9 76.9 115.3#
 141 481.2 74.4 111.6#

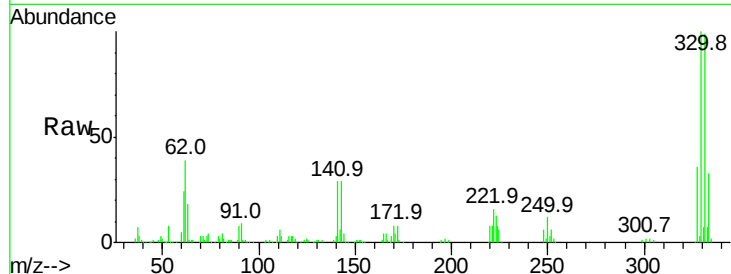


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

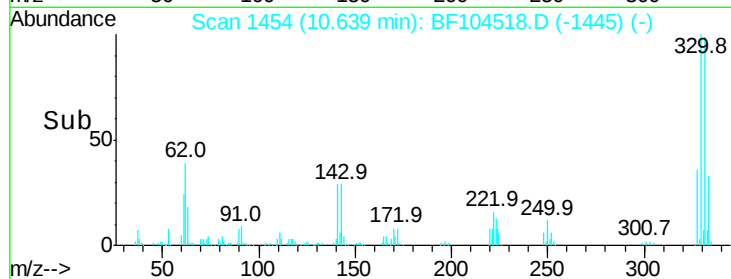
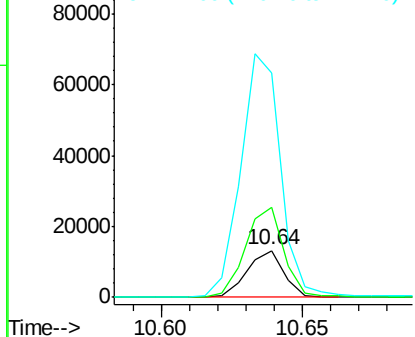



#75
 Chrysene-d12
 Concen: 20.000 ng
 RT: 13.98 min Scan# 2022
 Delta R.T. -0.01 min
 Lab File: BF104518.D
 Acq: 14 Apr 2018 11:06

Tgt Ion:240 Resp: 227461
 Ion Ratio Lower Upper
 240 100
 120 11.4 9.5 14.3
 236 26.8 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E




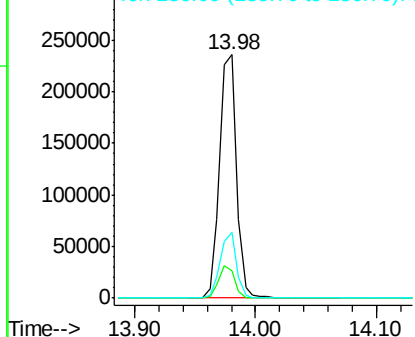


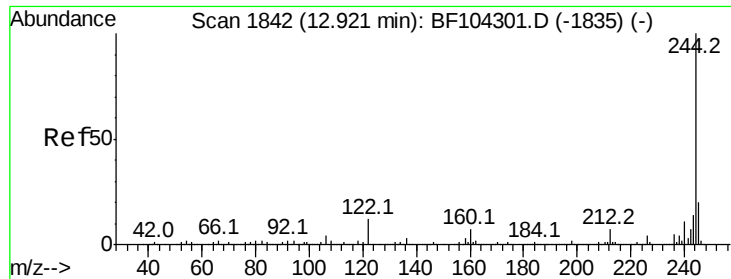

#78
 Terphenyl-d14
 Concen: 96.404 ng
 RT: 12.93 min Scan# 1843
 Delta R.T. -0.01 min
 Lab File: BF104518.D
 Acq: 14 Apr 2018 11:06

Instrument :
 BNA_F
 ClientSampleID :

Tot Ion:244 Resp: 961832
 Ion Ratio Lower Upper
 244 100
 212 6.9 5.4 8.0
 122 11.6 11.0 16.4

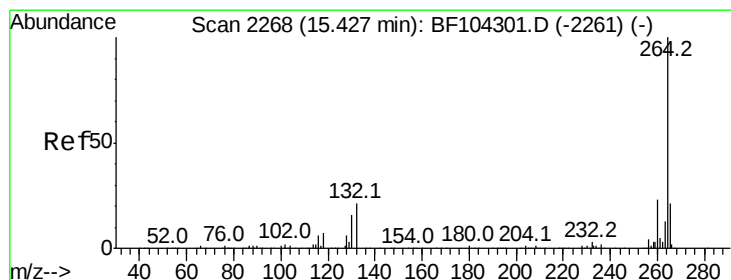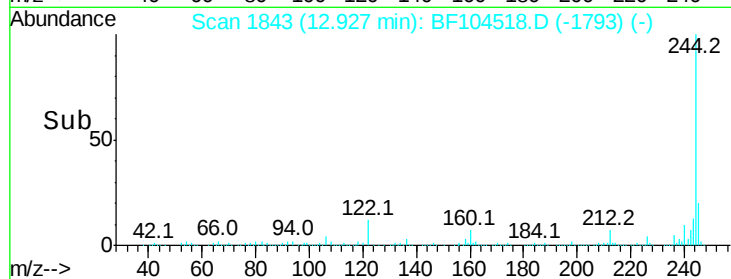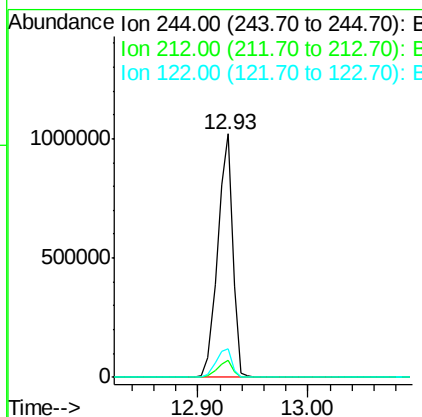

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.44 min Scan# 2270
 Delta R.T. -0.02 min
 Lab File: BF104518.D
 Acq: 14 Apr 2018 11:06

Tgt Ion:264 Resp: 179510
 Ion Ratio Lower Upper
 264 100
 260 25.1 19.2 28.8
 265 21.2 17.5 26.3

