
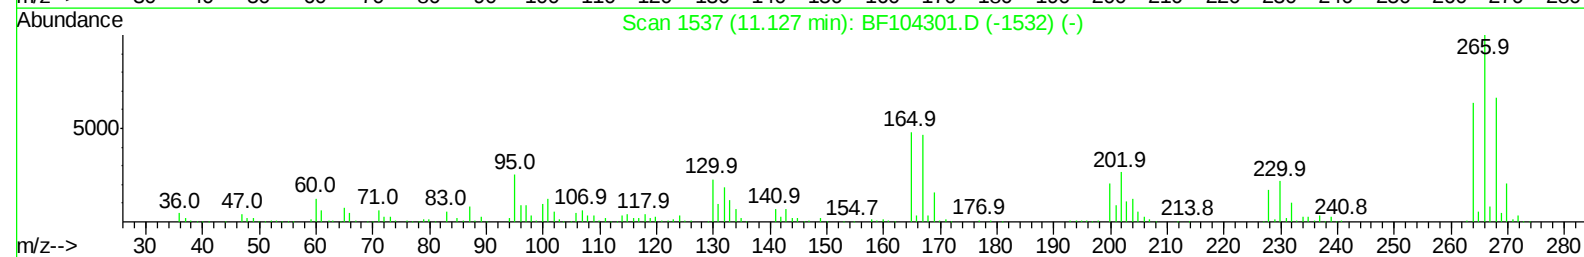
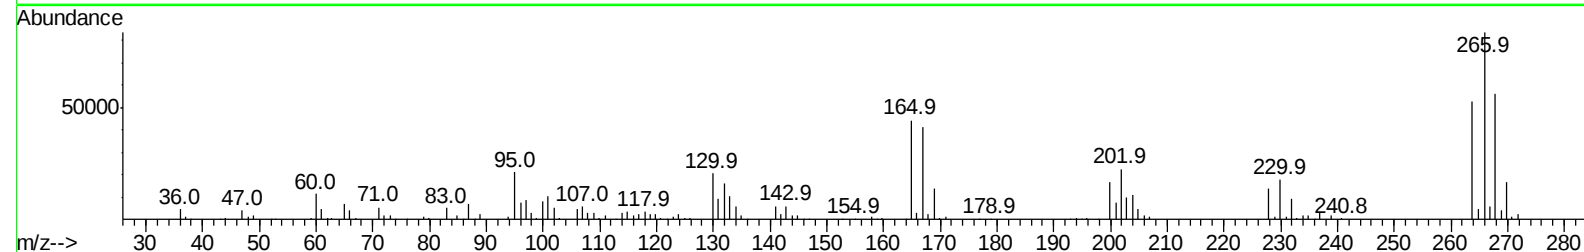


Data Path : Z:\HPCHEM1\BNA F\DATA\BF041318\
Data File : BF104472.D
Acq On : 13 Apr 2018 12:21
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 01:36:50 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 13 17:38:31 2018
Response via : Initial Calibration

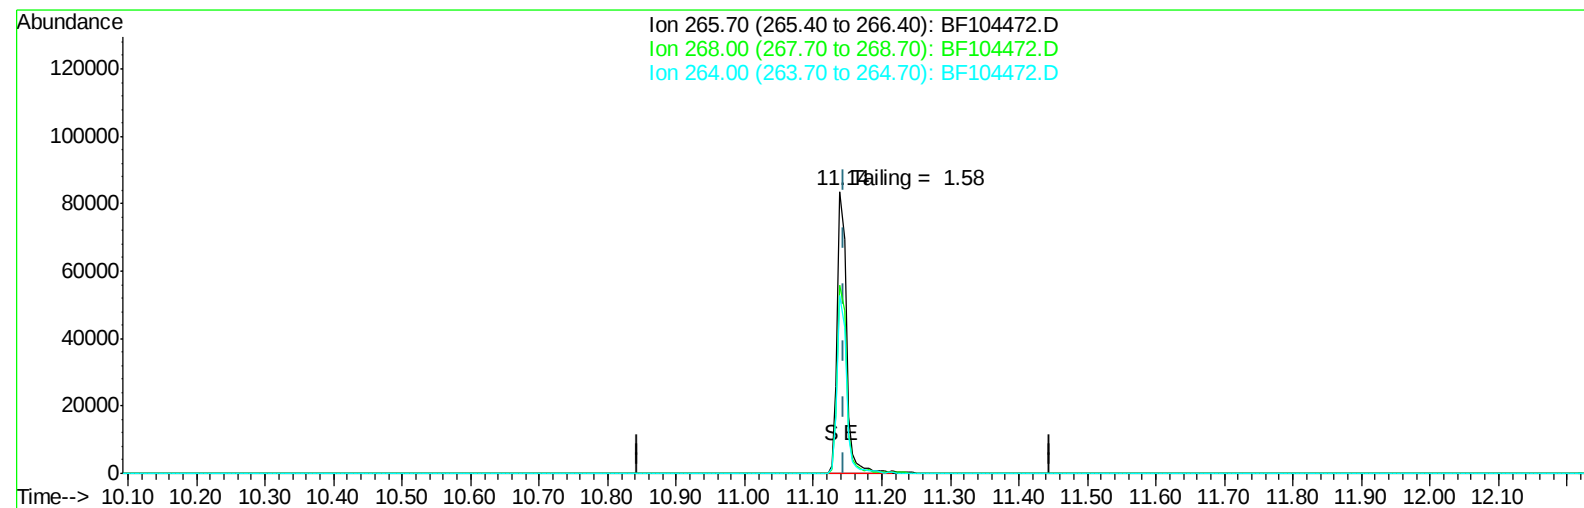

TIC: BF104472.D

(69) Pentachlorophenol (C)




11.139min (-0.006) 35816.22ng

response 76377

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	67.04
264.00	61.90	63.36
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041318\
Data File : BF104472.D
Acq On : 13 Apr 2018 12:21
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 01:36:50 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 13 17:38:31 2018
Response via : Initial Calibration

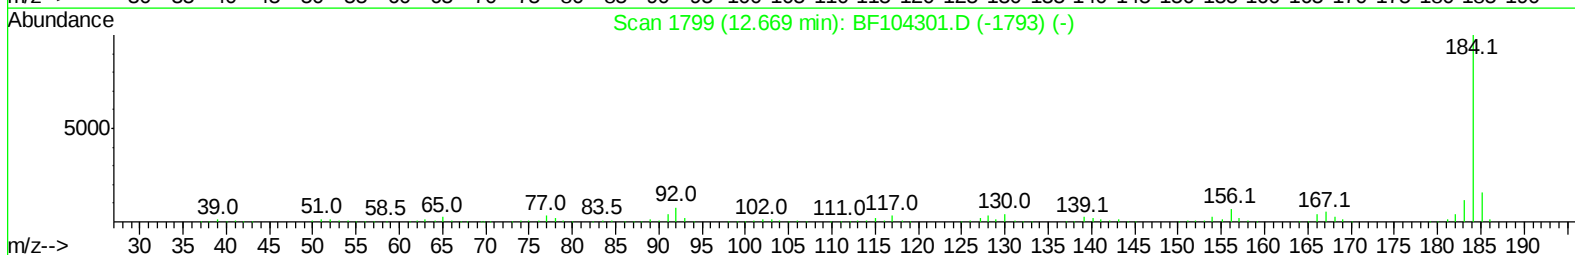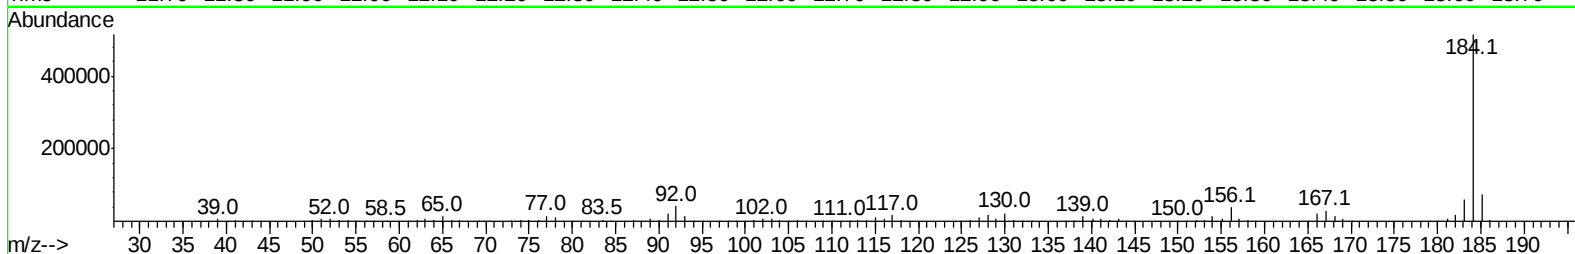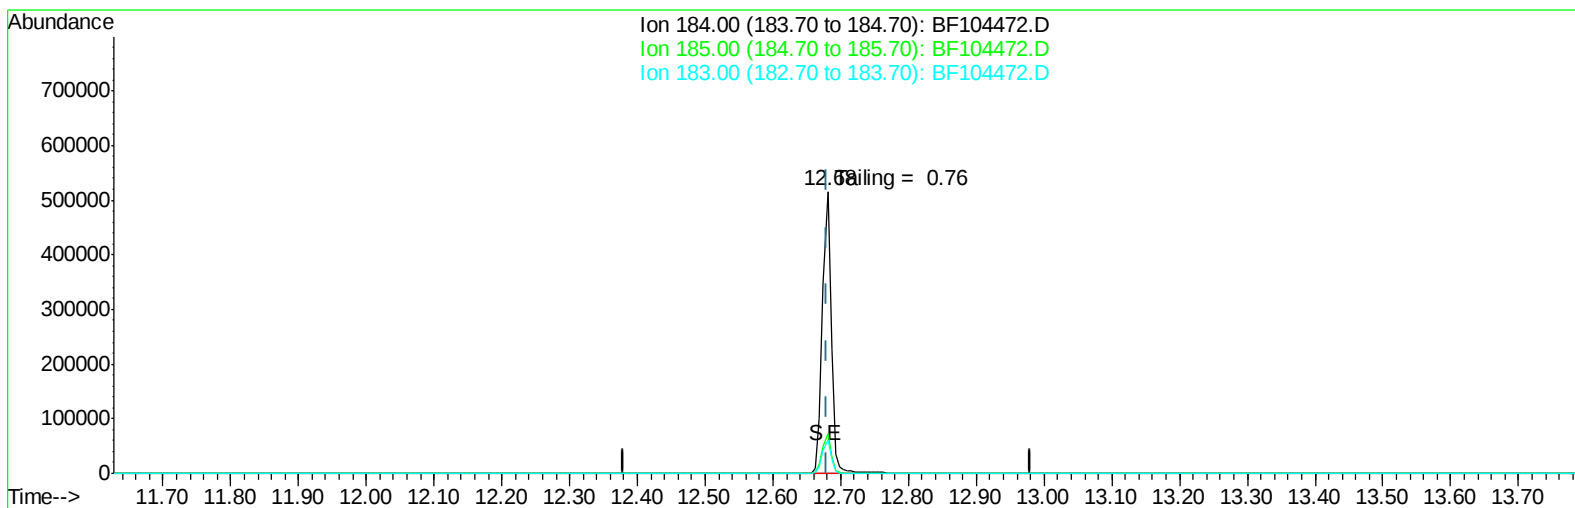

TIC: BF104472.D

(76) Benzidine

12.680min (+0.000) 0.00ng

response 452863

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.16
183.00	11.60	11.90
0.00	0.00	0.00