
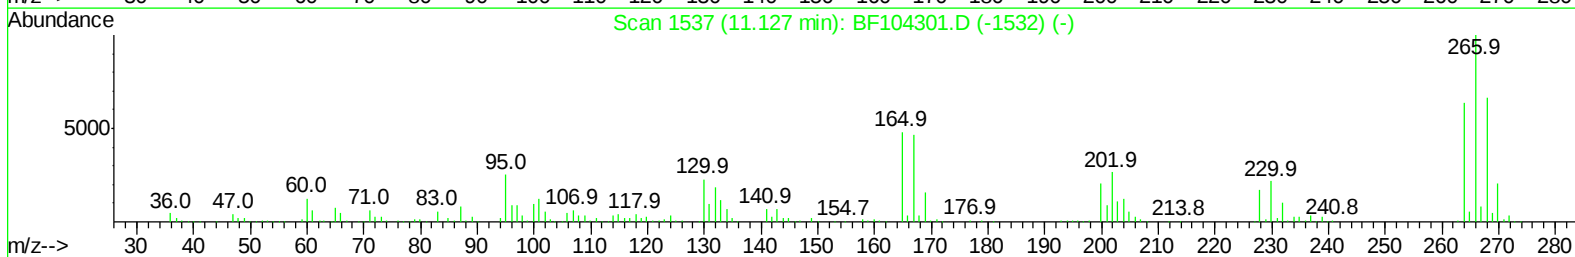
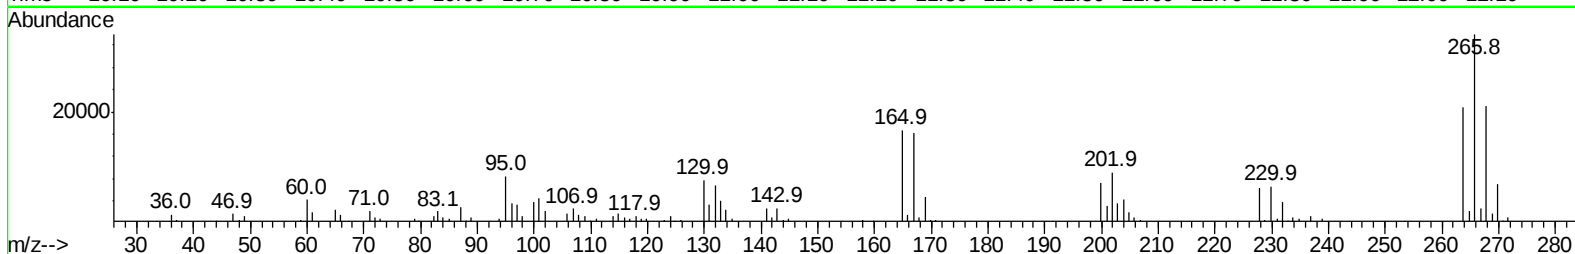


Data Path : Z:\HPCHEM1\BNA F\DATA\BF041318\
Data File : BF104499.D
Acq On : 14 Apr 2018 1:22
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 01:50:22 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 13 17:38:31 2018
Response via : Initial Calibration

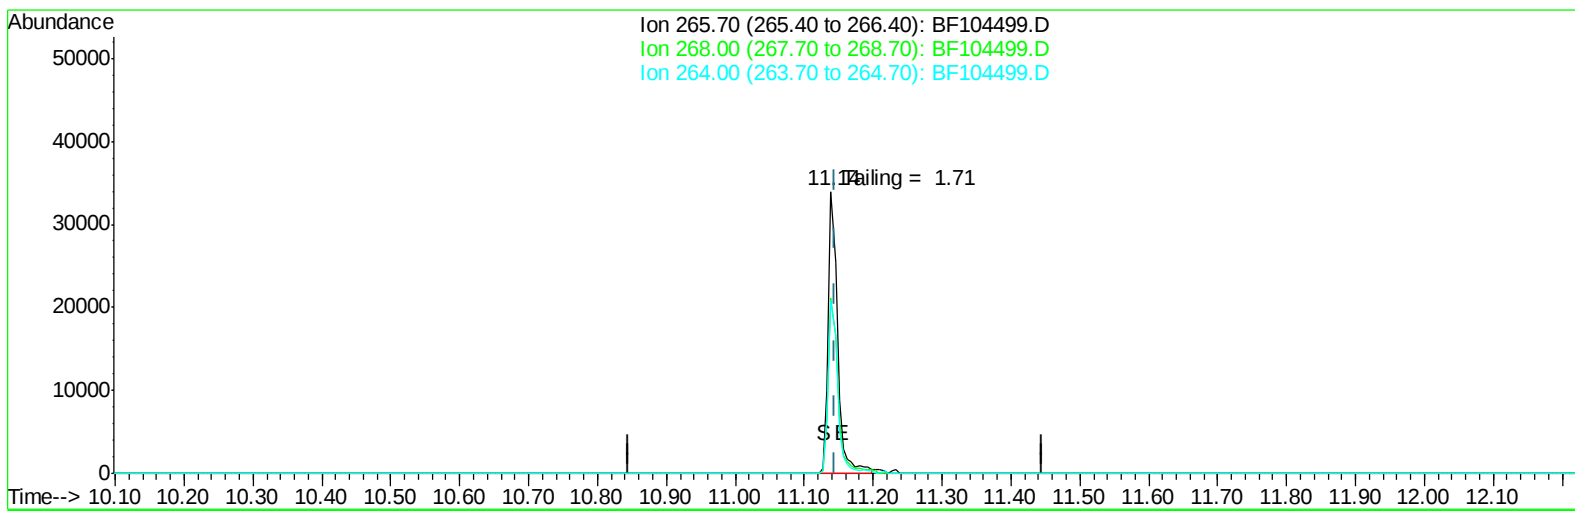

TIC: BF104499.D

(69) Pentachlorophenol (C)




11.139min (-0.006) 34227.18ng

response 31679

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.13
264.00	61.90	61.38
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041318\
 Data File : BF104499.D
 Acq On : 14 Apr 2018 1:22
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 01:50:22 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 13 17:38:31 2018
 Response via : Initial Calibration

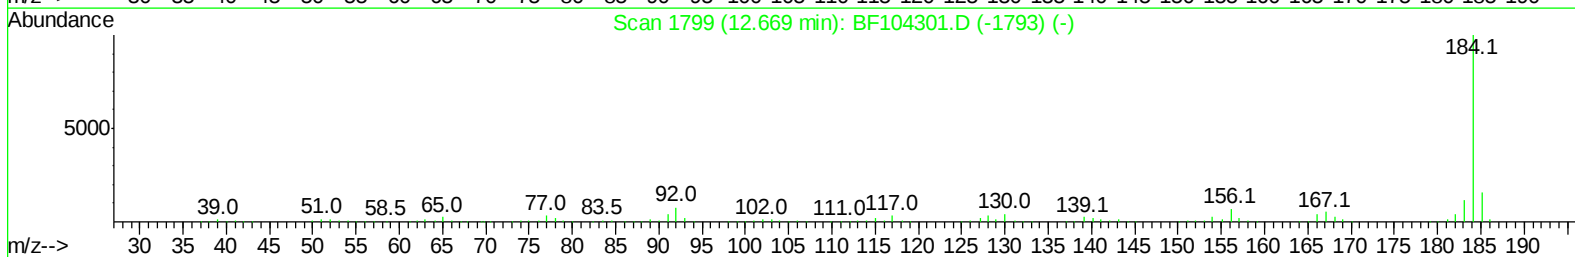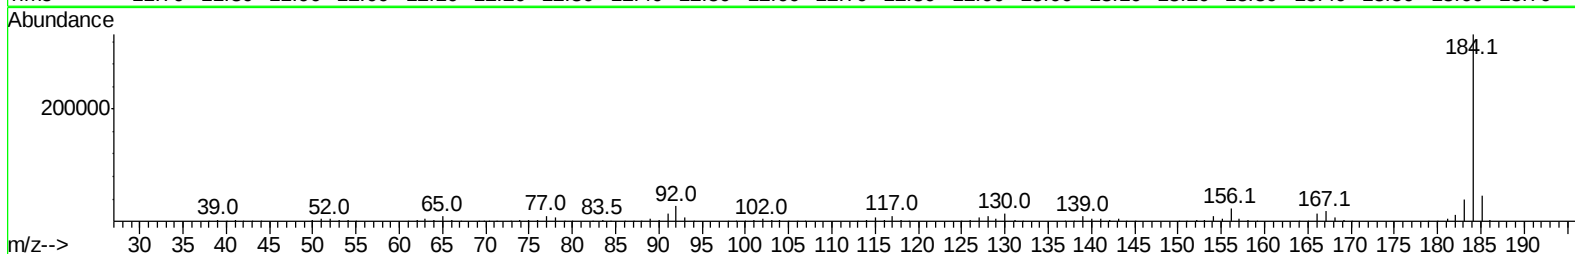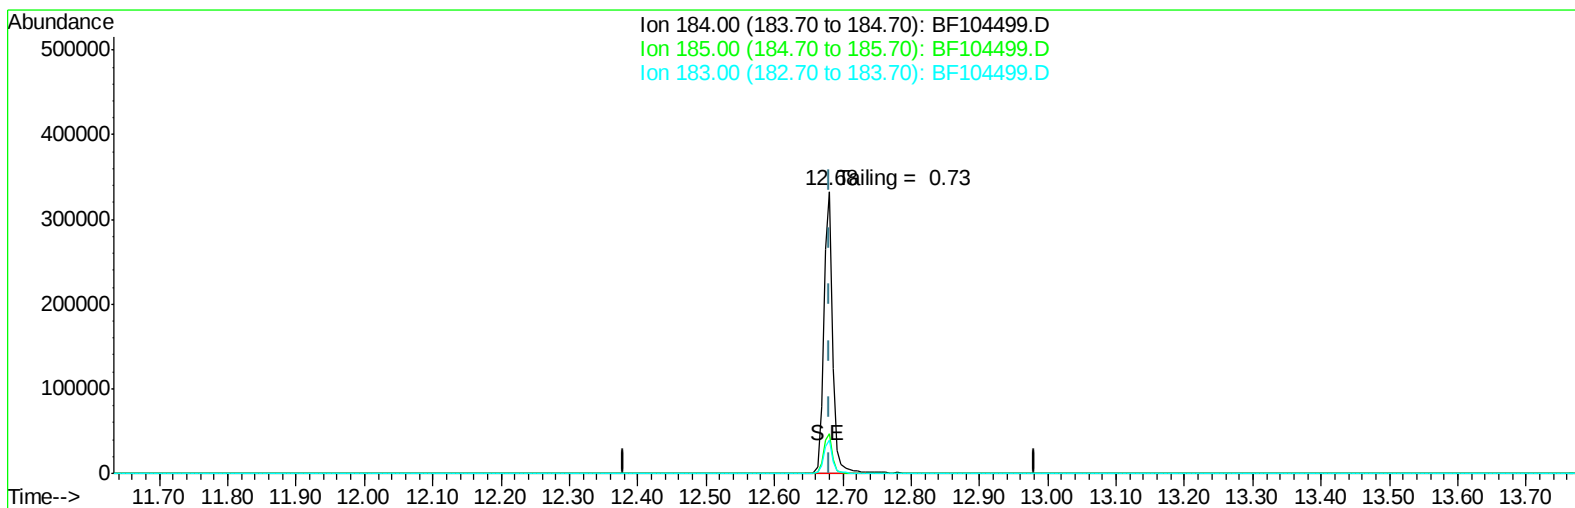

TIC: BF104499.D

(76) Benzidine

12.680min (-0.000) 0.00ng

response 309444

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.93
183.00	11.60	11.69
0.00	0.00	0.00