

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041318\
 Data File : BF104487.D
 Acq On : 13 Apr 2018 19:08
 Operator : JU/SJ
 Sample : J2166-03 2X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TR-04-041218

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.010	493	497	507	rVB	65136	71445	4.20%	0.435%
2	5.416	562	566	569	rBV	1669605	1502768	88.43%	9.153%
3	6.045	669	673	680	rBV	33298	40051	2.36%	0.244%
4	6.440	735	740	750	rBV	1511936	1544213	90.87%	9.405%
5	6.575	759	763	766	rBV	1874586	1591549	93.65%	9.693%
6	6.810	799	803	806	rBV	1002406	794417	46.75%	4.838%
7	6.963	825	829	833	rBV	1511962	1255234	73.86%	7.645%
8	7.369	894	898	901	rBV	1017108	933923	54.95%	5.688%
9	8.092	1017	1021	1024	rBV	1344498	1026615	60.41%	6.253%
10	9.169	1200	1204	1207	rBV	2013367	1699439	100.00%	10.351%
11	9.563	1267	1271	1279	rVB	155939	148831	8.76%	0.906%
12	9.775	1304	1307	1310	rVB	64185	44436	2.61%	0.271%
13	9.851	1316	1320	1329	rVB	1164432	1061686	62.47%	6.466%
14	10.275	1389	1392	1395	rVB	75866	55293	3.25%	0.337%
15	10.498	1425	1430	1432	rBV	18389	23571	1.39%	0.144%
16	10.639	1450	1454	1463	rVB	921011	873904	51.42%	5.323%
17	10.751	1470	1473	1482	rBV	55477	62282	3.66%	0.379%
18	11.198	1546	1549	1552	rBV	25794	23142	1.36%	0.141%
19	11.339	1569	1573	1576	rBV	1026216	909900	53.54%	5.542%
20	12.551	1776	1779	1782	rBV	61822	45988	2.71%	0.280%
21	12.780	1815	1818	1824	rVB	56538	50348	2.96%	0.307%
22	12.927	1839	1843	1846	rBV	1307972	1249105	73.50%	7.608%
23	13.821	1992	1995	1997	rBV2	54322	57936	3.41%	0.353%
24	13.980	2018	2022	2026	rBV	778367	768107	45.20%	4.678%
25	15.451	2268	2272	2280	rVB	451014	584572	34.40%	3.560%


Sum of corrected areas: 16418755

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041318\
Data File : BF104487.D
Acq On : 13 Apr 2018 19:08
Operator : JU/SJ
Sample : J2166-03 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TR-04-041218

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

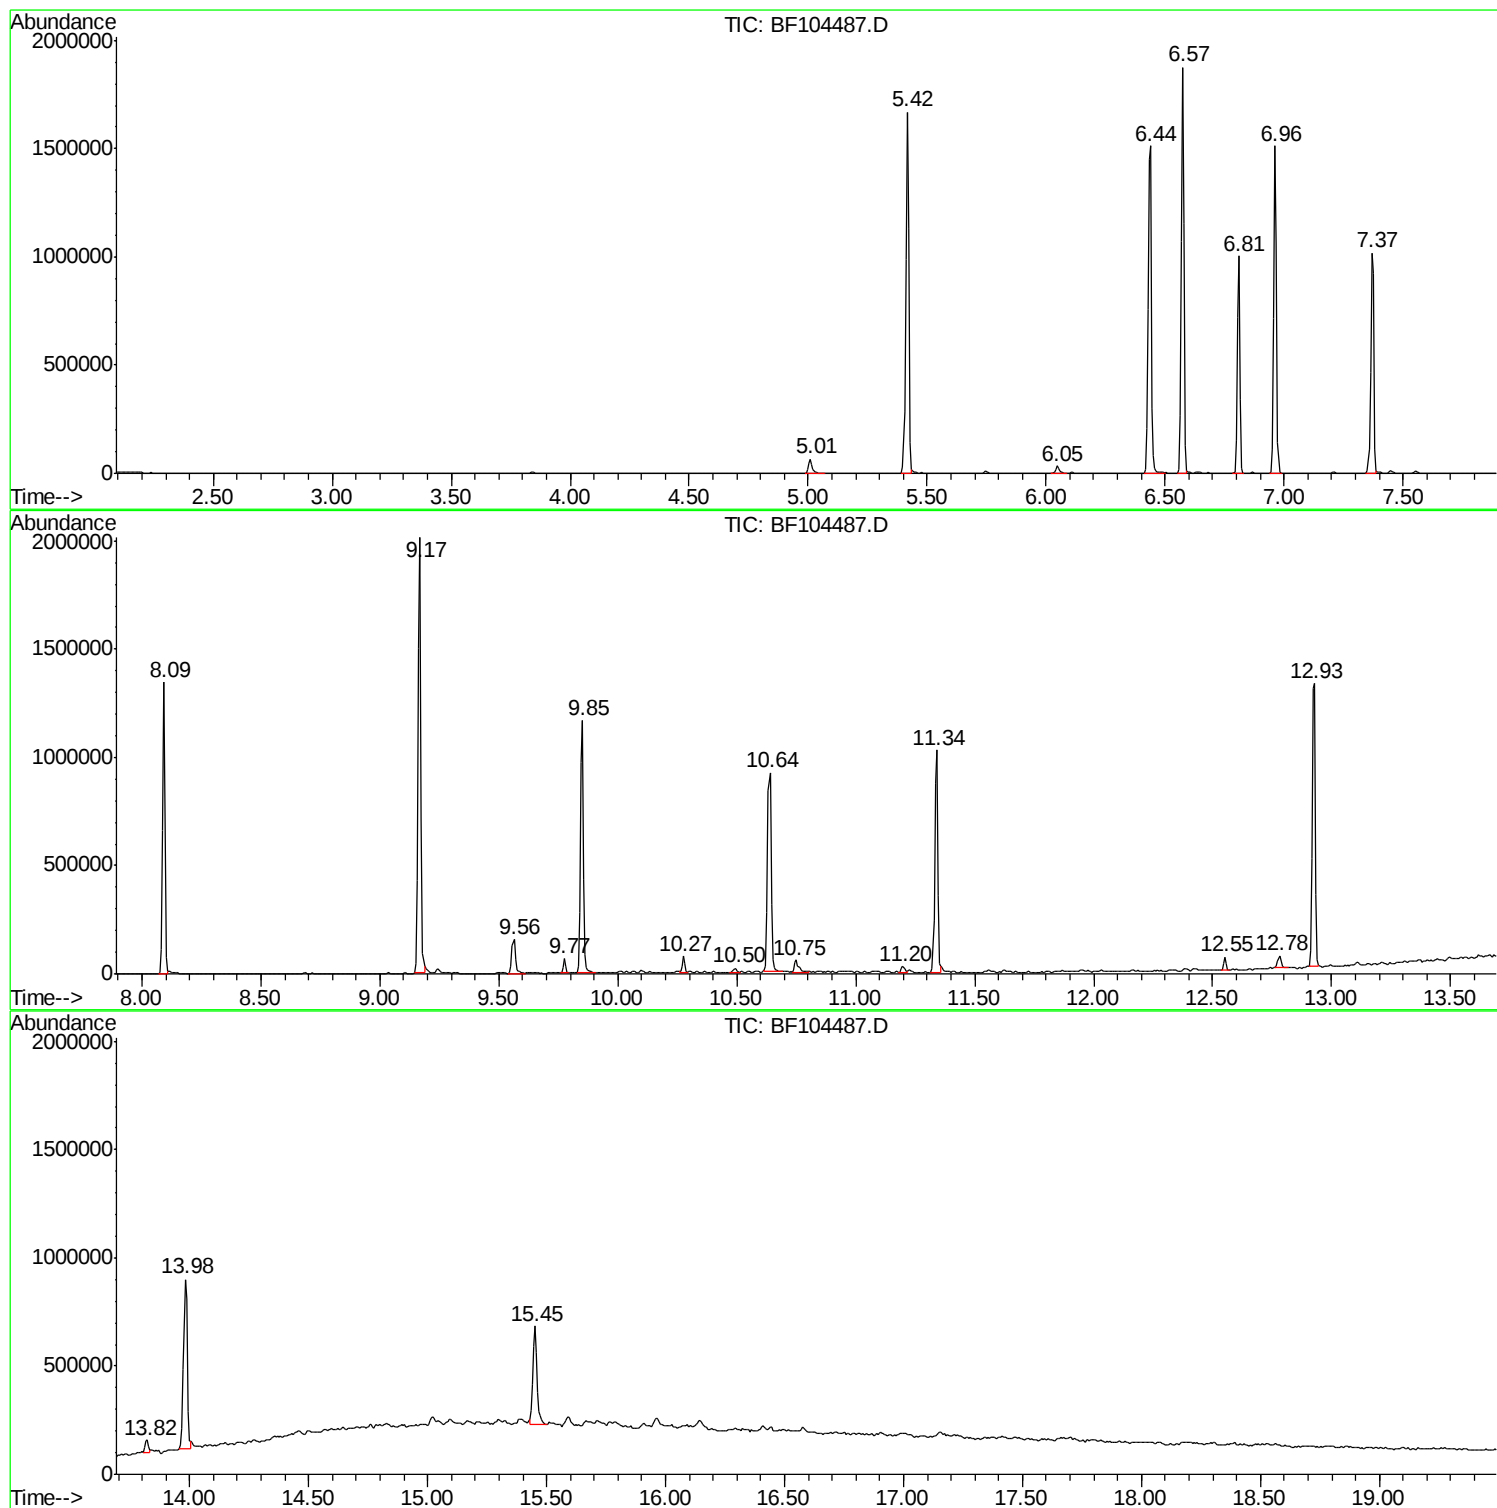

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041318\
Data File : BF104487.D
Acq On : 13 Apr 2018 19:08
Operator : JU/SJ
Sample : J2166-03 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TR-04-041218










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.57 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.57	40.07 ng	1591550	1,4-Dichlorobenzene-d4	6.81

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
5		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

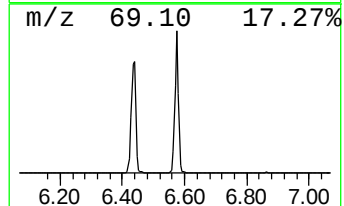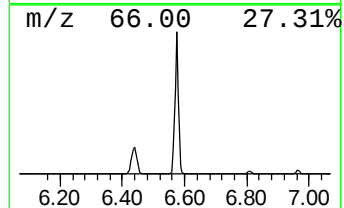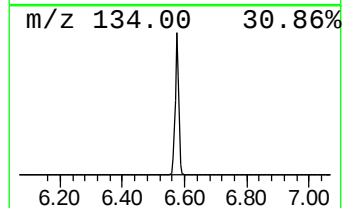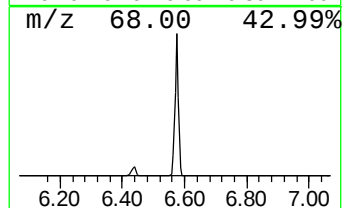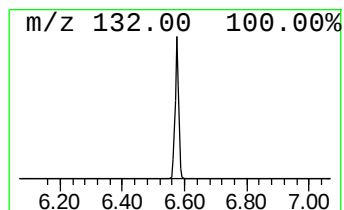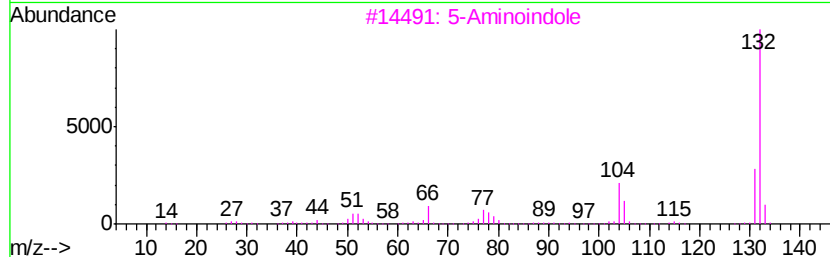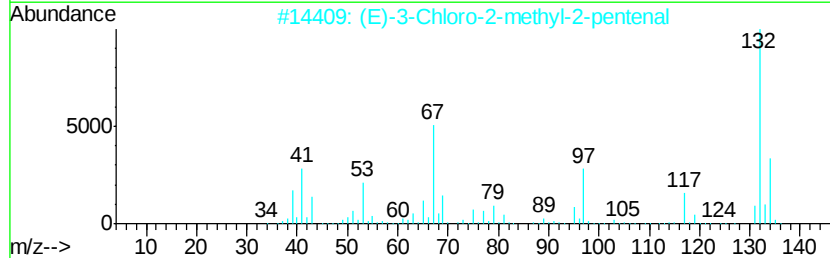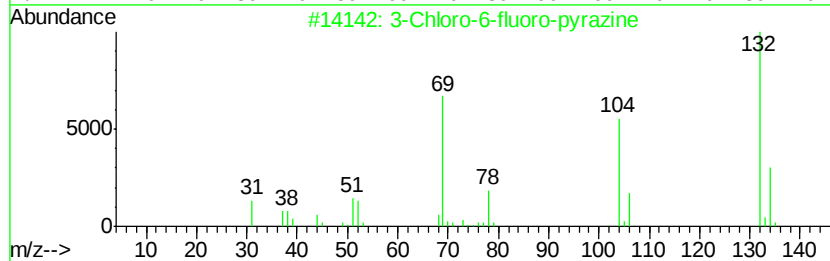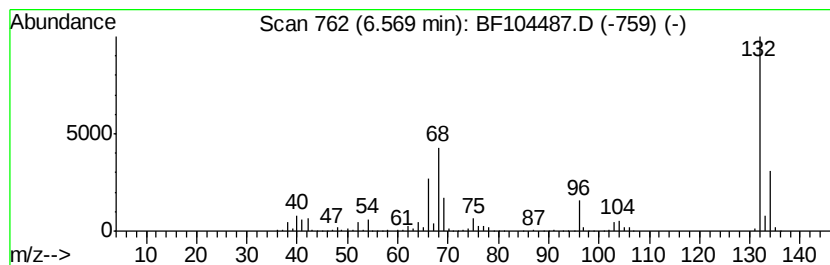

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041318\
Data File : BF104487.D
Acq On : 13 Apr 2018 19:08
Operator : JU/SJ
Sample : J2166-03 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TR-04-041218

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.57	6.57	40.1	ng	1591550	1	6.81	794417	20.0