


Data Path : Z:\HPCHEM1\BNA_F\Data\BF041318\
 Data File : BF104472.D
 Acq On : 13 Apr 2018 12:21
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 16 12:15:25 2018

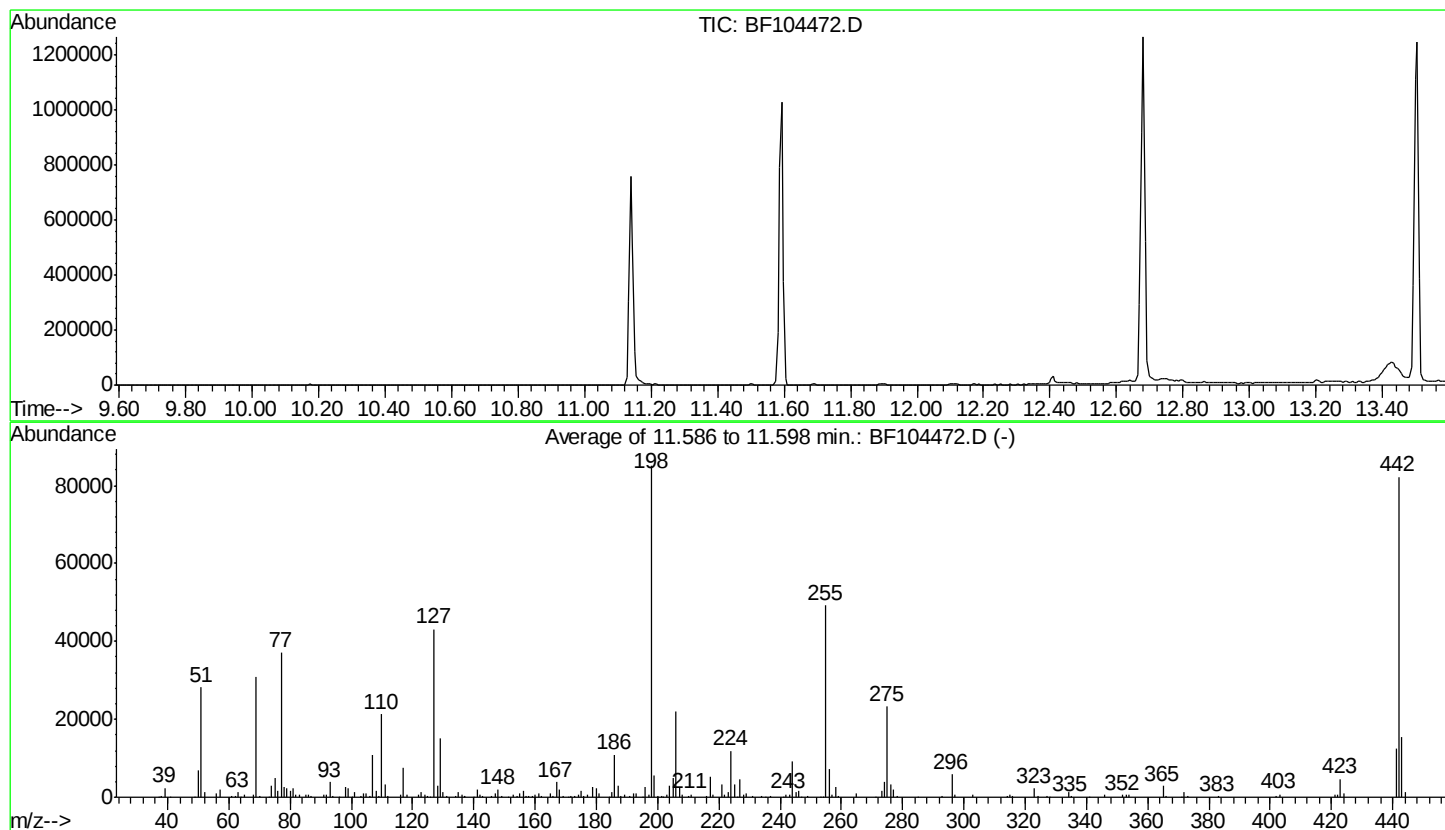

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.1	28156	PASS
68	69	0.00	2	1.7	521	PASS
69	198	0.00	100	36.4	30975	PASS
70	69	0.00	2	0.8	259	PASS
127	198	10	80	50.7	43180	PASS
197	198	0.00	2	0.9	787	PASS
198	198	100	100	100.0	85138	PASS
199	198	5	9	6.8	5759	PASS
275	198	10	60	27.3	23279	PASS
365	198	1	100	3.5	2951	PASS
441	443	0.01	100	81.0	12415	PASS
442	198	50	100	96.7	82338	PASS
443	442	15	24	18.6	15329	PASS