


Data Path : Z:\HPCHEM1\BNA F\Data\BF041318\
 Data File : BF104499.D
 Acq On : 14 Apr 2018 1:22
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 16 12:15:25 2018

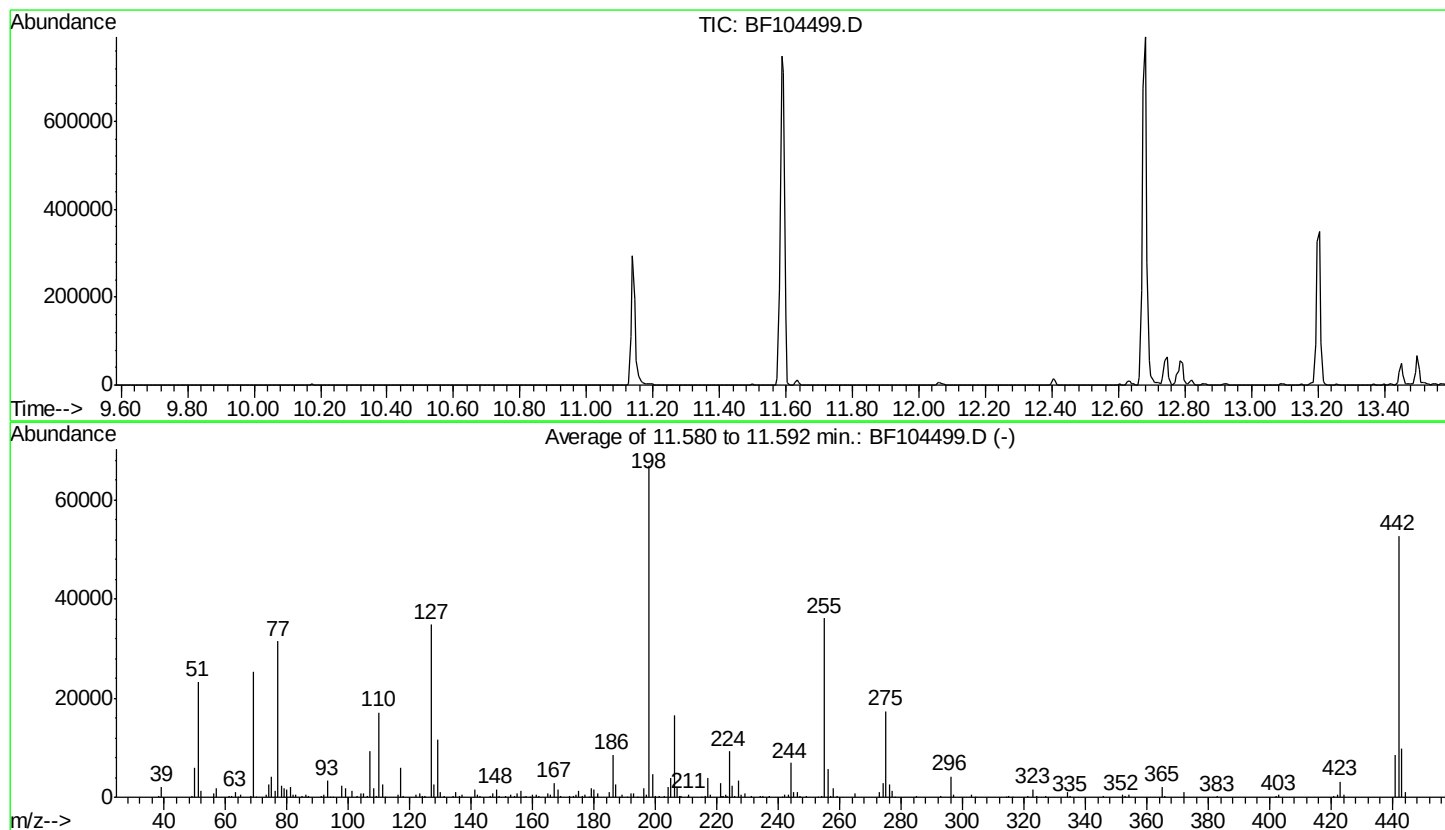

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	23303	PASS
68	69	0.00	2	1.3	332	PASS
69	198	0.00	100	37.9	25341	PASS
70	69	0.00	2	0.4	112	PASS
127	198	10	80	52.0	34794	PASS
197	198	0.00	2	0.9	579	PASS
198	198	100	100	100.0	66949	PASS
199	198	5	9	7.0	4678	PASS
275	198	10	60	26.0	17419	PASS
365	198	1	100	3.2	2149	PASS
441	443	0.01	100	86.1	8506	PASS
442	198	50	100	78.9	52849	PASS
443	442	15	24	18.7	9878	PASS