
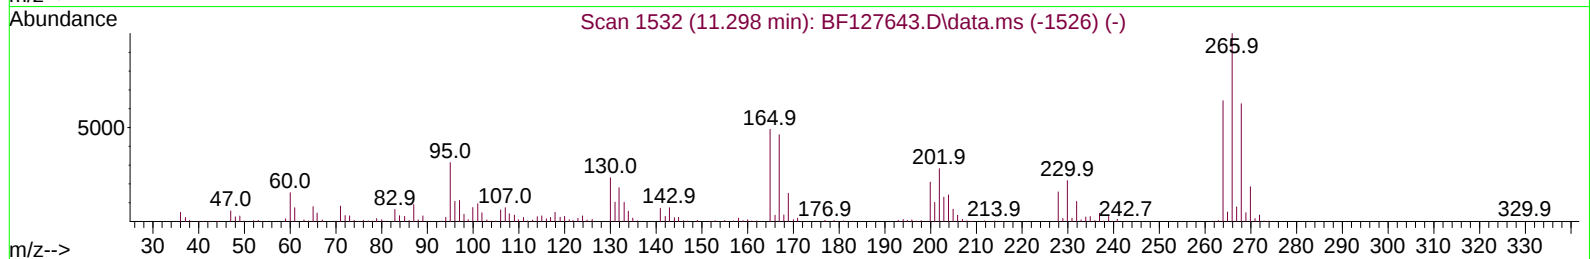
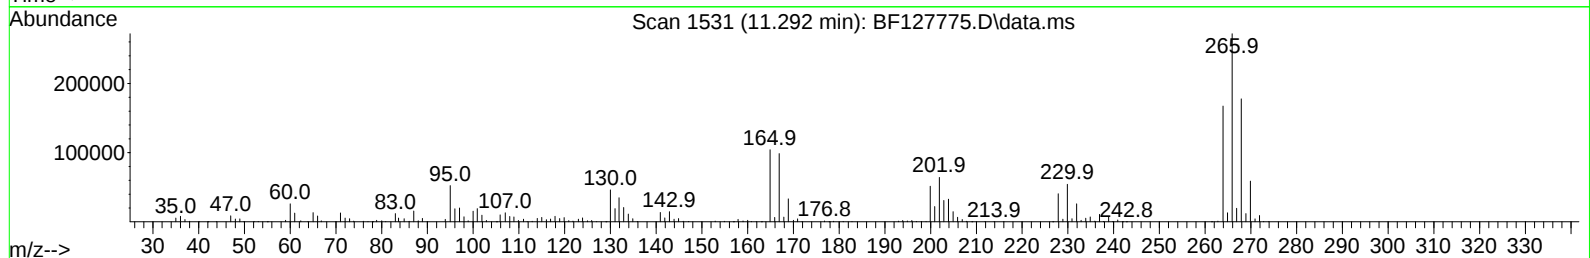


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF041322\  
Data File : BF127775.D  
Acq On : 13 Apr 2022 10:07  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 16:44:26 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF040622.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Apr 13 16:40:15 2022  
Response via : Initial Calibration

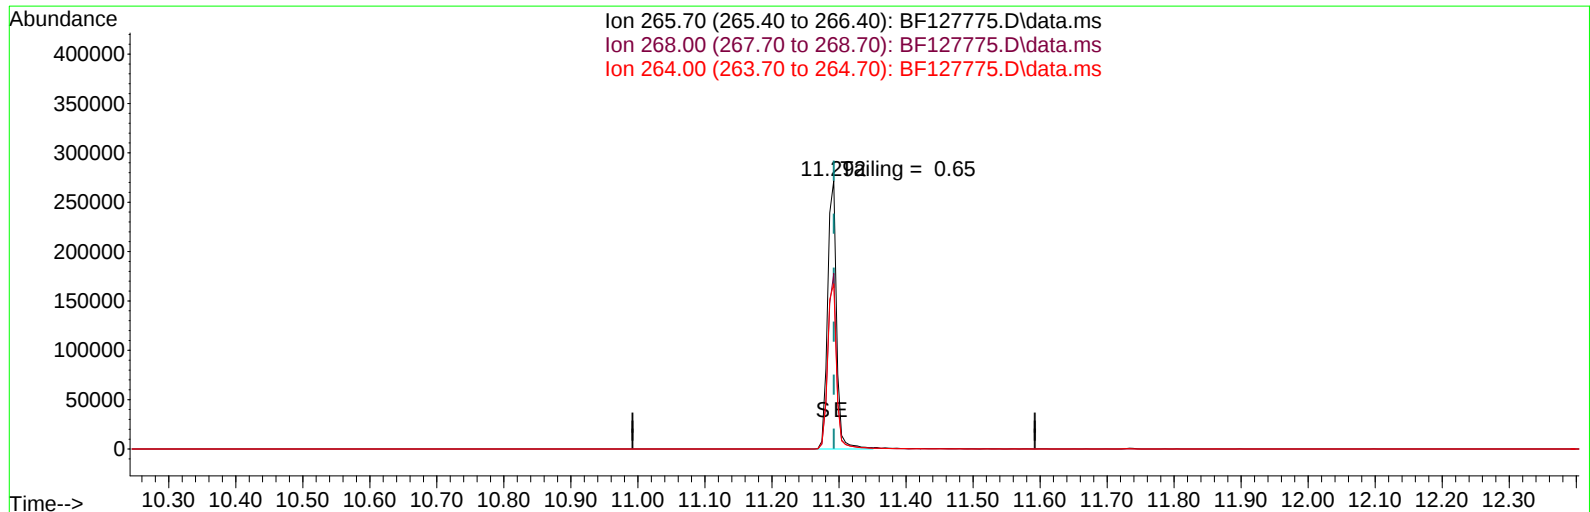

TIC: BF127775.D\data.ms

**(70) Pentachlorophenol (C)**

**11.292min (-0.000) 574222.34 ng**

**response 254798**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.00  | 65.42  |
| 264.00 | 60.60  | 61.58  |
| 0.00   | 0.00   | 0.00   |