
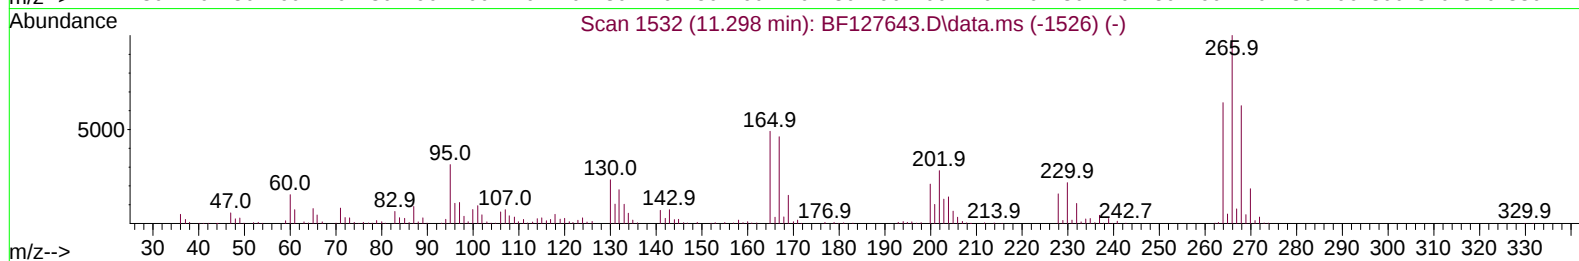
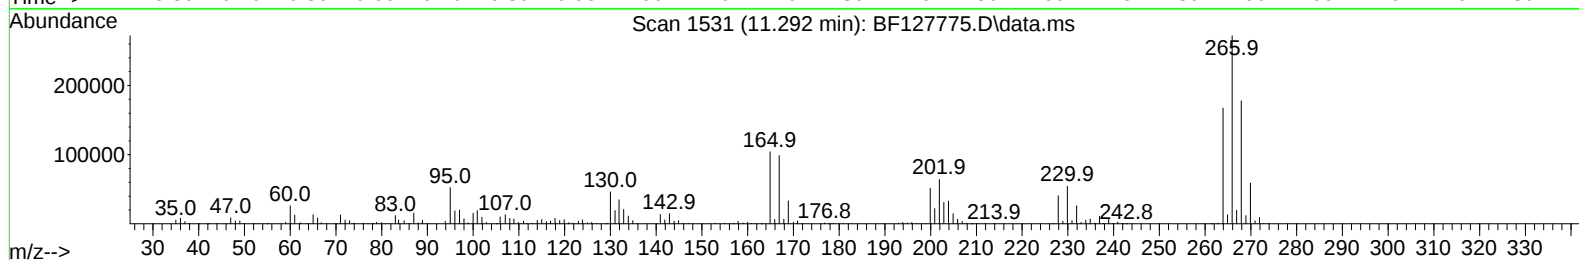


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041322\
 Data File : BF127775.D
 Acq On : 13 Apr 2022 10:07
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 16:44:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 13 16:40:15 2022
 Response via : Initial Calibration

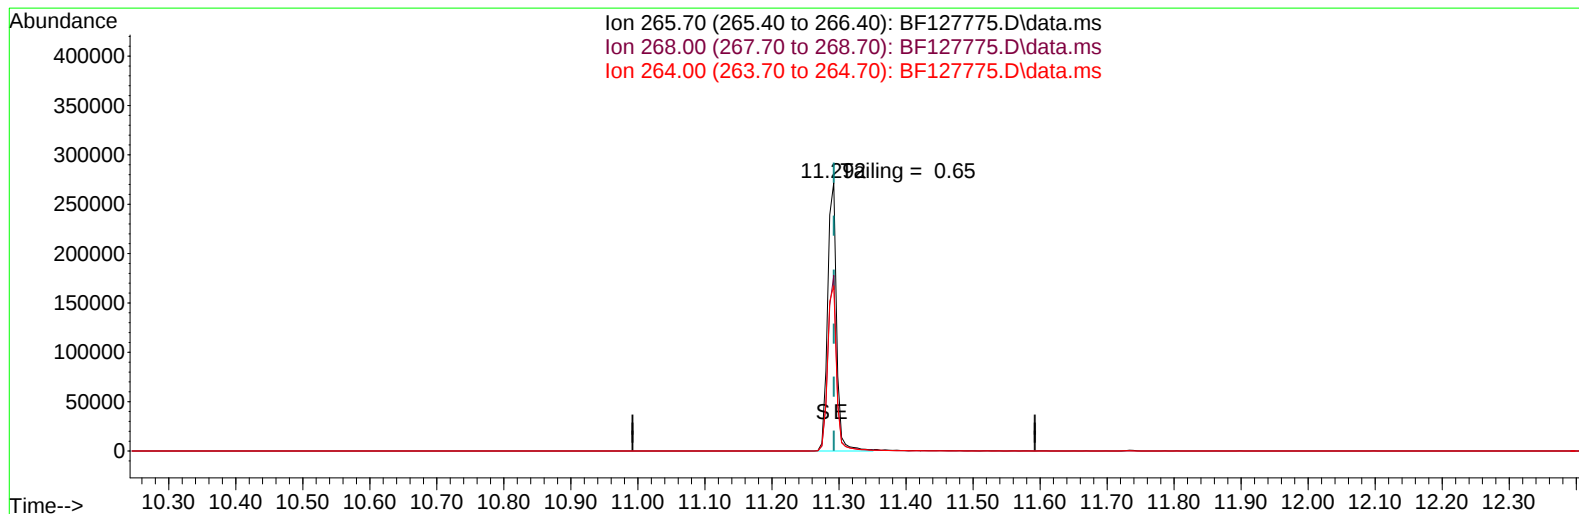

TIC: BF127775.D\data.ms

(70) Pentachlorophenol (C)




11.292min (-0.000) 574222.34 ng

response 254798

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	65.42
264.00	60.60	61.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041322\
Data File : BF127775.D
Acq On : 13 Apr 2022 10:07
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 16:44:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 16:40:15 2022
Response via : Initial Calibration

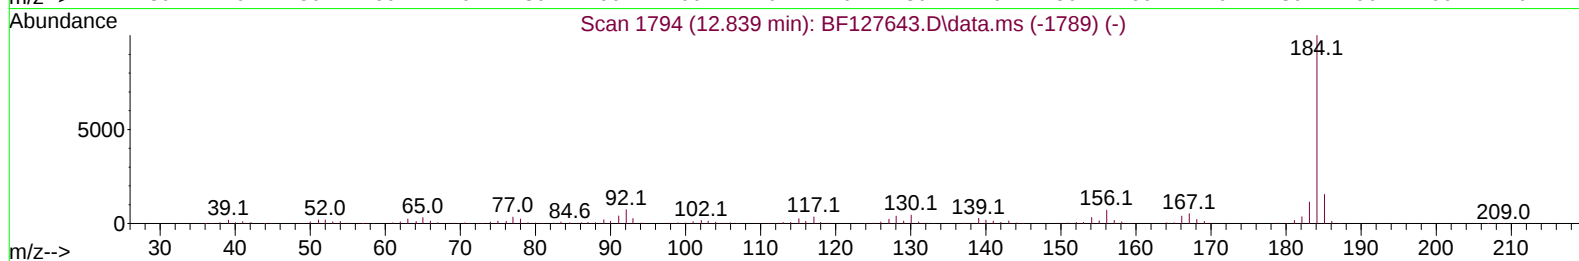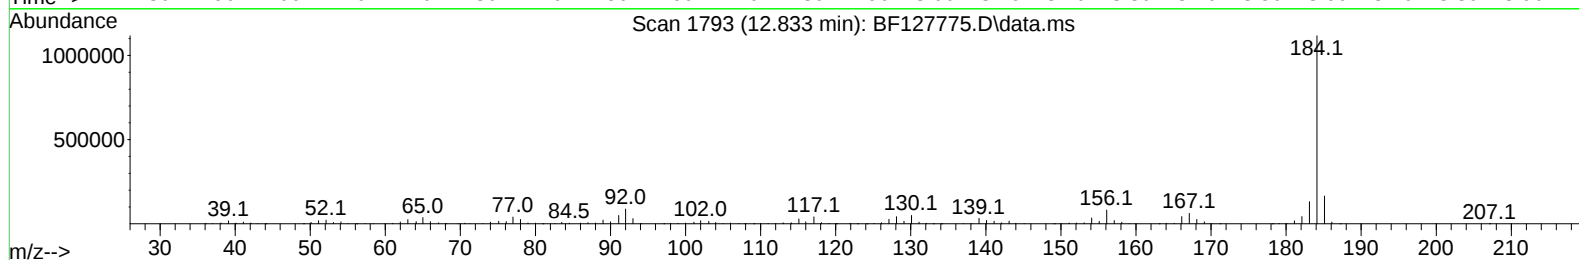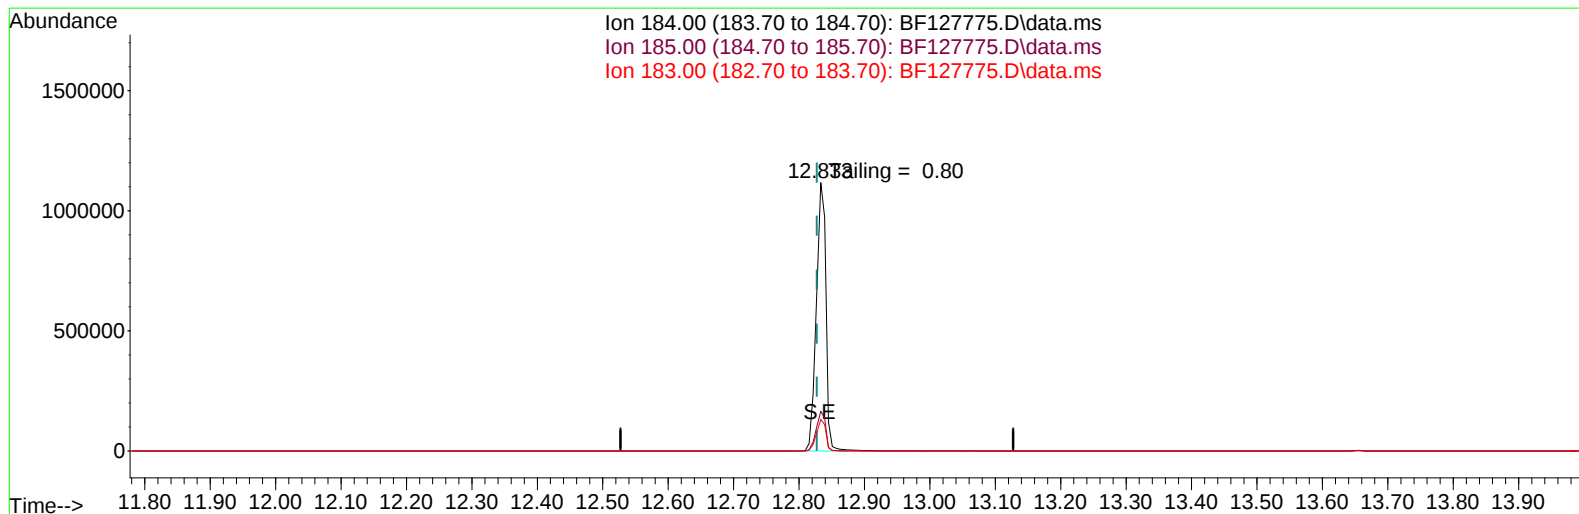

TIC: BF127775.D\data.ms

(77) Benzidine

12.833min (+ 0.006) 132313.26 ng

response 1143098

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.77
183.00	11.70	11.76
0.00	0.00	0.00