
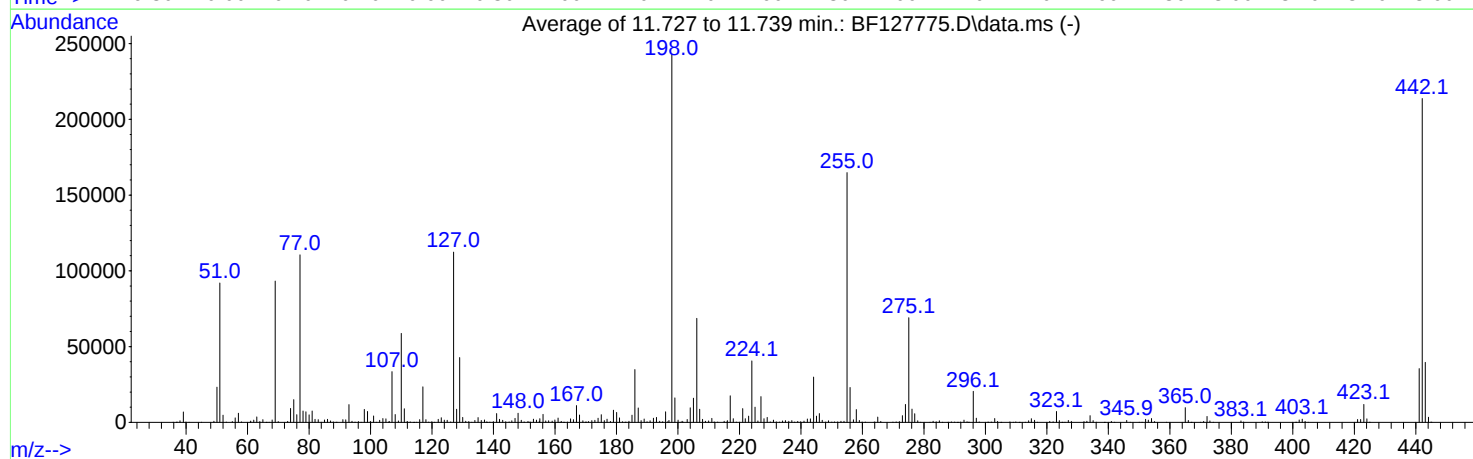


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041322\
 Data File : BF127775.D
 Acq On : 13 Apr 2022 10:07
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 13 16:40:15 2022

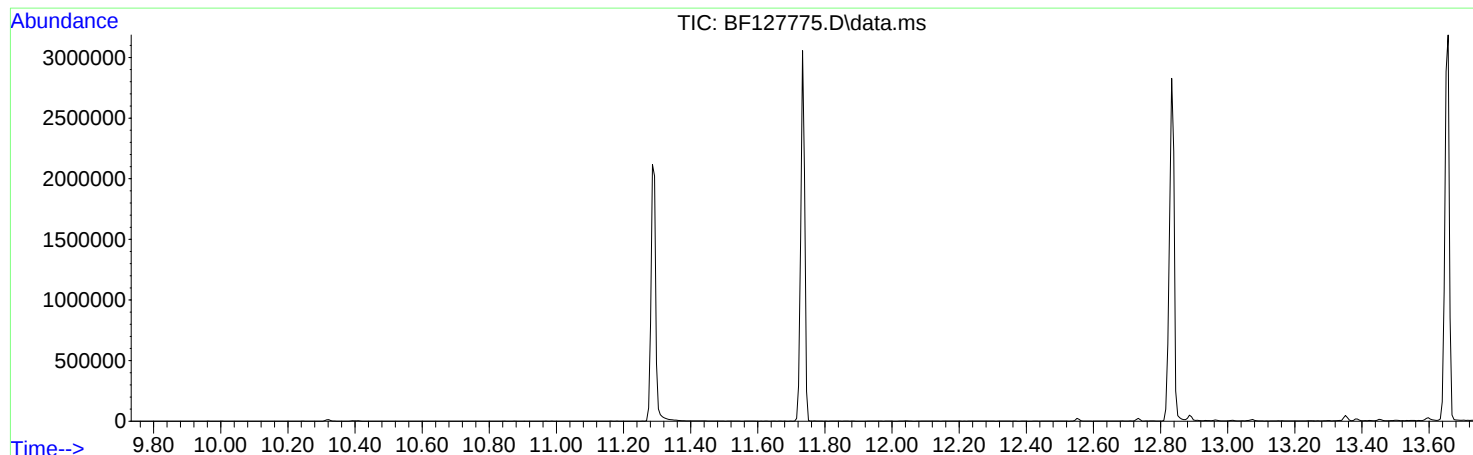




AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	91944	PASS
68	69	0.00	2	1.7	1593	PASS
69	198	0.00	100	38.4	93208	PASS
70	69	0.00	2	0.5	490	PASS
127	198	10	80	46.3	112360	PASS
197	198	0.00	2	0.5	1323	PASS
198	198	100	100	100.0	242773	PASS
199	198	5	9	6.7	16214	PASS
275	198	10	60	28.5	69072	PASS
365	198	1	100	4.0	9702	PASS
441	198	0.01	100	14.6	35500	PASS
442	442	50	100	100.0	213768	PASS
443	442	15	24	18.5	39553	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041322\
Data File : BF127775.D
Acq On : 13 Apr 2022 10:07
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 13 16:44:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 16:40:15 2022
Response via : Initial Calibration

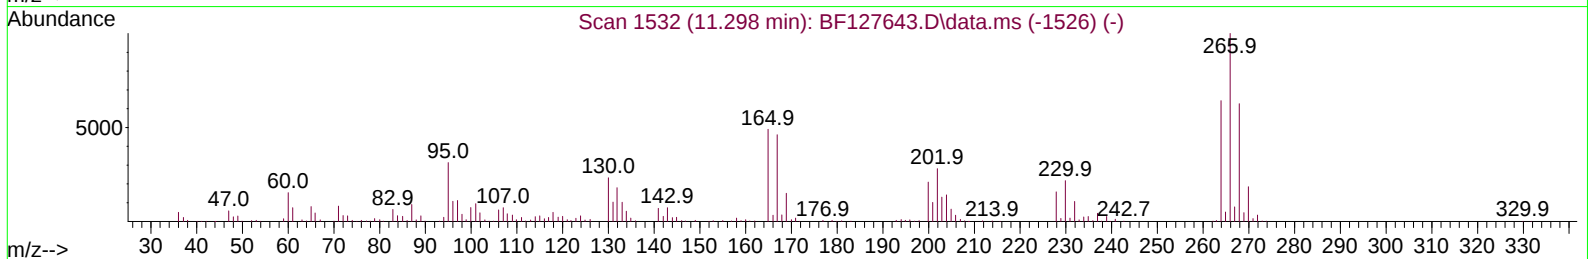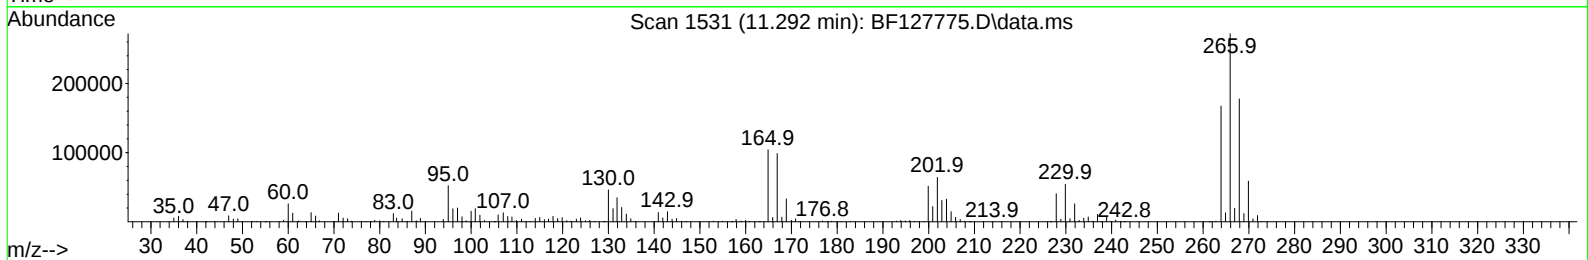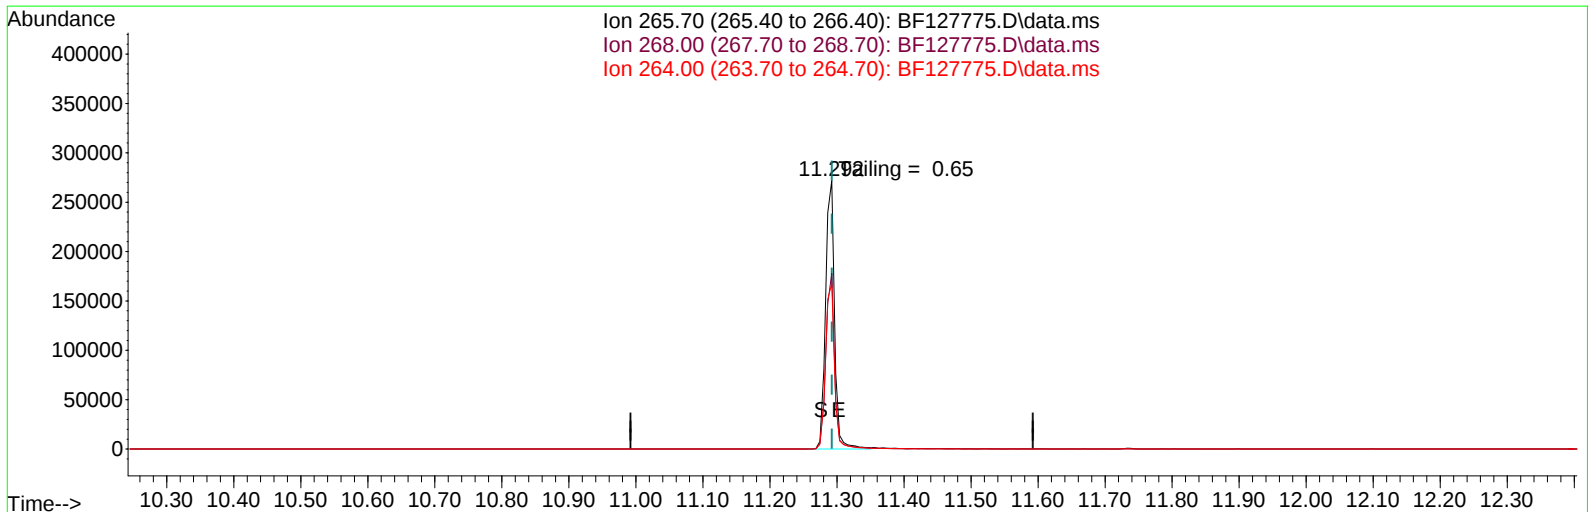

TIC: BF127775.D\data.ms

(70) Pentachlorophenol (C)

11.292min (-0.000) 574222.34 ng




response 254798

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	65.42
264.00	60.60	61.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041322\
Data File : BF127775.D
Acq On : 13 Apr 2022 10:07
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 13 16:44:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 16:40:15 2022
Response via : Initial Calibration

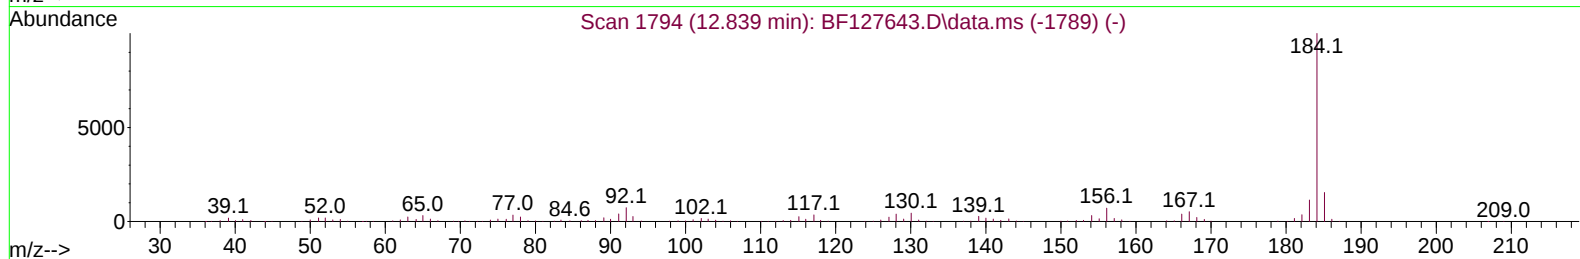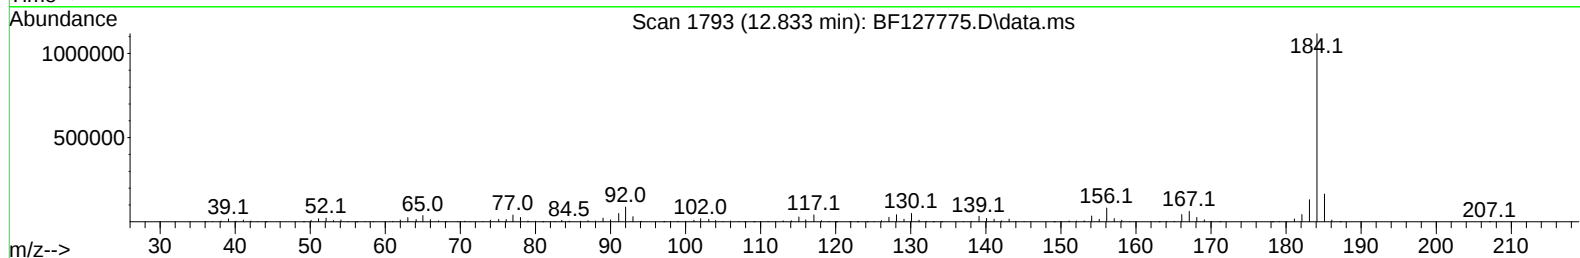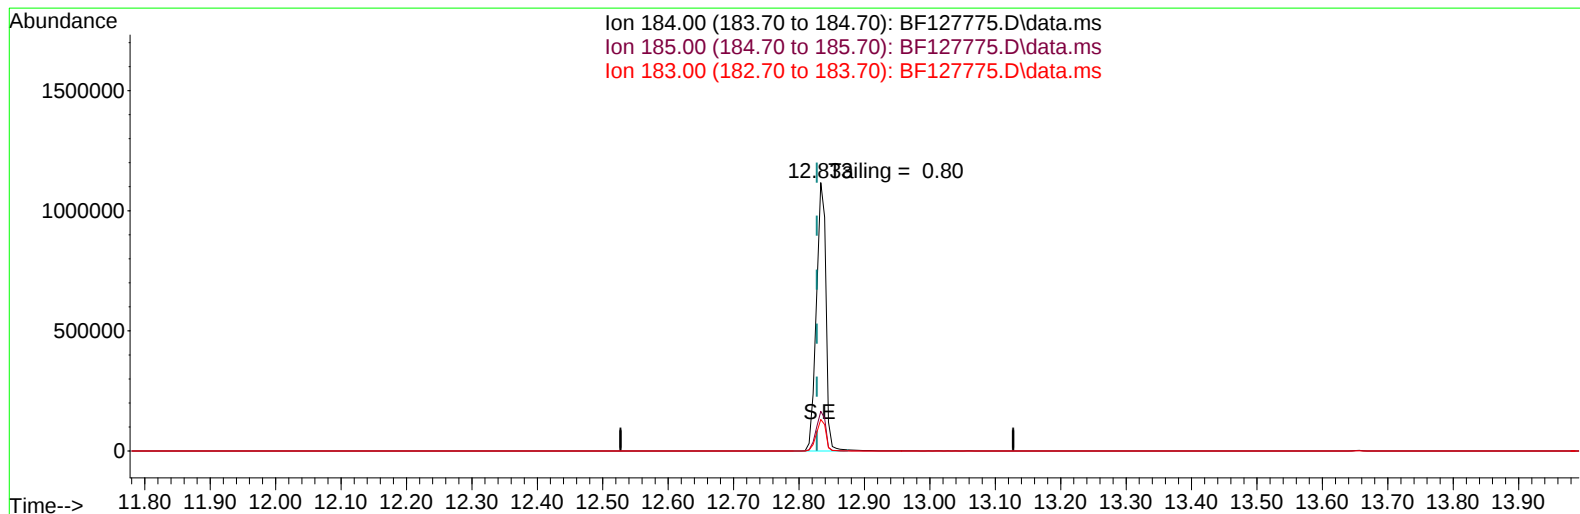

TIC: BF127775.D\data.ms

(77) Benzidine

12.833min (+ 0.006) 132313.26 ng

response 1143098

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.77
183.00	11.70	11.76
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/13/2022	BNA_F	<u>BF127775.D</u>
Compound Name	Response	Retention Time
DDT	572648	13.65
DDD	7813	13.35
DDE	909	13.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8722	581370	1.50

Instrument :
BNA_F
ClientSampleId :
DFTPP