
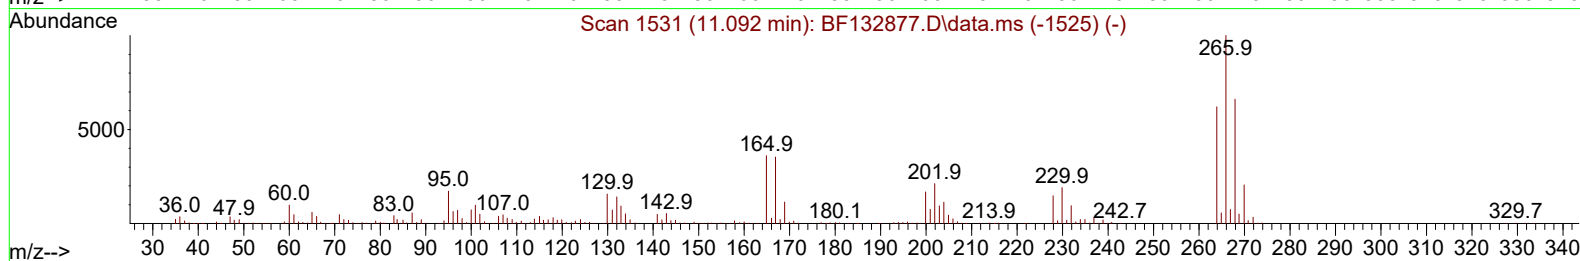
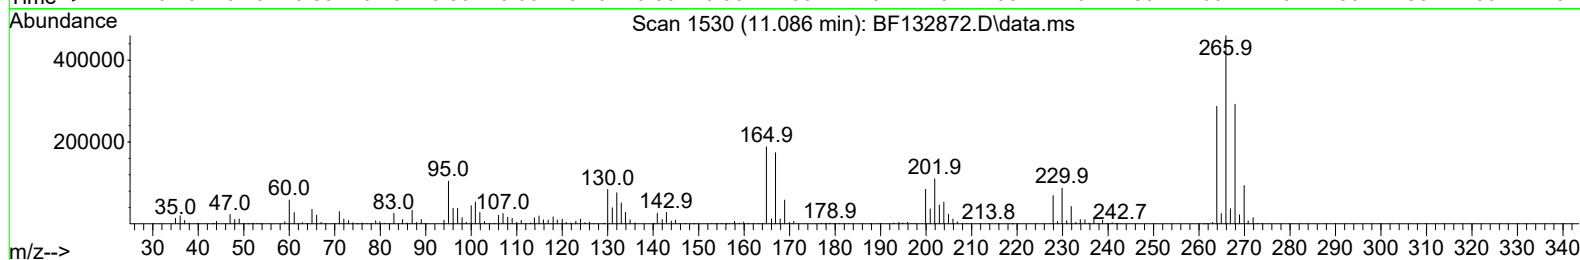


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041323\  
Data File : BF132872.D  
Acq On    : 13 Apr 2023  11:48  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Apr 14 07:14:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 14 05:12:08 2023
Response via : Initial Calibration

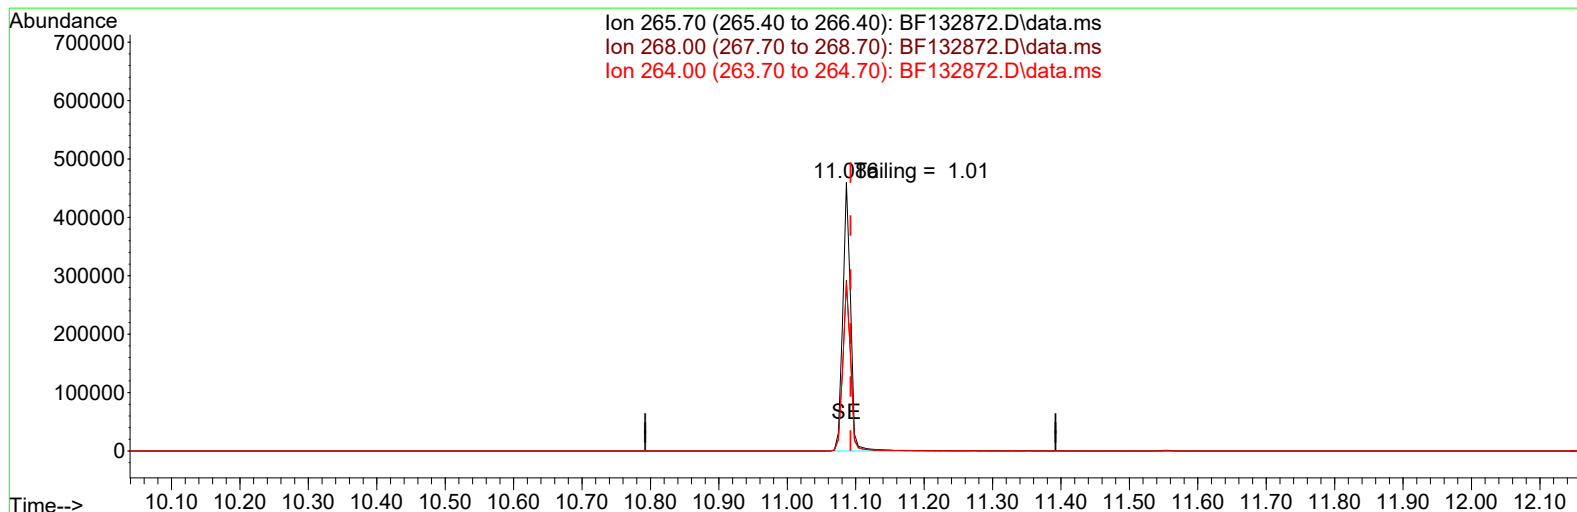

TIC: BF132872.D\data.ms

(70) Pentachlorophenol (C)




11.086min (-0.006) 325723.02 ng

response **366050**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	63.62
264.00	62.10	62.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041323\
 Data File : BF132872.D
 Acq On : 13 Apr 2023 11:48
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 07:14:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 14 05:12:08 2023
 Response via : Initial Calibration

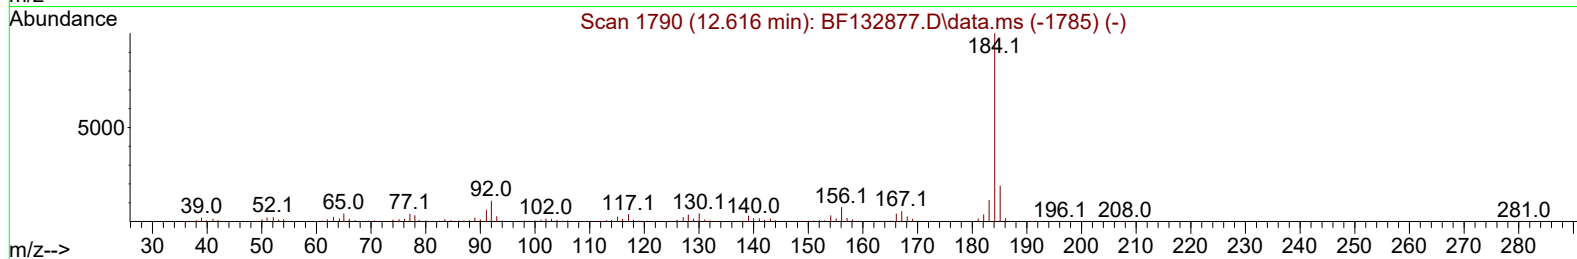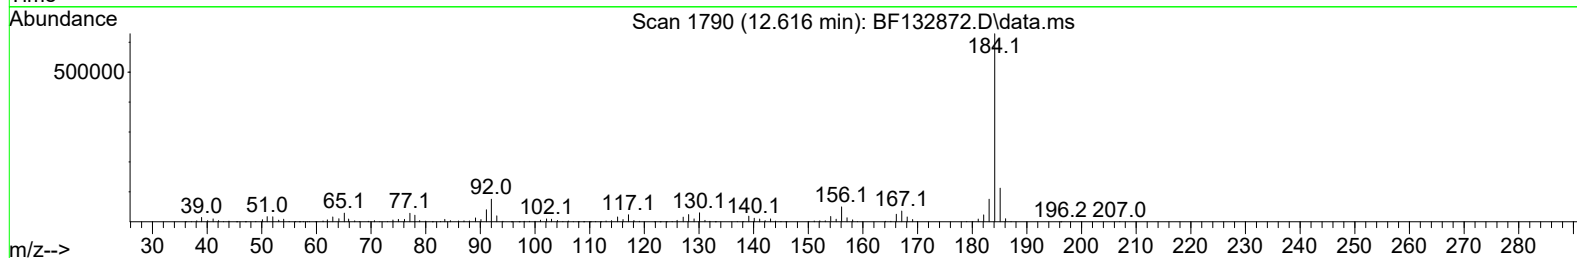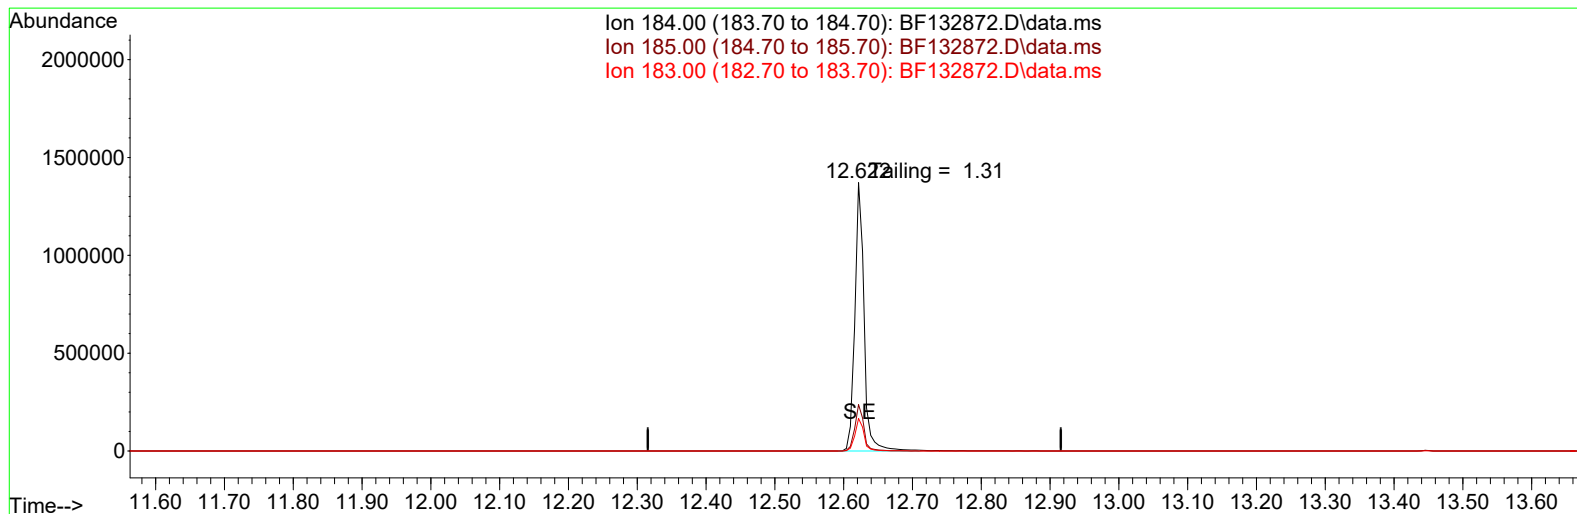

TIC: BF132872.D\data.ms

(77) Benzidine

12.616min (-12.616) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	18.90	0.00#
183.00	11.40	0.00#
0.00	0.00	0.00