


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041323\
 Data File : BF132872.D
 Acq On : 13 Apr 2023 11:48
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 14 05:12:08 2023

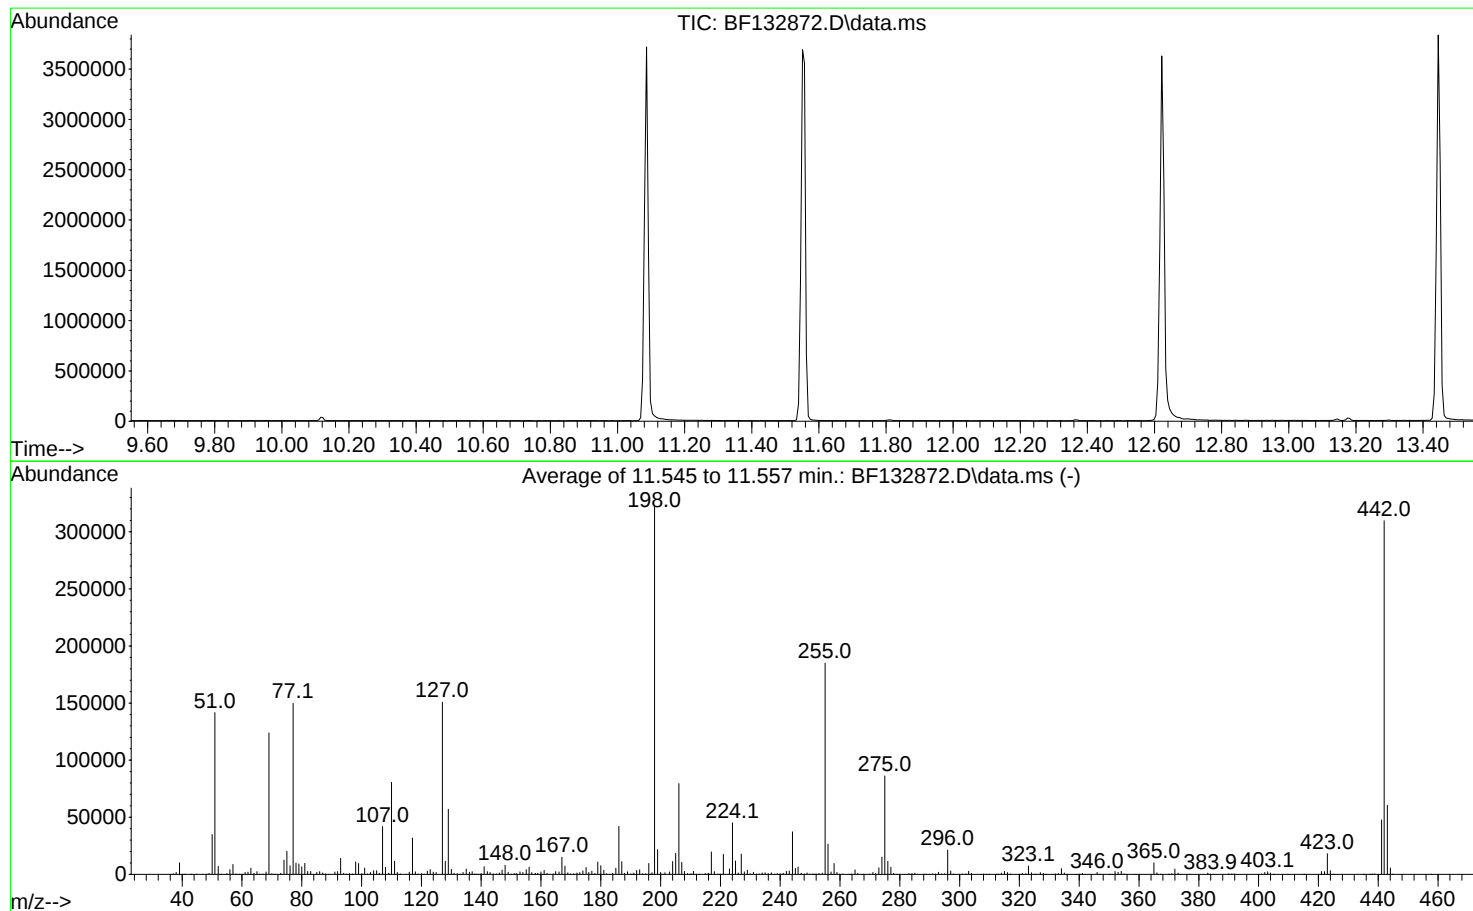

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.0	141634	PASS
68	69	0.00	2	1.7	2147	PASS
69	198	0.00	100	38.4	123824	PASS
70	69	0.00	2	0.5	636	PASS
127	198	10	80	46.8	150851	PASS
197	198	0.00	2	0.5	1455	PASS
198	198	100	100	100.0	322176	PASS
199	198	5	9	6.7	21638	PASS
275	198	10	60	26.8	86235	PASS
365	198	1	100	3.1	10116	PASS
441	198	0.01	100	14.8	47598	PASS
442	442	50	100	100.0	309736	PASS
443	442	15	24	19.5	60353	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/13/2023	BNA_F	<u>BF132872.D</u>
Compound Name	Response	Retention Time
DDT	483698	13.445
DDD	4886	13.18
DDE	143	12.816
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5029	488727	1.03

Instrument :
BNA_F
ClientSampleId :
DFTPP

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041323\  
Data File : BF132872.D  
Acq On    : 13 Apr 2023  11:48  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 14 07:14:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 14 05:12:08 2023
Response via : Initial Calibration

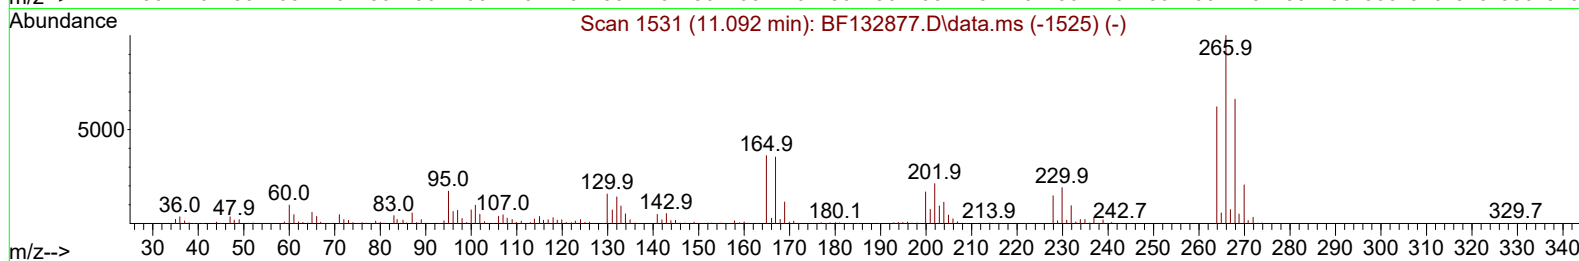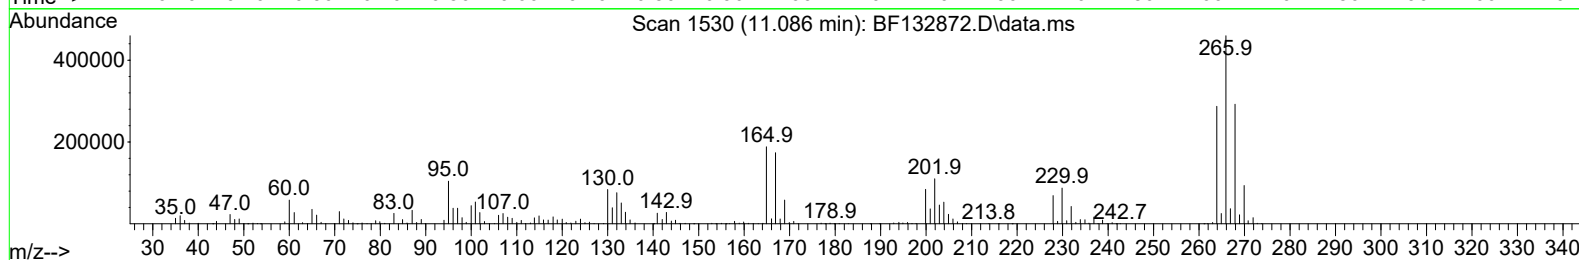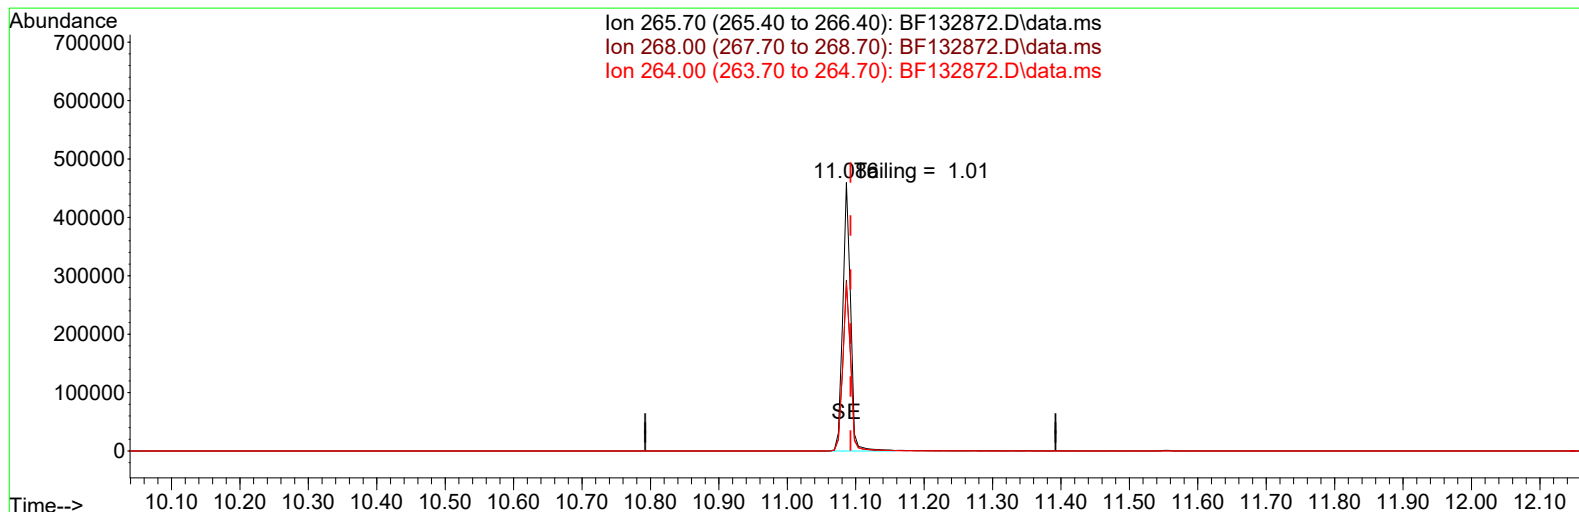

TIC: BF132872.D\data.ms

(70) Pentachlorophenol (C)

11.086min (-0.006) 325723.02 ng




response **366050**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	63.62
264.00	62.10	62.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041323\
Data File : BF132872.D
Acq On : 13 Apr 2023 11:48
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 14 07:14:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 14 05:12:08 2023
Response via : Initial Calibration

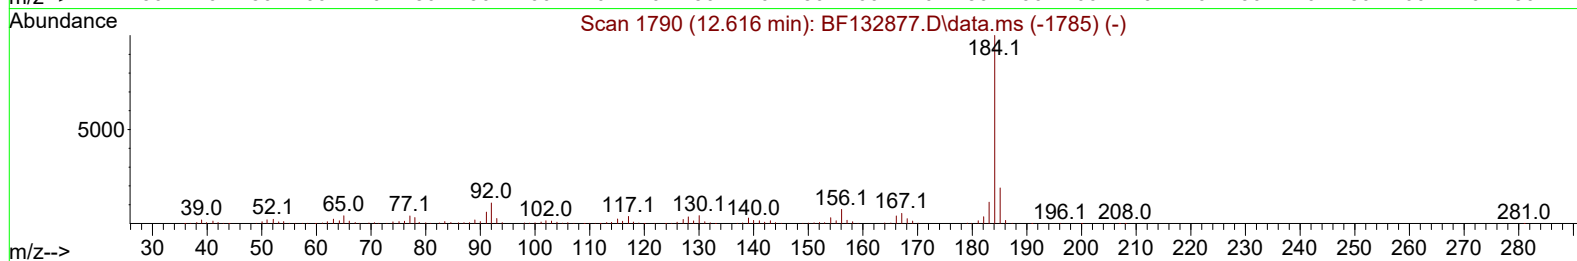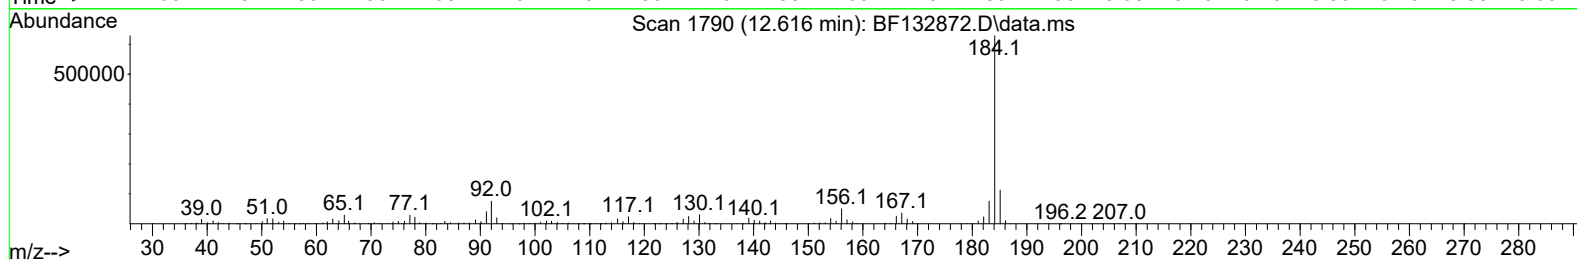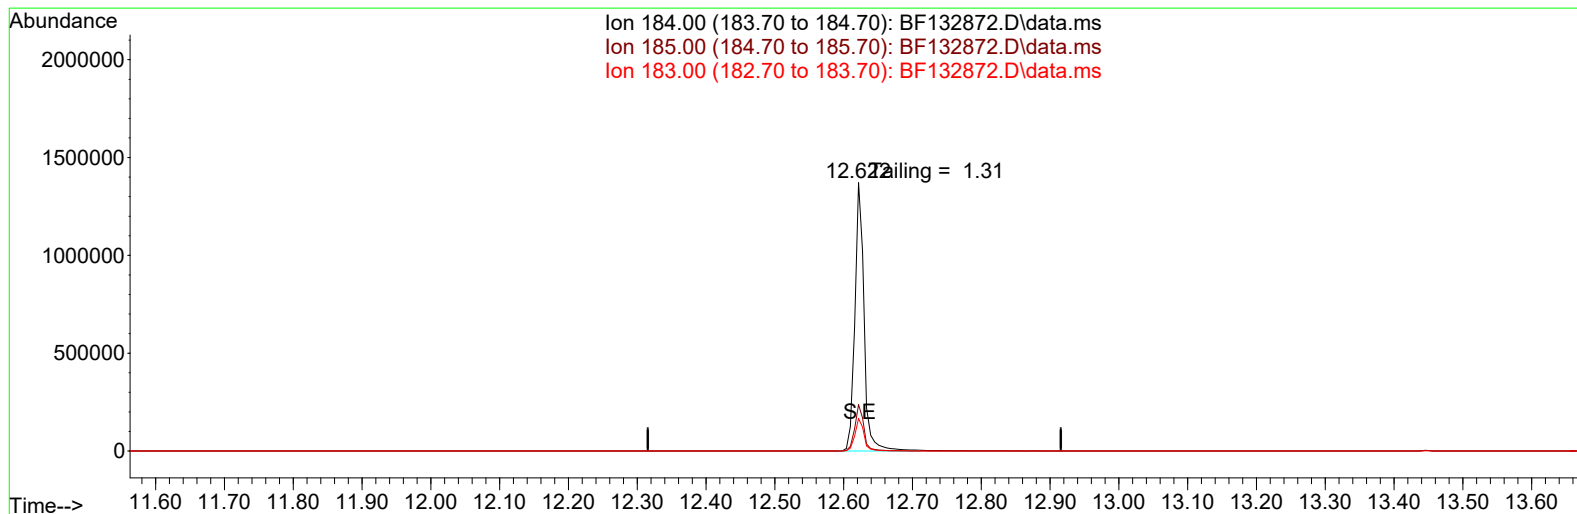

TIC: BF132872.D\data.ms

(77) Benzidine

12.616min (-12.616) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	18.90	0.00#
183.00	11.40	0.00#
0.00	0.00	0.00