
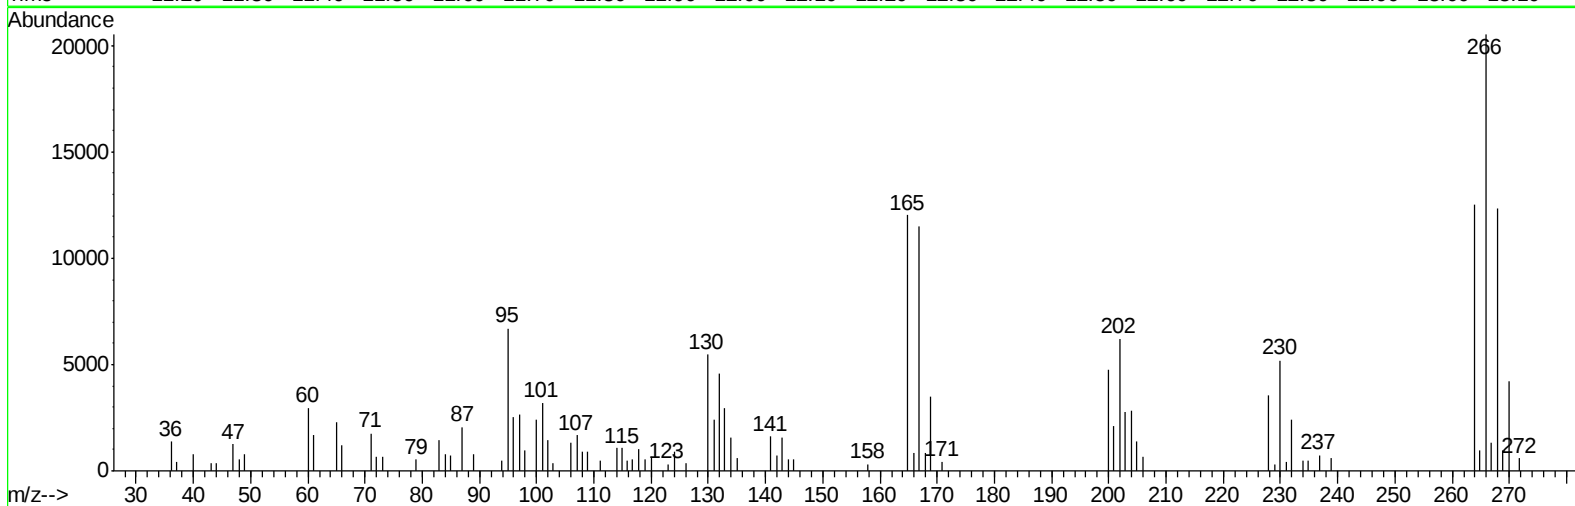


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041415\
Data File : BF078503.D
Acq On : 14 Apr 2015 15:41
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 15 09:11:41 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 15 01:10:59 2015
Response via : Initial Calibration

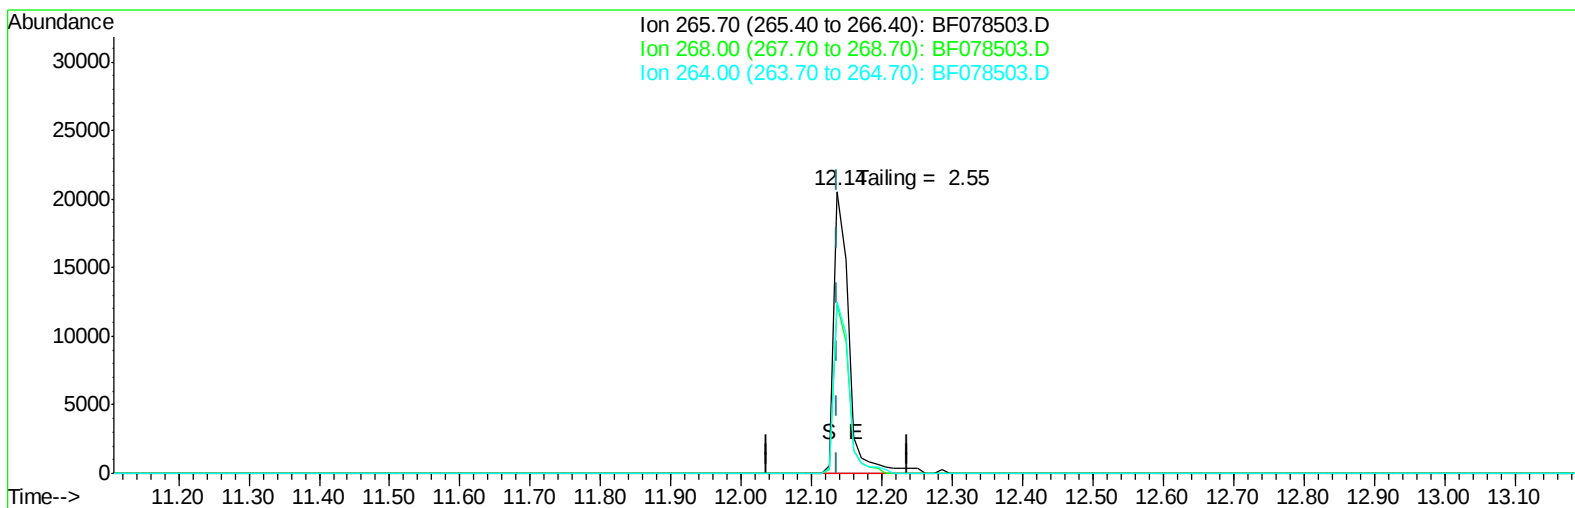

TIC: BF078503.D

(69) Pentachlorophenol (C)



12.137min (+0.000) 17467.66ng

response 28757

Ion	Exp%	Act%
265.70	100	100
268.00	62.60	60.20
264.00	62.50	61.02
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041415\
 Data File : BF078503.D
 Acq On : 14 Apr 2015 15:41
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 15 09:11:41 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 15 01:10:59 2015
 Response via : Initial Calibration

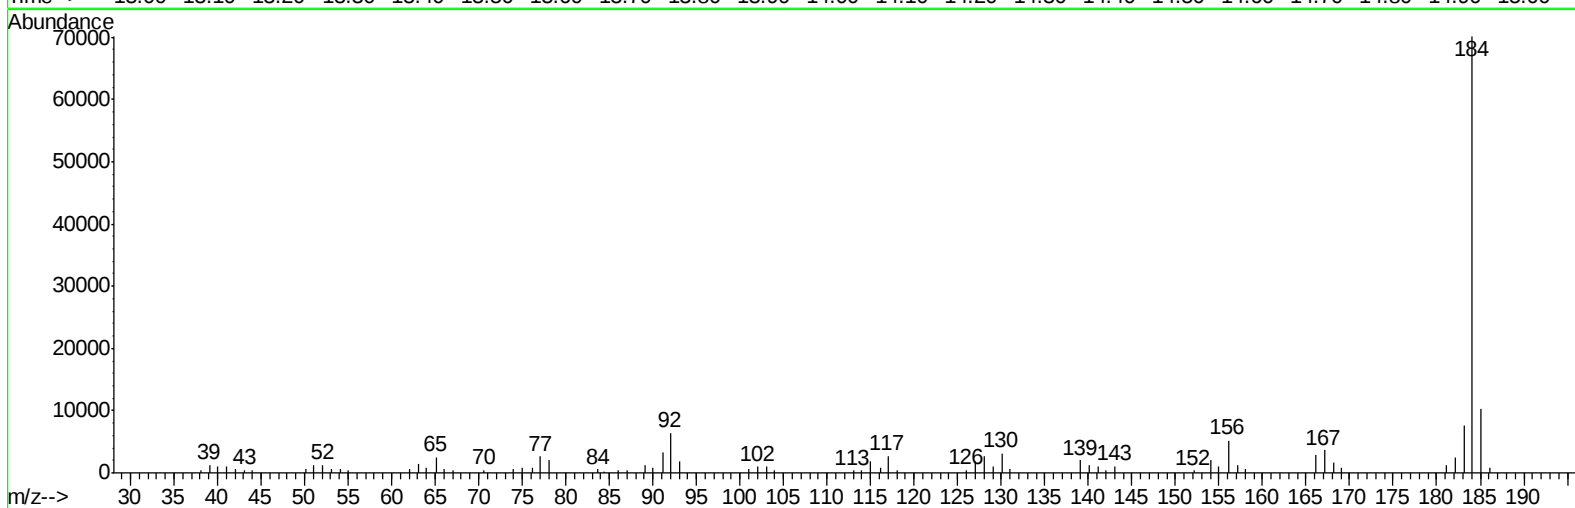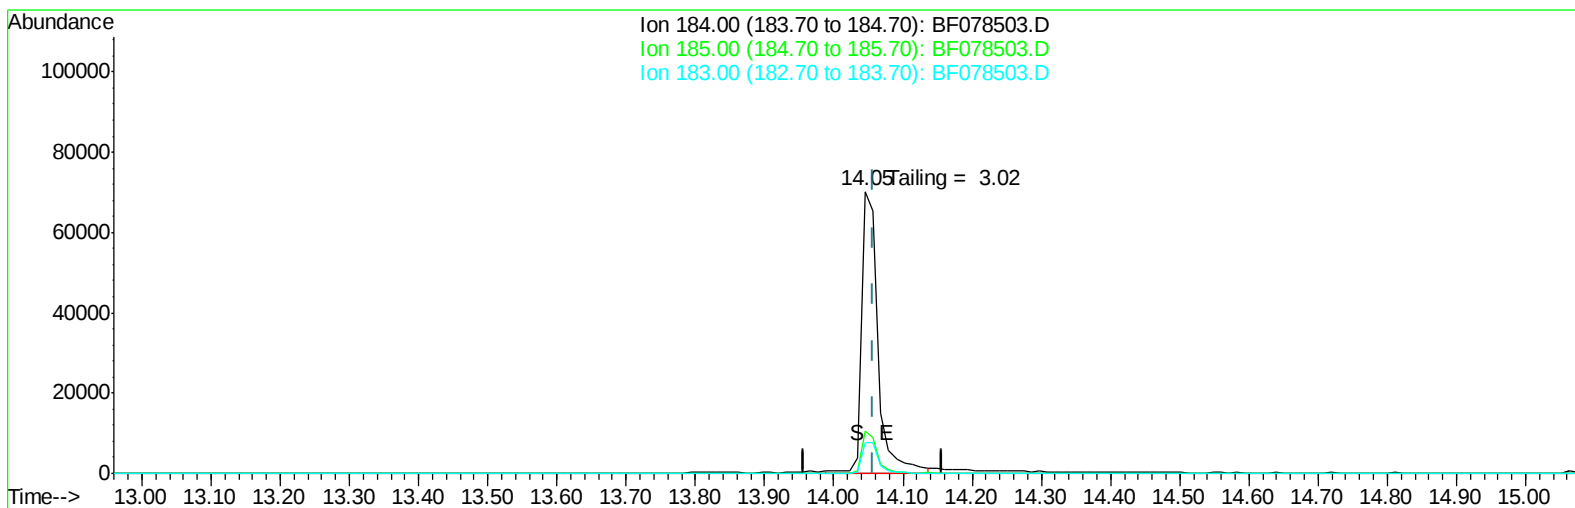

TIC: BF078503.D

(76) Benzidine

14.045min (-0.011) 7622.23ng

response 109768

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.80
183.00	11.90	10.80
0.00	0.00	0.00