
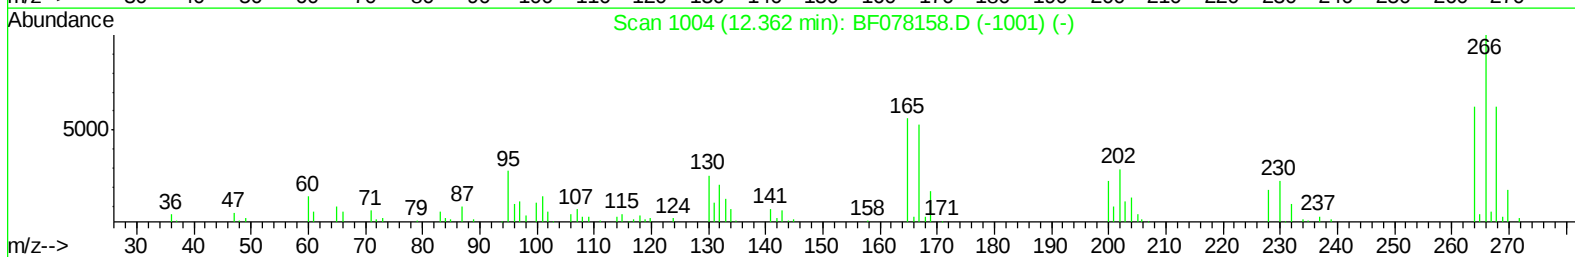
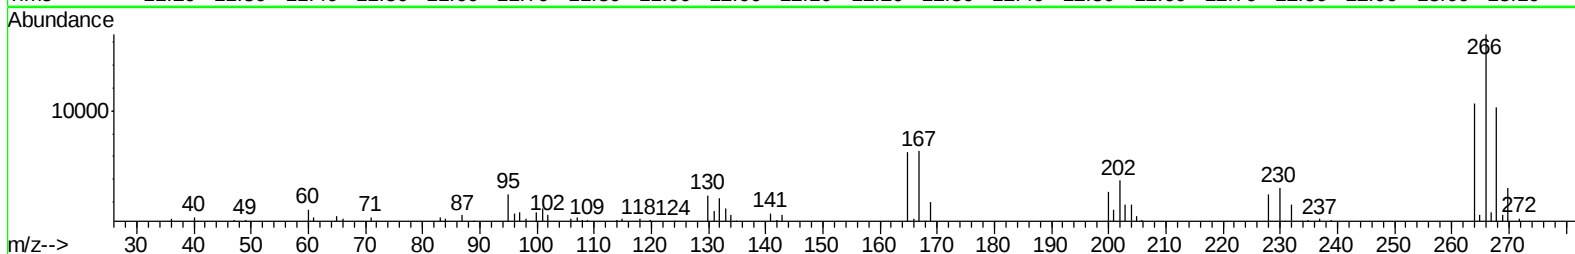


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041415\
Data File : BF078526.D
Acq On : 15 Apr 2015 5:27
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 15 09:13:42 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 15 01:10:59 2015
Response via : Initial Calibration

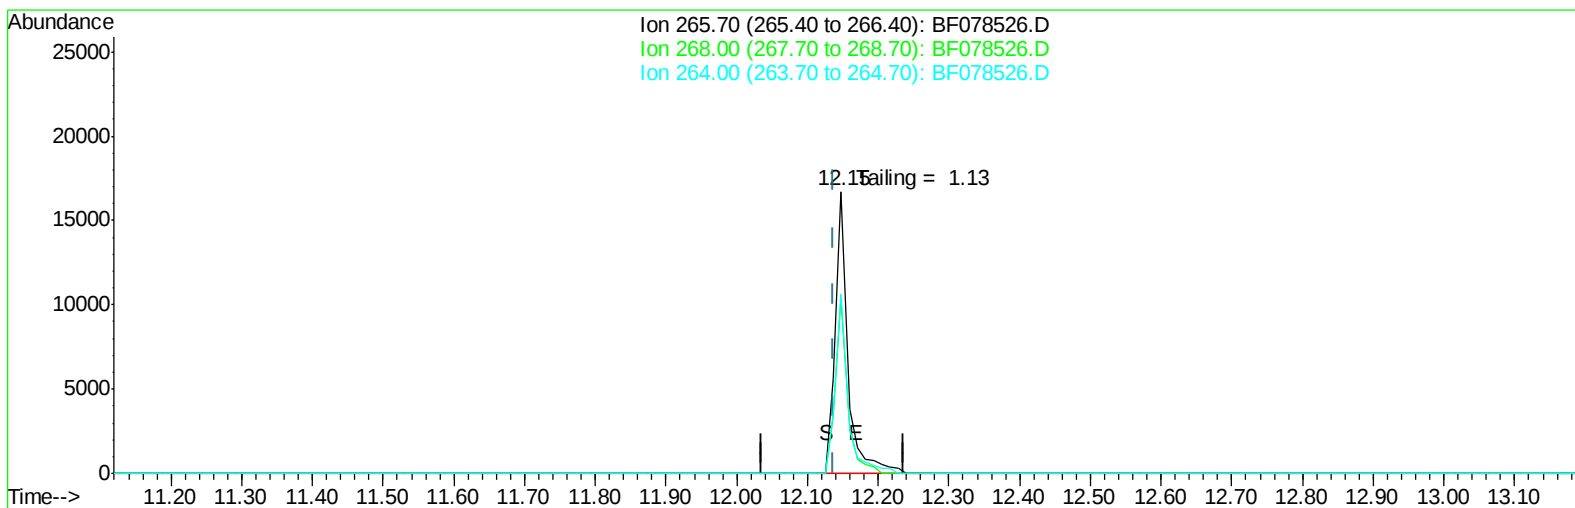

TIC: BF078526.D

(69) Pentachlorophenol (C)




12.148min (+0.011) 9410.74ng

response 20042

Ion	Exp%	Act%
265.70	100	100
268.00	62.60	61.76
264.00	62.50	63.77
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041415\
Data File : BF078526.D
Acq On : 15 Apr 2015 5:27
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 15 09:13:42 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 15 01:10:59 2015
Response via : Initial Calibration

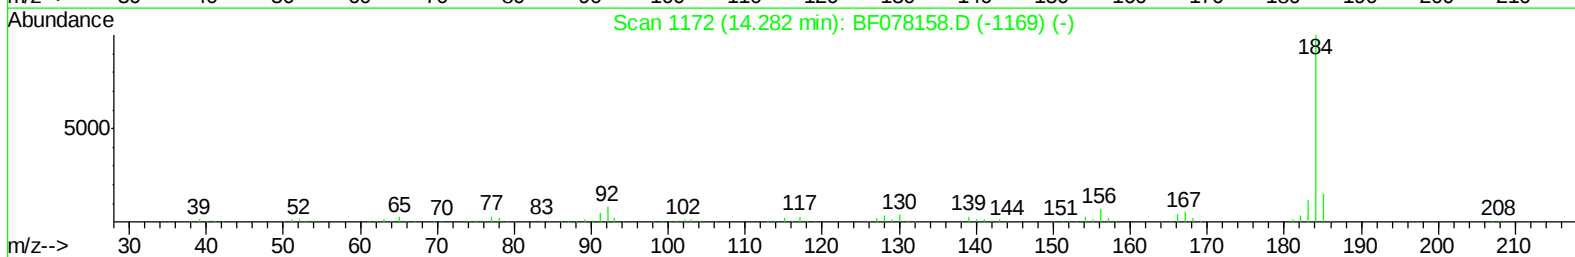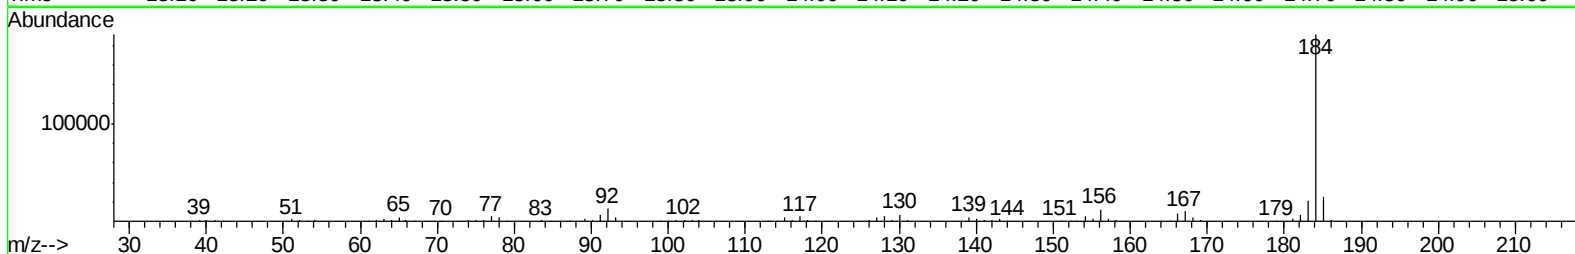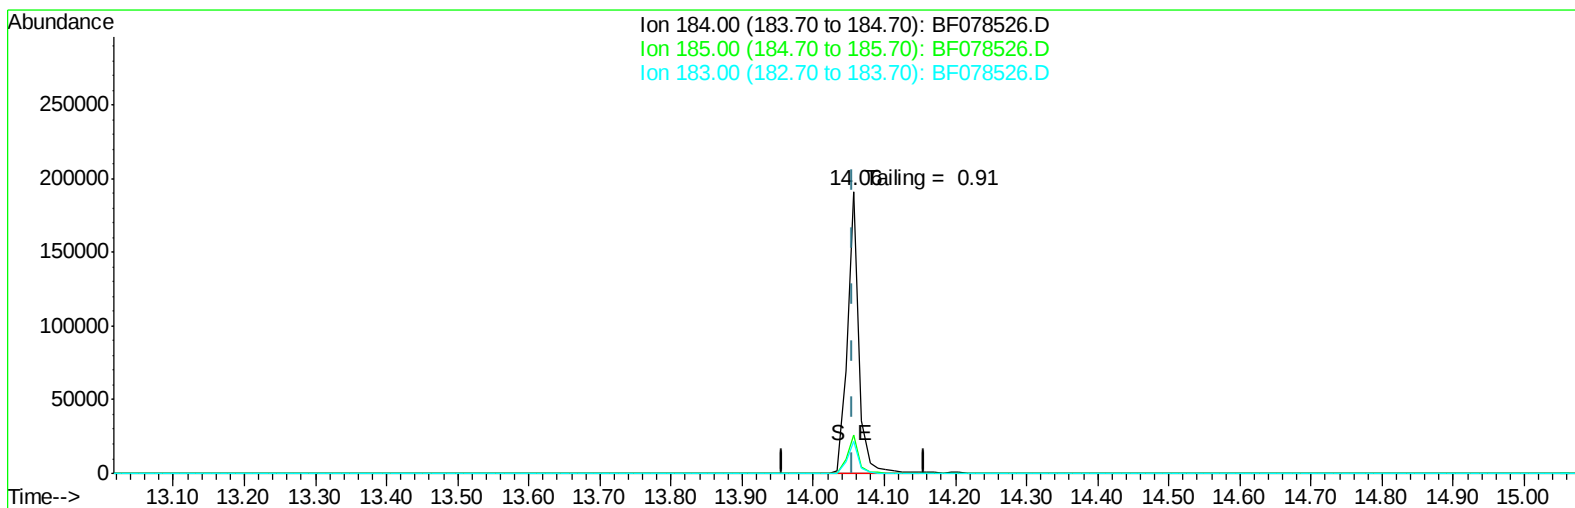

TIC: BF078526.D

(76) Benzidine

14.057min (-0.000) 11509.21ng

response 209175

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	13.45
183.00	11.90	11.22
0.00	0.00	0.00