


Data Path : Z:\HPCHEM1\BNA F\Data\BF041417\
 Data File : BF094428.D
 Acq On : 14 Apr 2017 14:55
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 14 16:39:08 2017

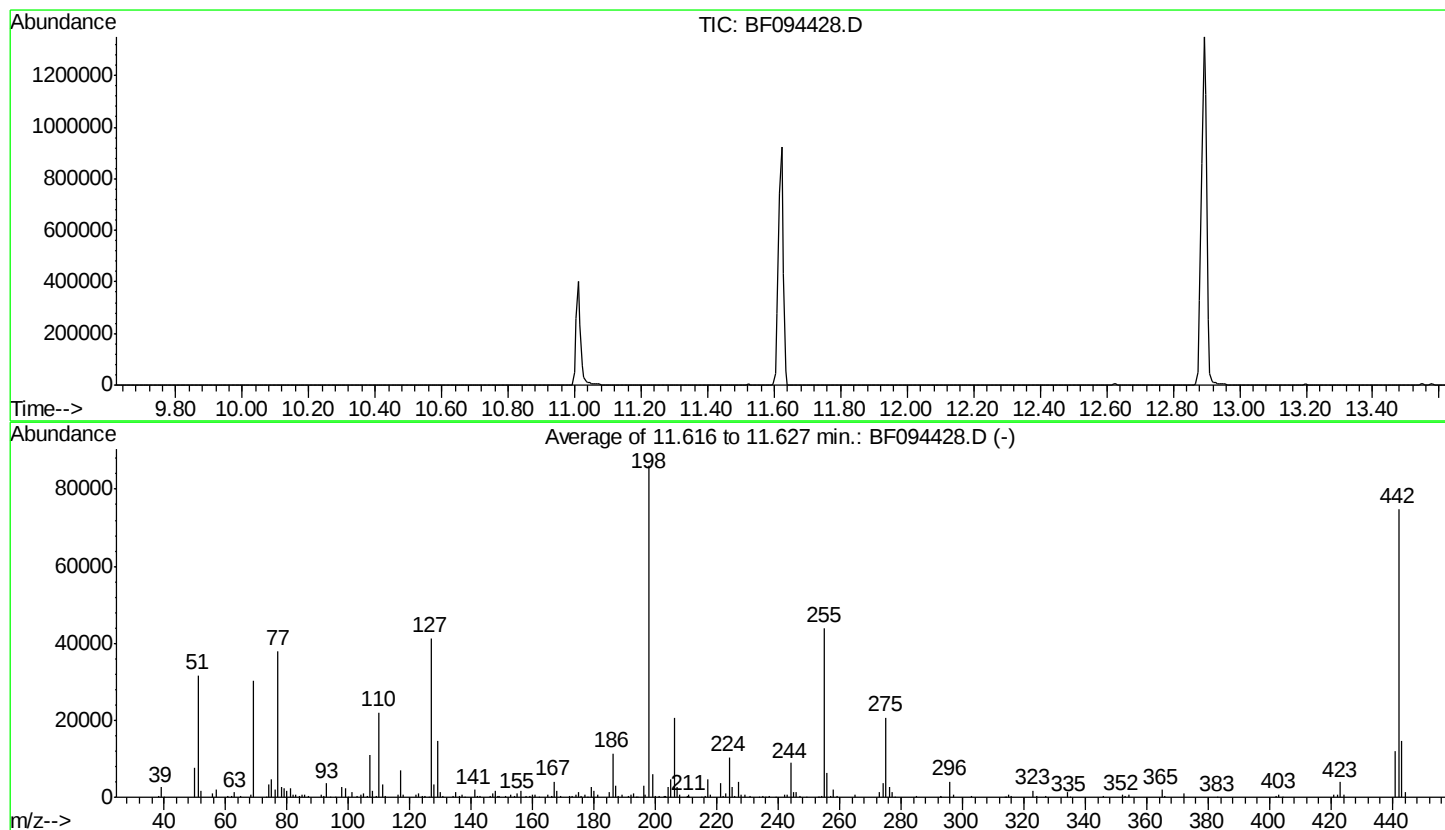

AutoFind: Scans 1654, 1655, 1656; Background Corrected with Scan 1648

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	31682	PASS
68	69	0.00	2	1.7	525	PASS
69	198	0.00	100	35.3	30386	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.0	41389	PASS
197	198	0.00	2	0.8	648	PASS
198	198	100	100	100.0	86141	PASS
199	198	5	9	6.9	5921	PASS
275	198	10	60	24.1	20741	PASS
365	198	1	100	2.2	1902	PASS
441	442	0.01	24	16.2	12139	PASS
442	198	50	100	87.1	74986	PASS
443	442	15	24	19.5	14636	PASS