


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041422\
 Data File : BF127790.D
 Acq On : 14 Apr 2022 09:44
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 13 16:40:15 2022

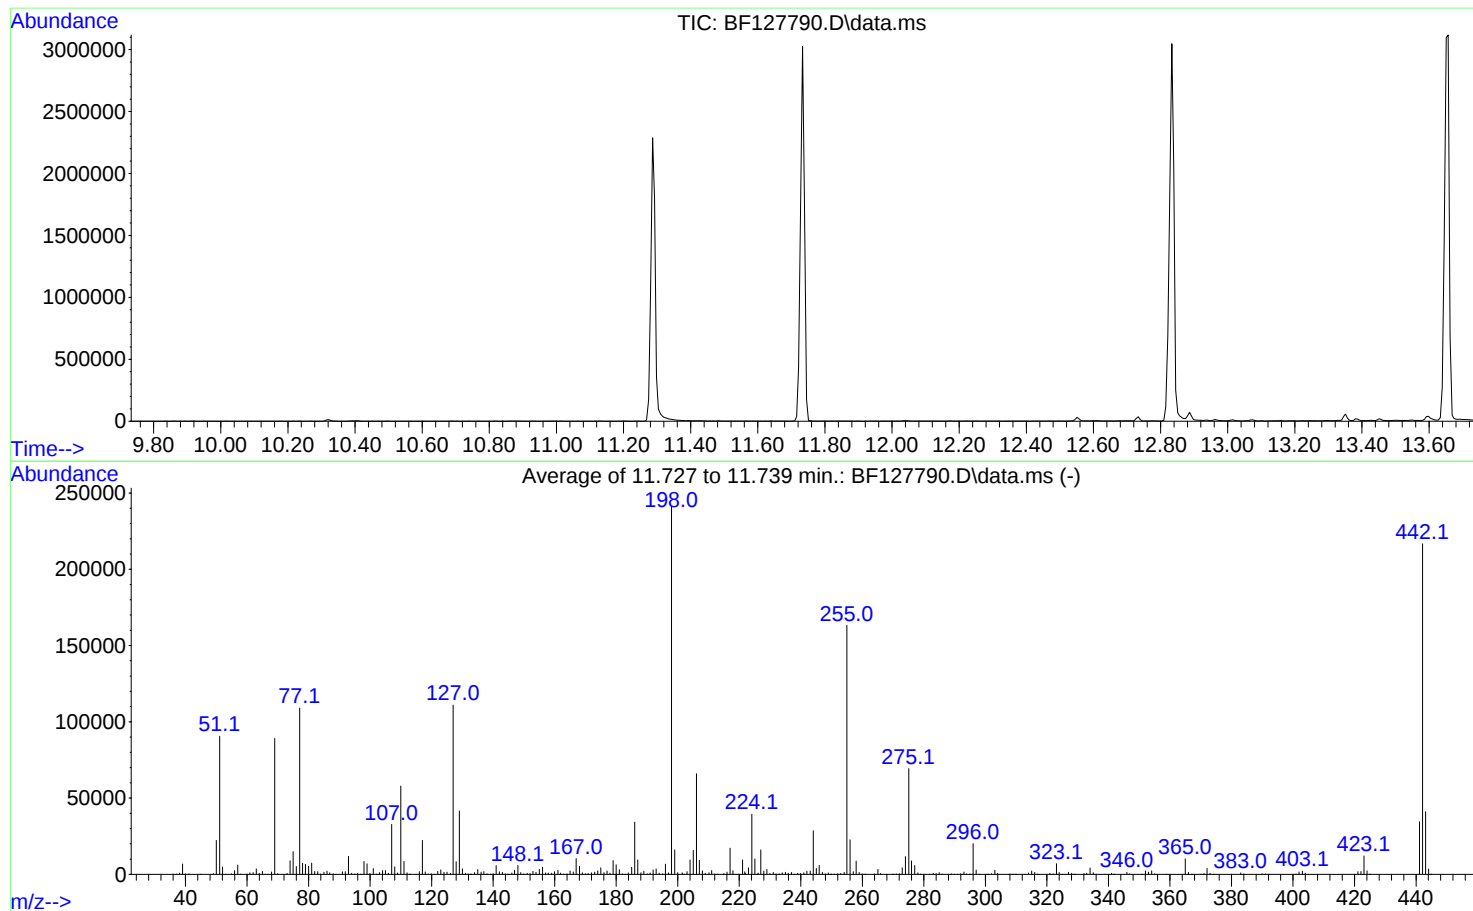




AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	90563	PASS
68	69	0.00	2	1.8	1573	PASS
69	198	0.00	100	36.9	89077	PASS
70	69	0.00	2	0.5	488	PASS
127	198	10	80	46.0	110968	PASS
197	198	0.00	2	0.4	906	PASS
198	198	100	100	100.0	241152	PASS
199	198	5	9	6.7	16045	PASS
275	198	10	60	28.8	69339	PASS
365	198	1	100	4.2	10212	PASS
441	198	0.01	100	14.3	34552	PASS
442	442	50	100	100.0	216744	PASS
443	442	15	24	18.9	41029	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041422\
Data File : BF127790.D
Acq On : 14 Apr 2022 09:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 15 05:48:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 16:40:15 2022
Response via : Initial Calibration

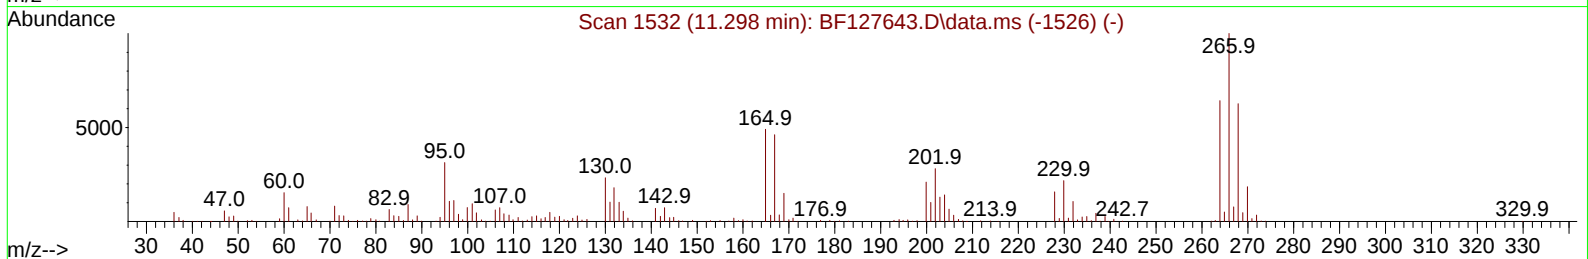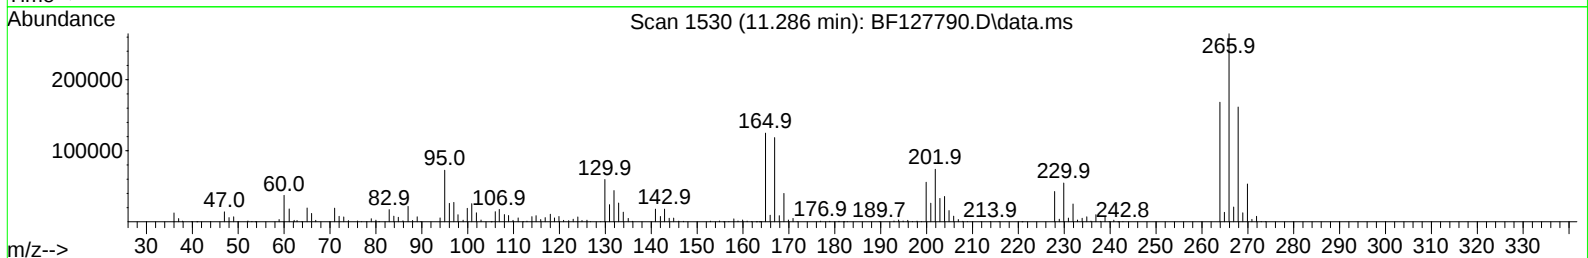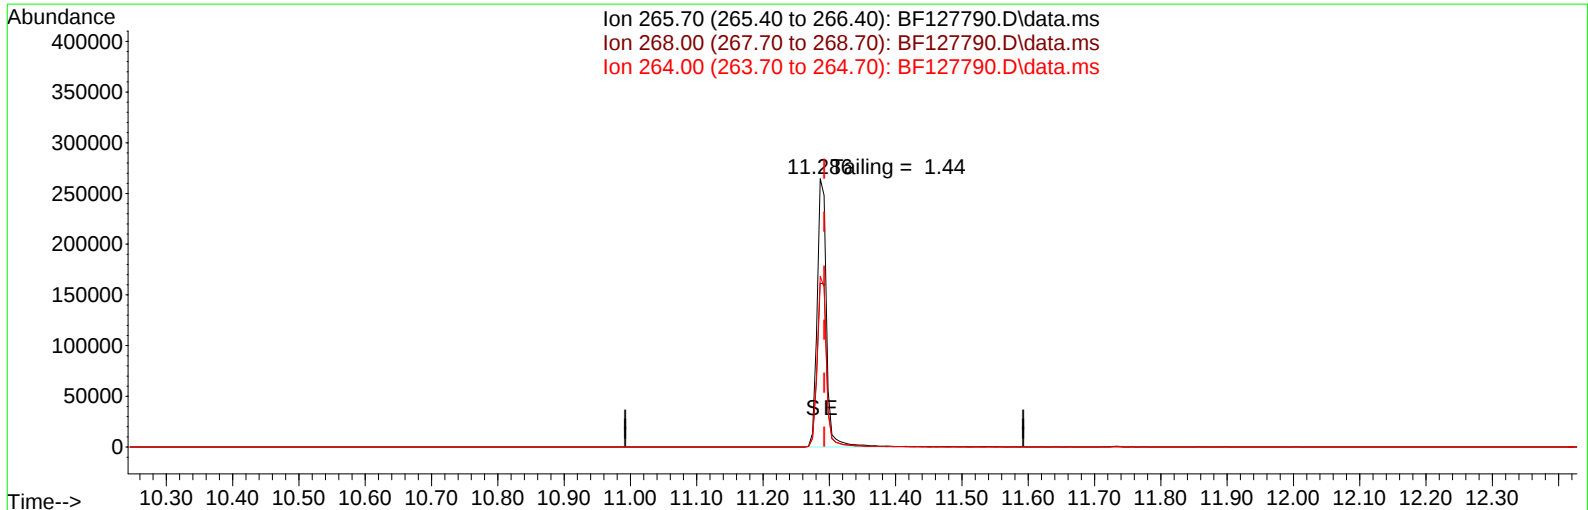

TIC: BF127790.D\data.ms

(70) Pentachlorophenol (C)

11.286min (-0.006) 624396.39 ng




response 262219

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	61.09
264.00	60.60	63.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041422\
Data File : BF127790.D
Acq On : 14 Apr 2022 09:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 15 05:48:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 16:40:15 2022
Response via : Initial Calibration

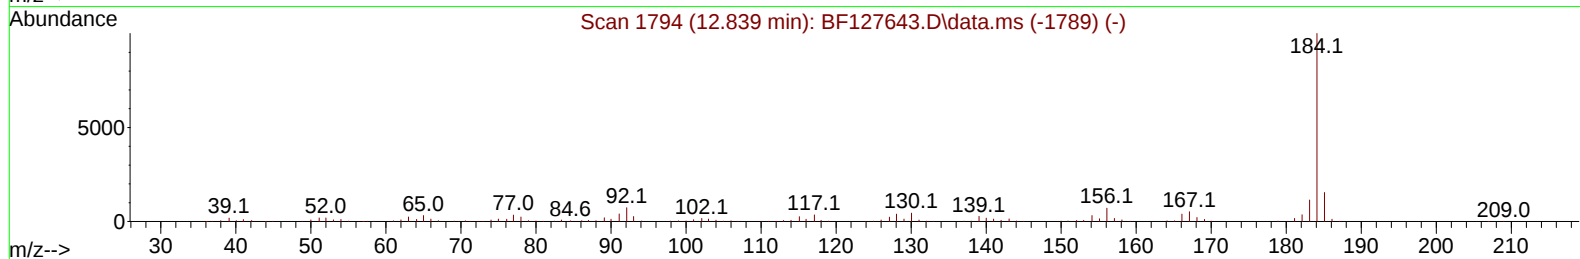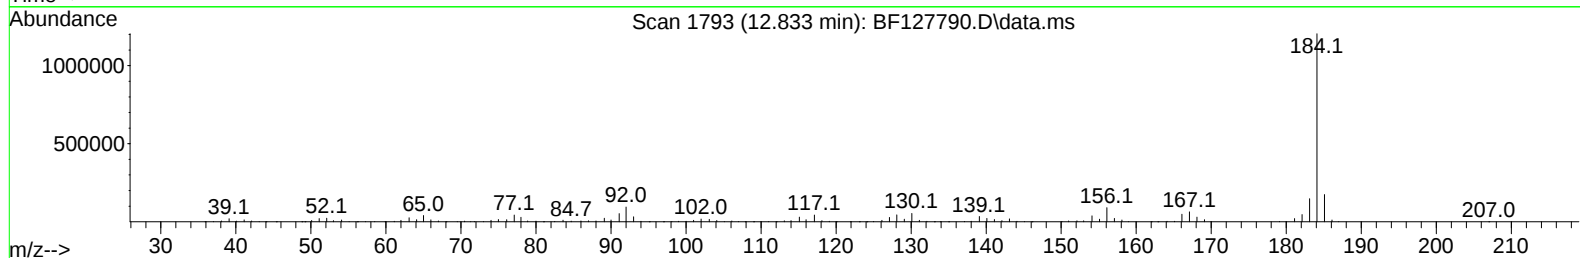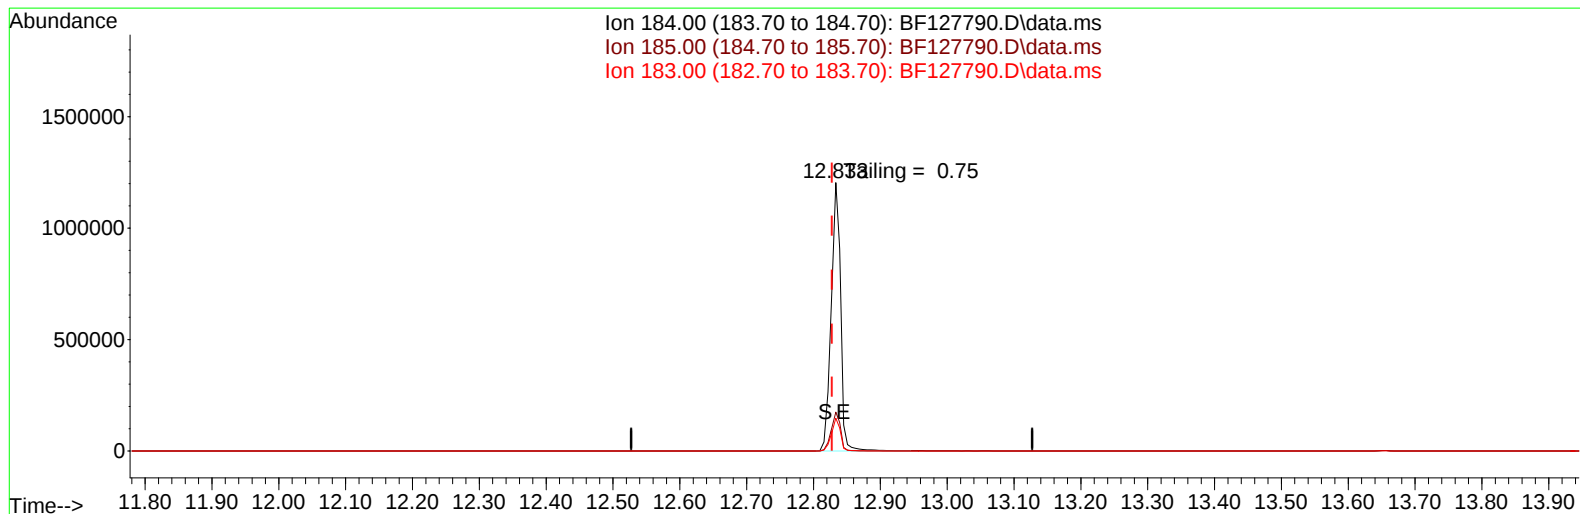

TIC: BF127790.D\data.ms

(77) Benzidine

12.833min (+ 0.006) 10024.70 ng

response 1186067

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.50
183.00	11.70	12.27
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/14/2022	BNA_F	<u>BF127790.D</u>
Compound Name	Response	Retention Time
DDT	604034	13.657
DDD	11712	13.351
DDE	1214	13.016
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12926	616960	2.10

Instrument :
BNA_F
ClientSampleId :
DFTPP