
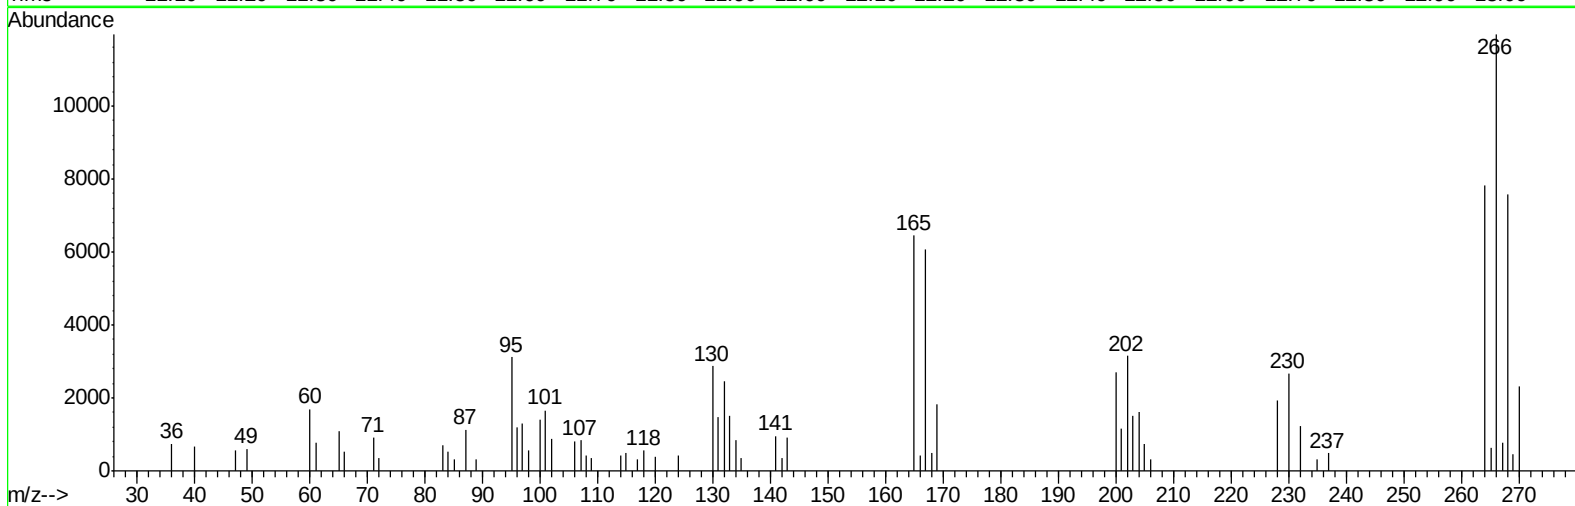


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041515\
Data File : BF078540.D
Acq On : 15 Apr 2015 17:09
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 07:15:35 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 16 01:25:24 2015
Response via : Initial Calibration

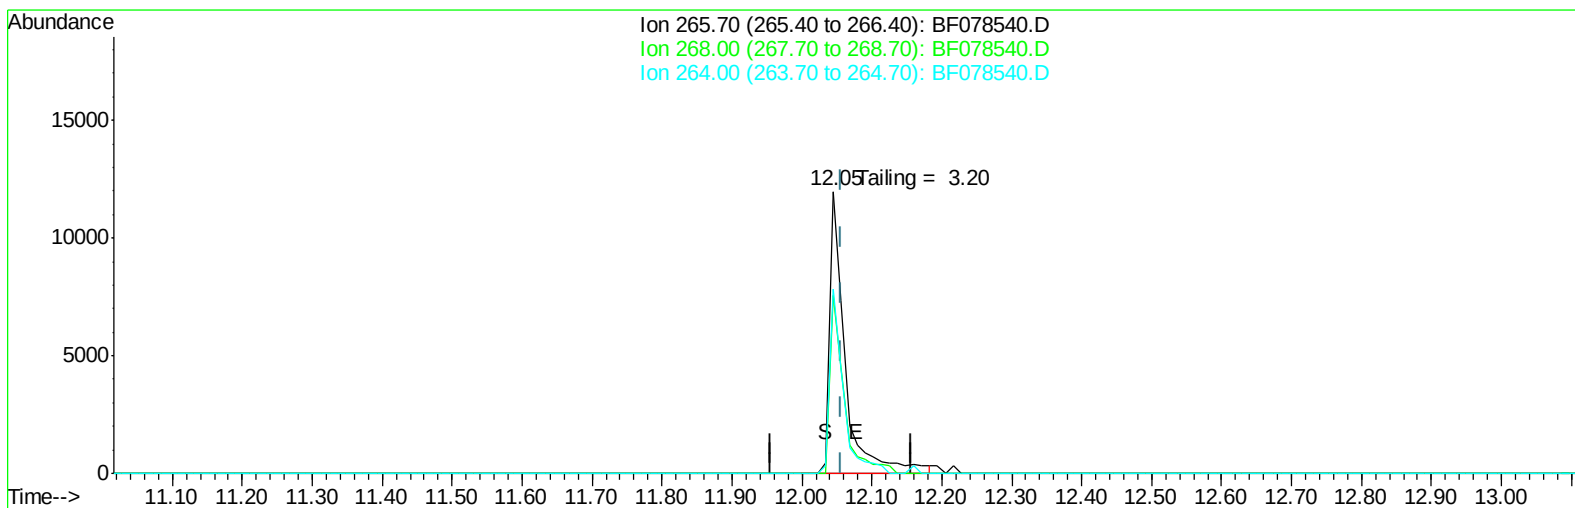

TIC: BF078540.D

(69) Pentachlorophenol (C)



12.045min (-0.011) 0.00ng

response 17195

Ion	Exp%	Act%
265.70	100	100
268.00	62.60	63.41
264.00	62.50	65.41
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041515\
Data File : BF078540.D
Acq On : 15 Apr 2015 17:09
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 07:15:35 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 16 01:25:24 2015
Response via : Initial Calibration

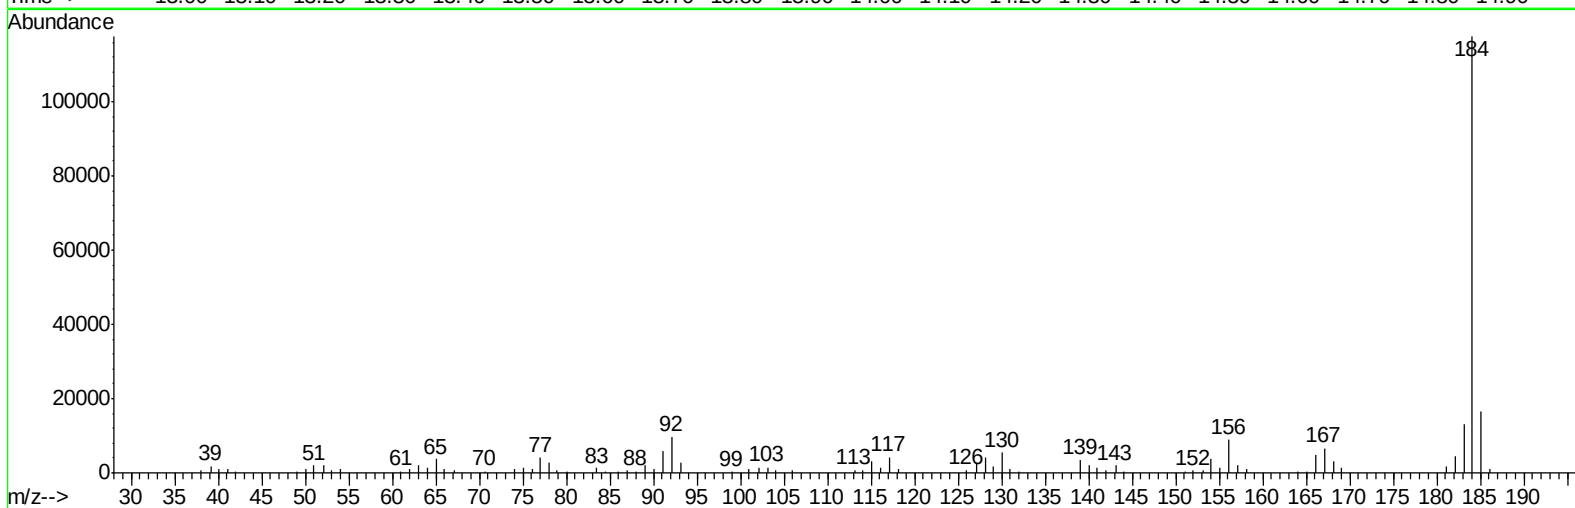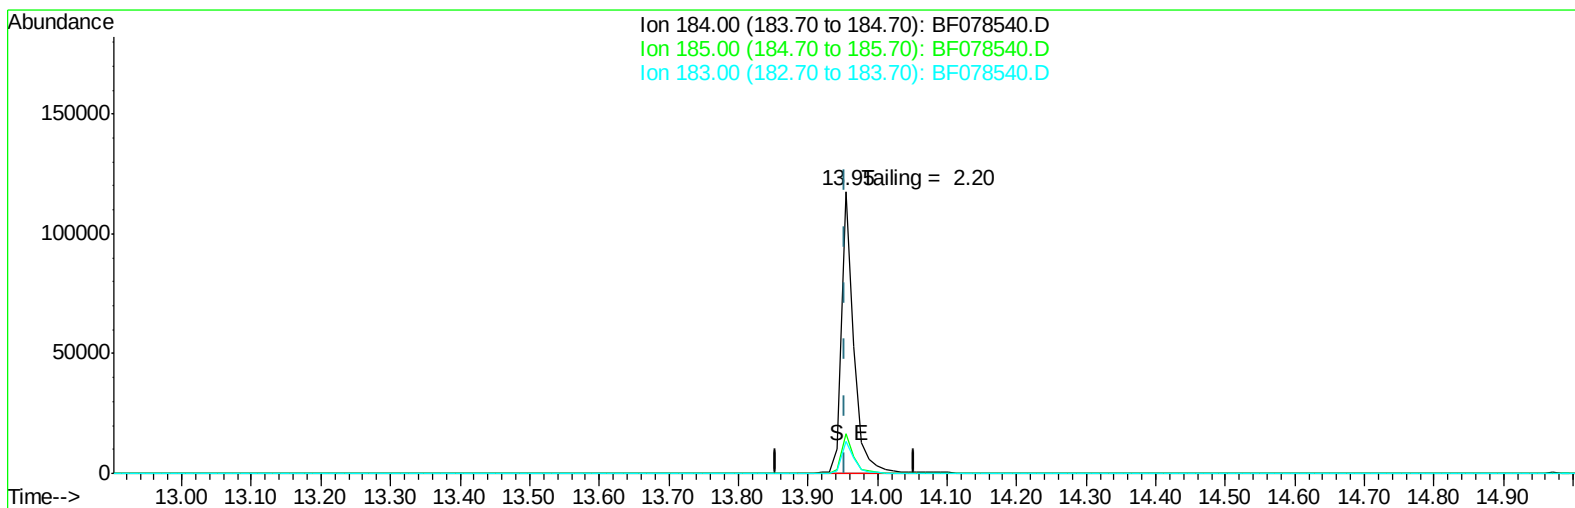

TIC: BF078540.D

(76) Benzidine

13.954min (0.000) 0.00ng

response 140693

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.22
183.00	11.90	11.24
0.00	0.00	0.00