

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041515\
 Data File : BF078557.D
 Acq On : 16 Apr 2015 1:40
 Operator : TP/IZ
 Sample : G1854-02 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 LS-SB11B(9.5-10)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.461	23	24	30	rVB	17500	30597	1.82%	0.684%
2	1.541	30	31	62	rVB	881478	1679814	100.00%	37.571%
3	4.947	327	329	338	rVB	72227	94219	5.61%	2.107%
4	6.319	447	449	456	rVB	105032	108469	6.46%	2.426%
5	6.422	456	458	461	rBV	113663	113590	6.76%	2.541%
6	6.707	481	483	486	rBV	192691	188231	11.21%	4.210%
7	6.890	497	499	502	rBV	74748	89925	5.35%	2.011%
8	7.416	543	545	550	rVB	64374	58947	3.51%	1.318%
9	8.296	619	622	624	rBV	228357	264643	15.75%	5.919%
10	9.645	738	740	742	rBV	152121	129852	7.73%	2.904%
11	10.445	808	810	813	rVB	238125	307212	18.29%	6.871%
12	11.428	894	896	898	rBB	50219	52359	3.12%	1.171%
13	12.274	968	970	972	rBV	325823	315408	18.78%	7.054%
14	14.034	1122	1124	1126	rBV	20693	19431	1.16%	0.435%
15	14.148	1132	1134	1137	rBV	27725	28435	1.69%	0.636%
16	14.262	1141	1144	1146	rBV	101043	96649	5.75%	2.162%
17	15.463	1246	1249	1252	rBV4	9049	17413	1.04%	0.389%
18	15.520	1252	1254	1256	rVV	310936	379061	22.57%	8.478%
19	16.766	1360	1363	1368	rBV	22637	58333	3.47%	1.305%
20	17.063	1387	1389	1391	rBV	12679	21569	1.28%	0.482%
21	17.120	1391	1394	1396	rVV	19255	29455	1.75%	0.659%
22	17.177	1396	1399	1402	rBV	328443	387429	23.06%	8.665%


Sum of corrected areas: 4471041

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041515\
Data File : BF078557.D
Acq On : 16 Apr 2015 1:40
Operator : TP/IZ
Sample : G1854-02 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LS-SB11B(9.5-10)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

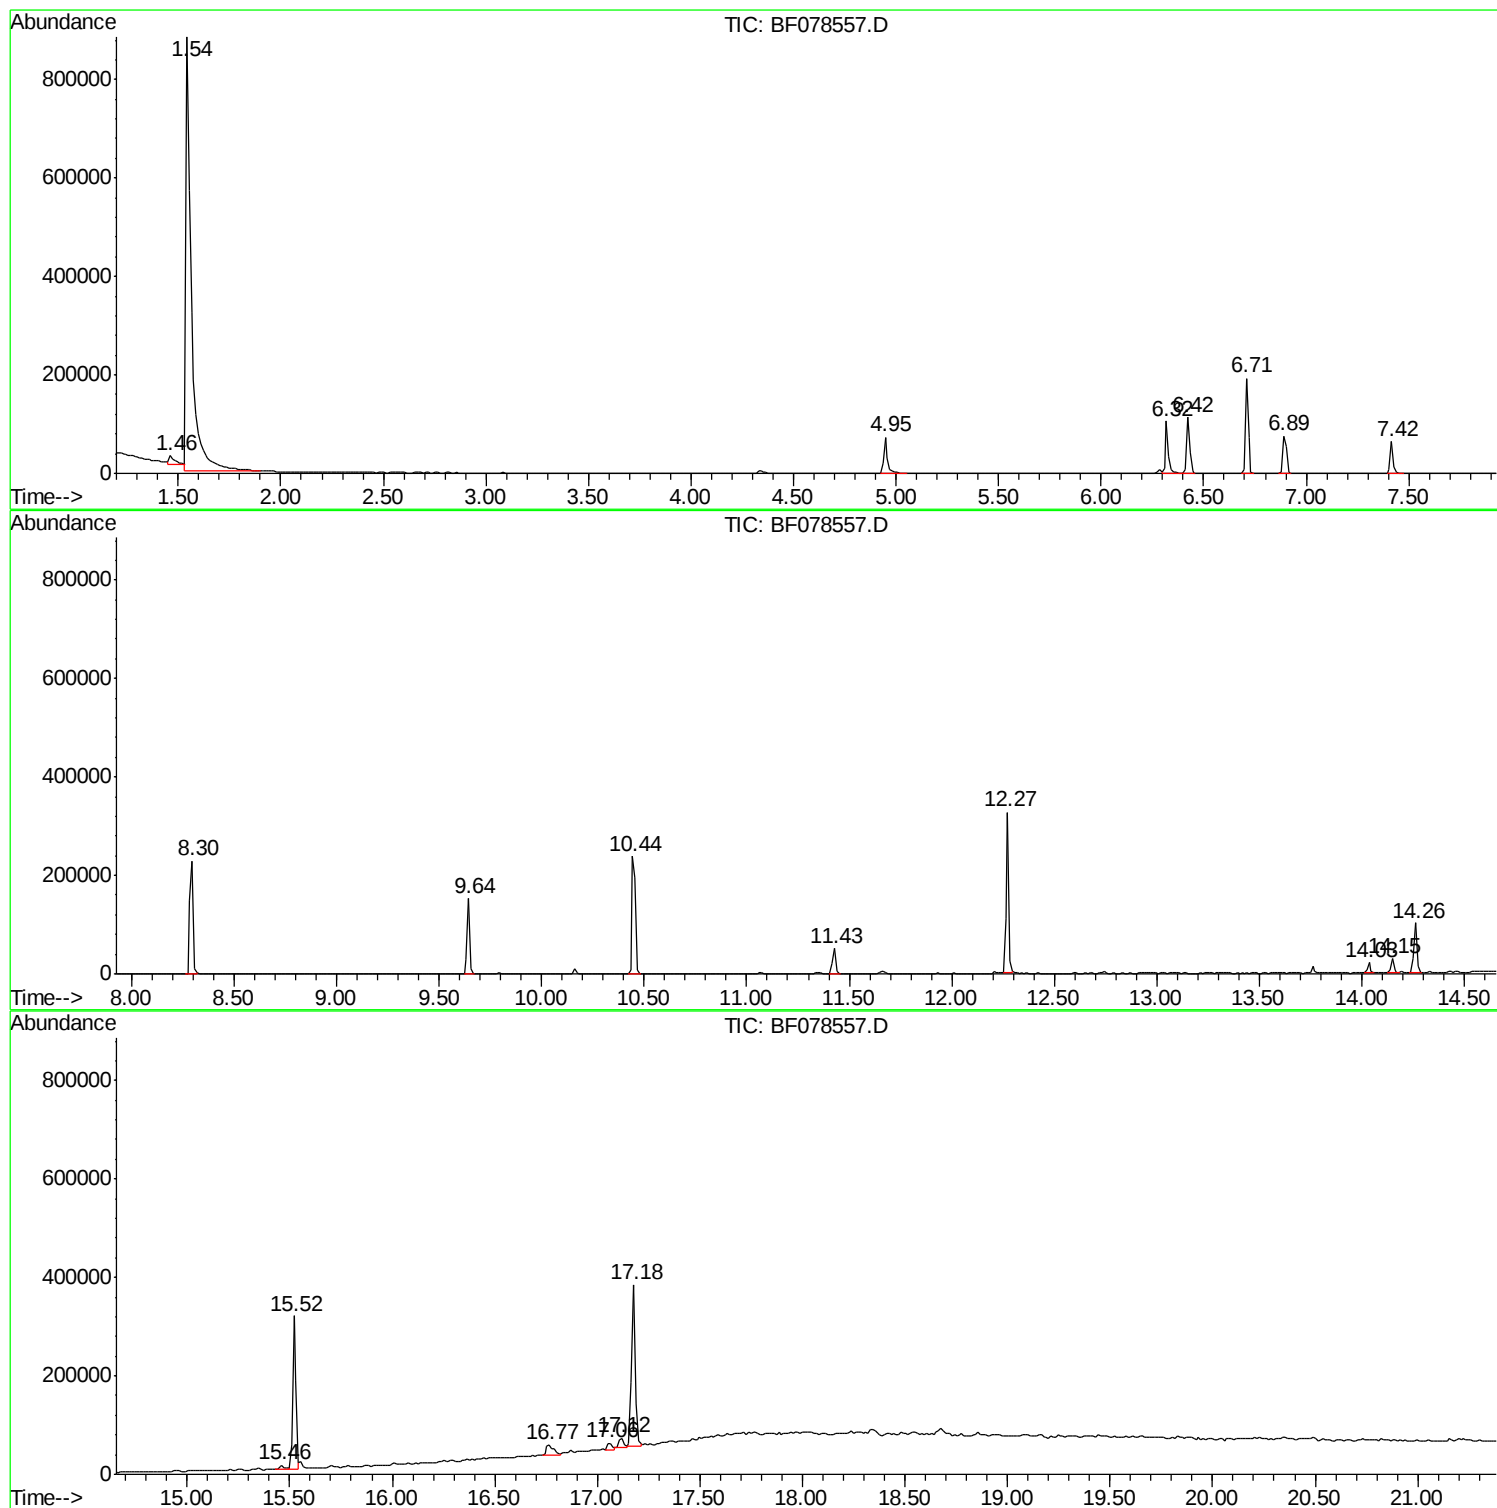

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041515\
Data File : BF078557.D
Acq On : 16 Apr 2015 1:40
Operator : TP/IZ
Sample : G1854-02 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LS-SB11B(9.5-10)










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 unknown6.42 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.42	12.07 ng	113590	1,4-Dichlorobenzene-d4	6.71

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3		5-Aminoindole	132	C8H8N2	005192-03-0	10
4		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
5		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9

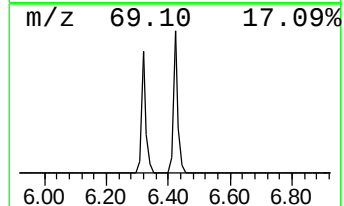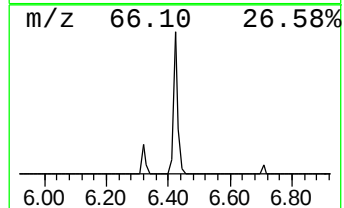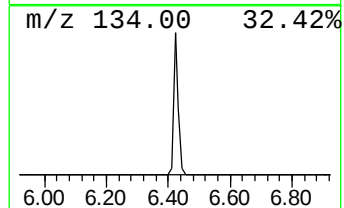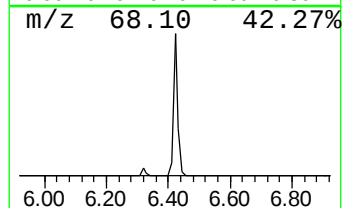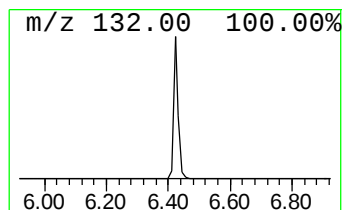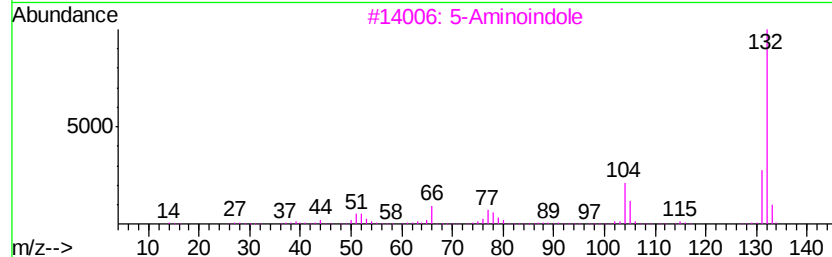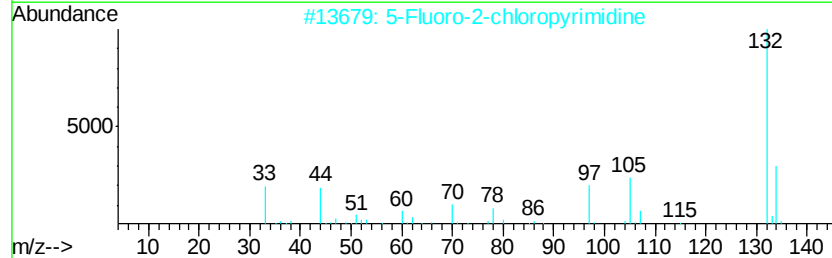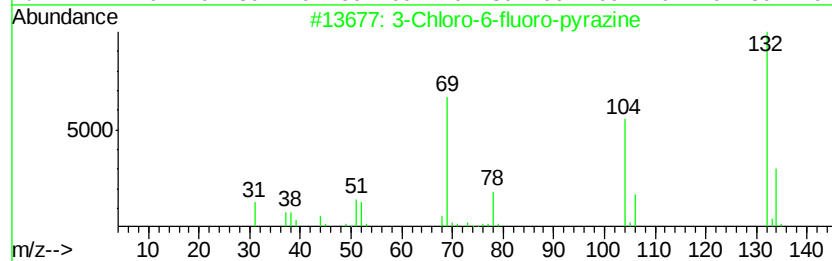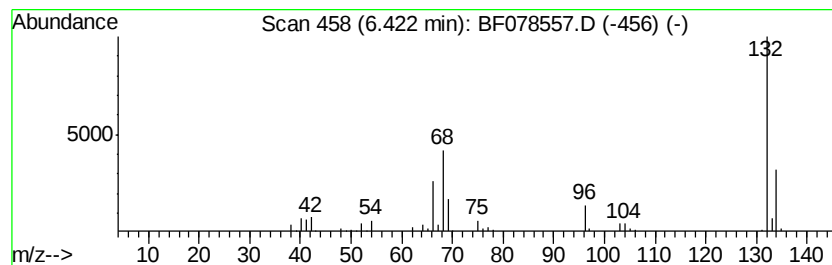

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041515\
Data File : BF078557.D
Acq On : 16 Apr 2015 1:40
Operator : TP/IZ
Sample : G1854-02 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LS-SB11B(9.5-10)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.42	6.42	12.1	ng	113590	1	6.71	188231	20.0