


Data Path : Z:\HPCHEM1\BNA_F\Data\BF041515\
 Data File : BF078540.D
 Acq On : 15 Apr 2015 17:09
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 31 14:58:34 2015

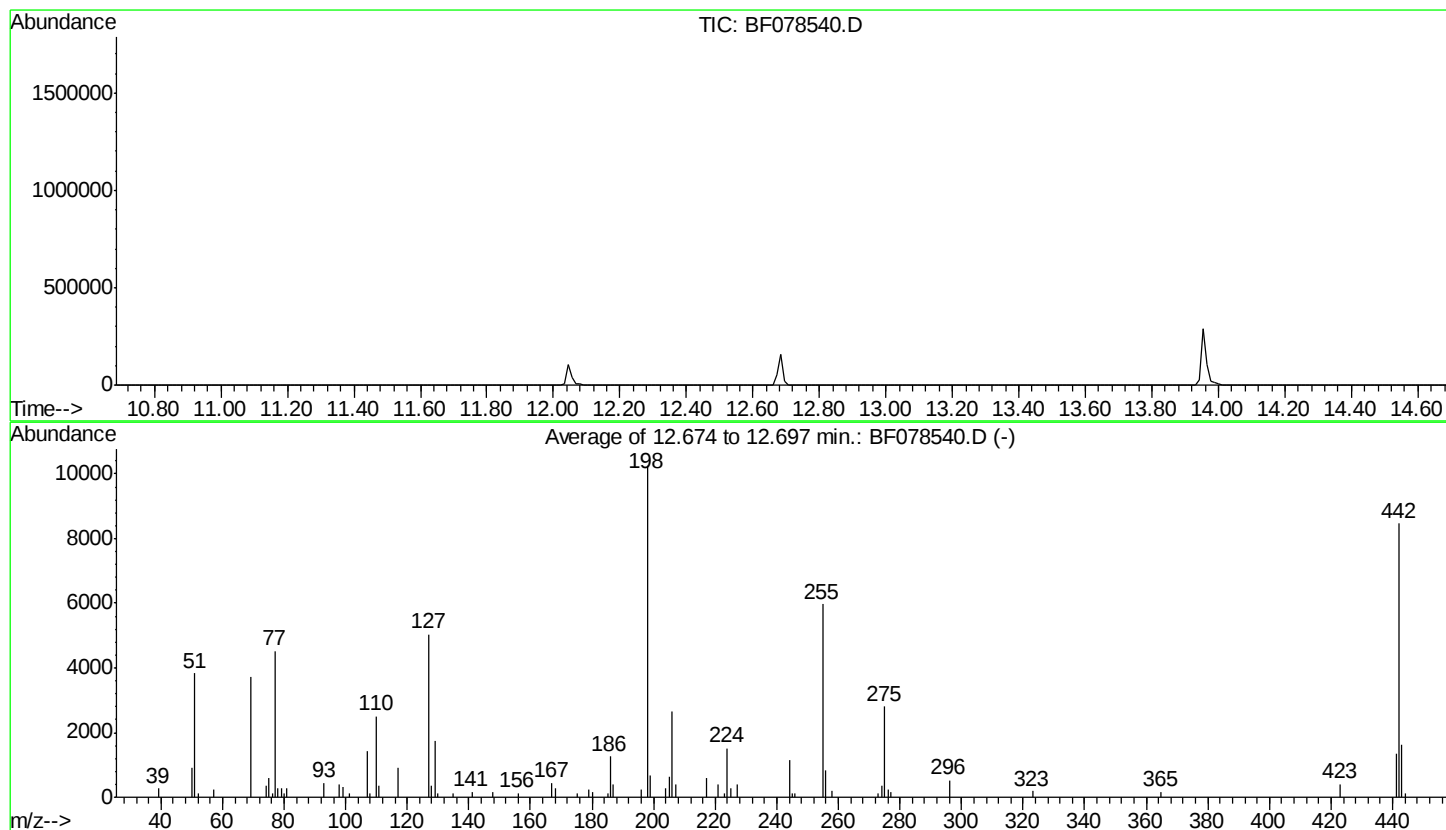

AutoFind: Scans 1005, 1006, 1007; Background Corrected with Scan 1002

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	3823	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.3	3726	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.1	5039	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	10257	PASS
199	198	5	9	6.4	656	PASS
275	198	10	60	27.3	2802	PASS
365	198	1	100	1.7	176	PASS
441	442	0.01	24	15.9	1348	PASS
442	198	50	100	82.4	8456	PASS
443	442	15	24	19.4	1638	PASS