


Acetophenone

Response Ratio

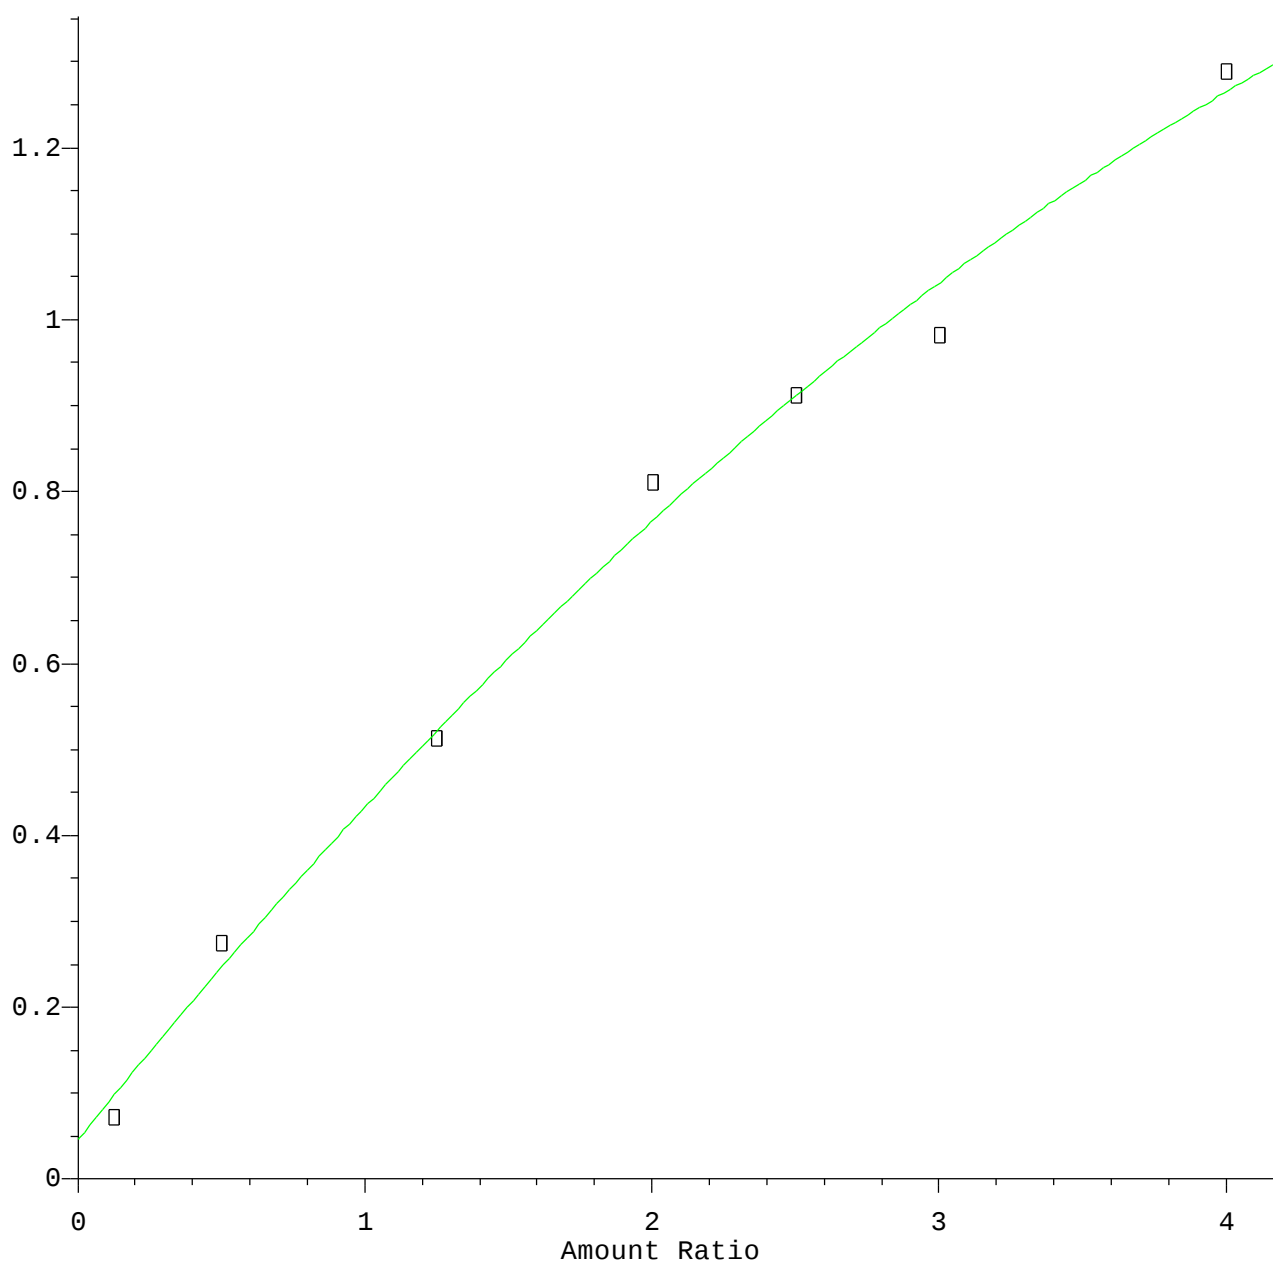


$R = -2.75e-002 A^2 + 4.15e-001 A + 4.58e-002$
Coef of Det (r^2) = 0.993 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF041516.M
Calibration Table Last Updated: Fri Apr 15 15:56:31 2016


1,2,4,5-Tetrachlorobenzene

Response Ratio

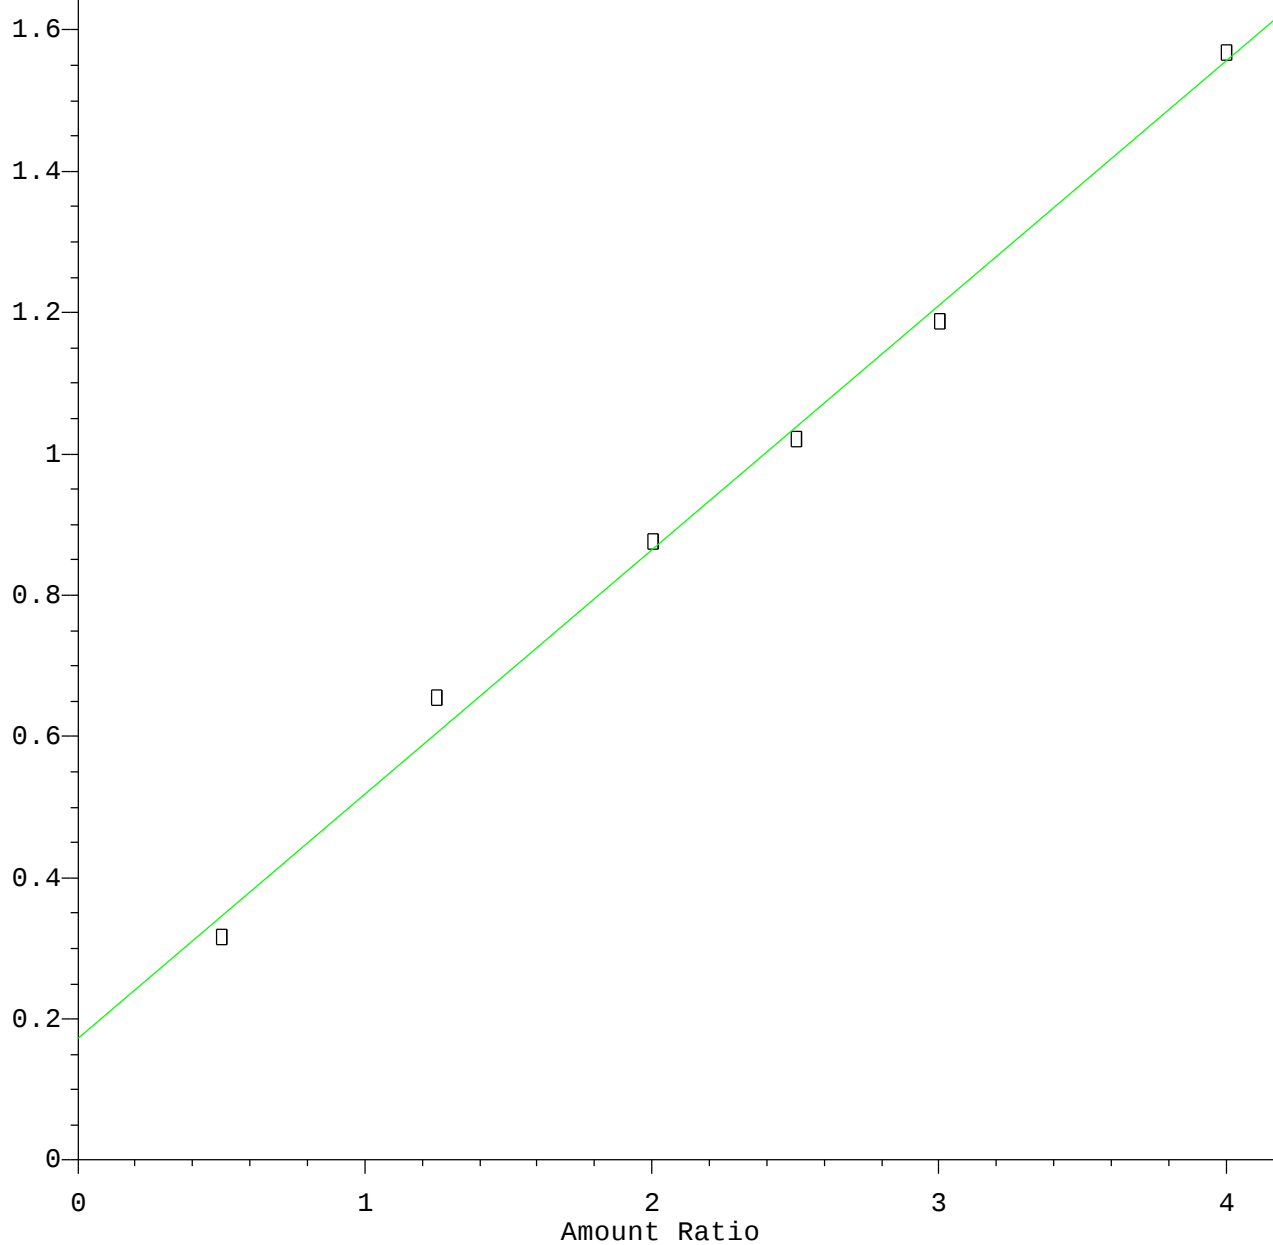


Resp Ratio = $3.46 \times 10^{-1} \times \text{Amt} + 1.72 \times 10^{-1}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF041516.M
Calibration Table Last Updated: Fri Apr 15 15:56:31 2016

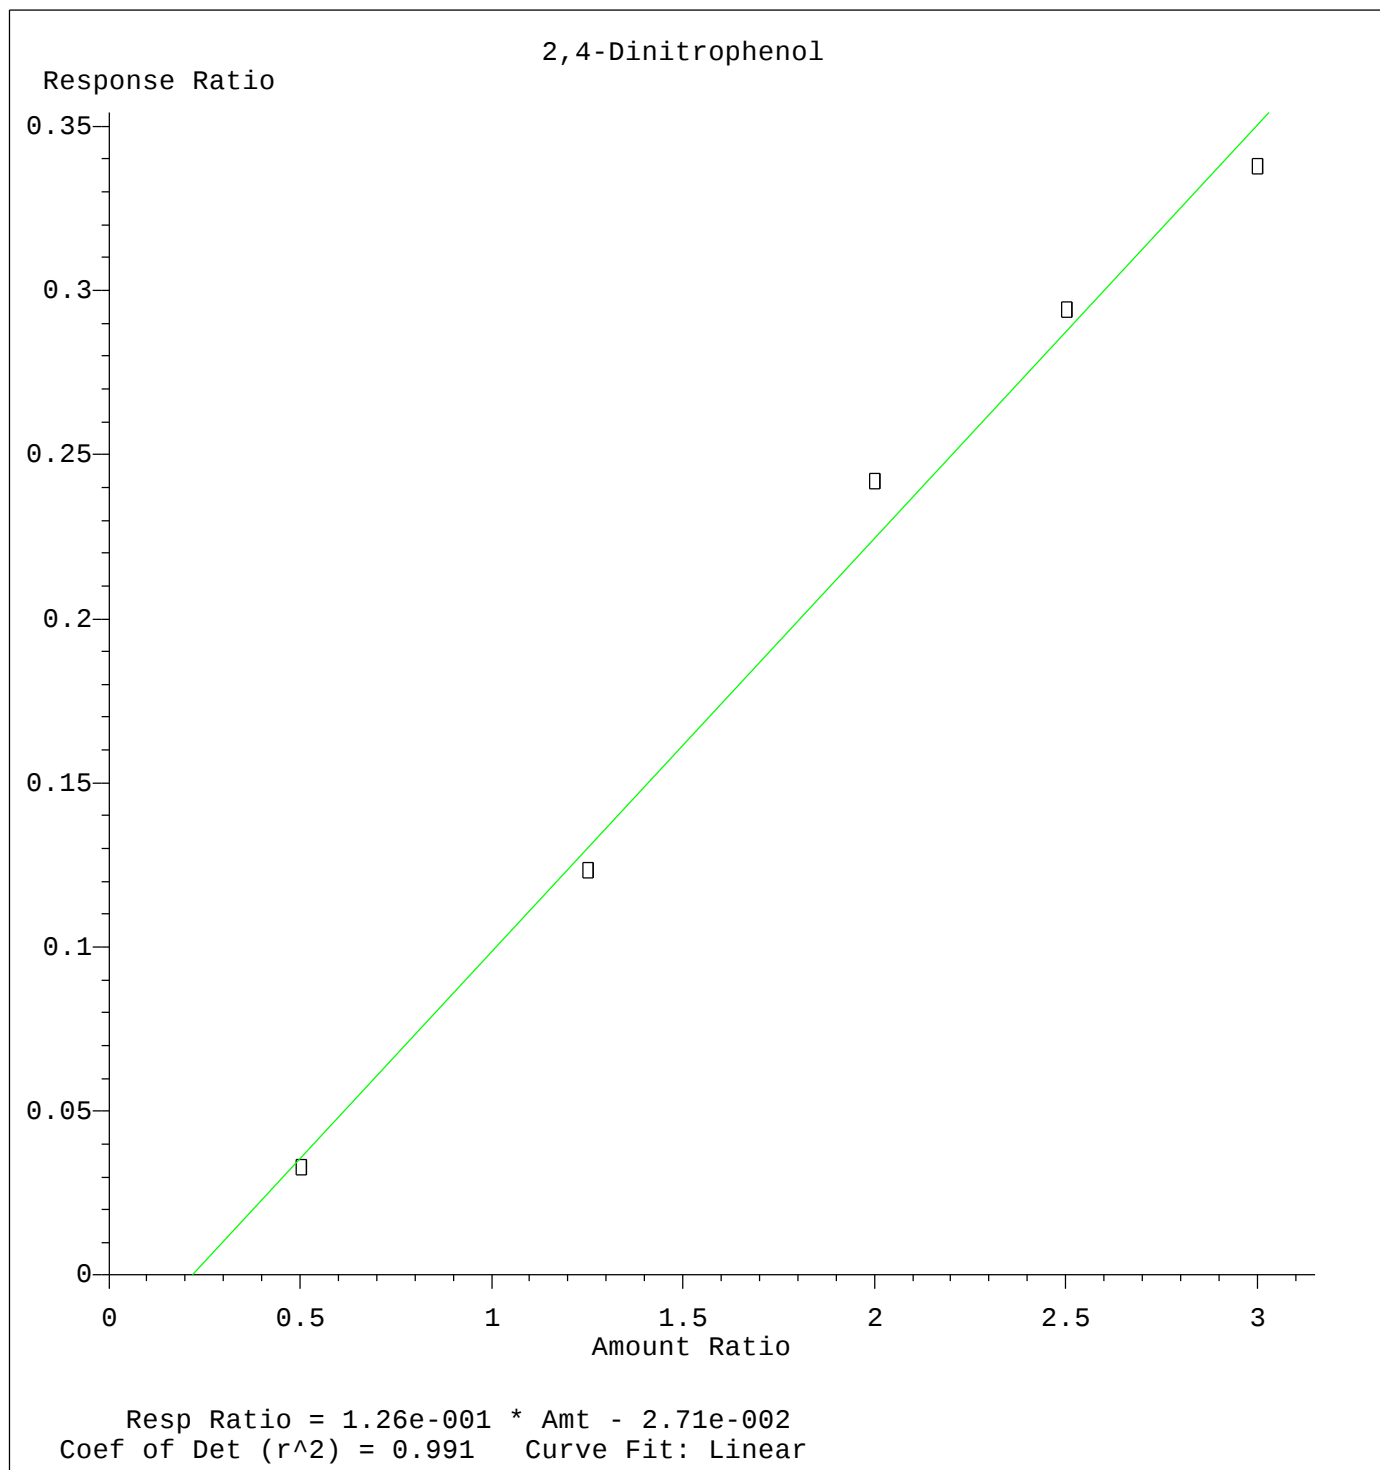


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF041516.M
Calibration Table Last Updated: Fri Apr 15 15:56:31 2016

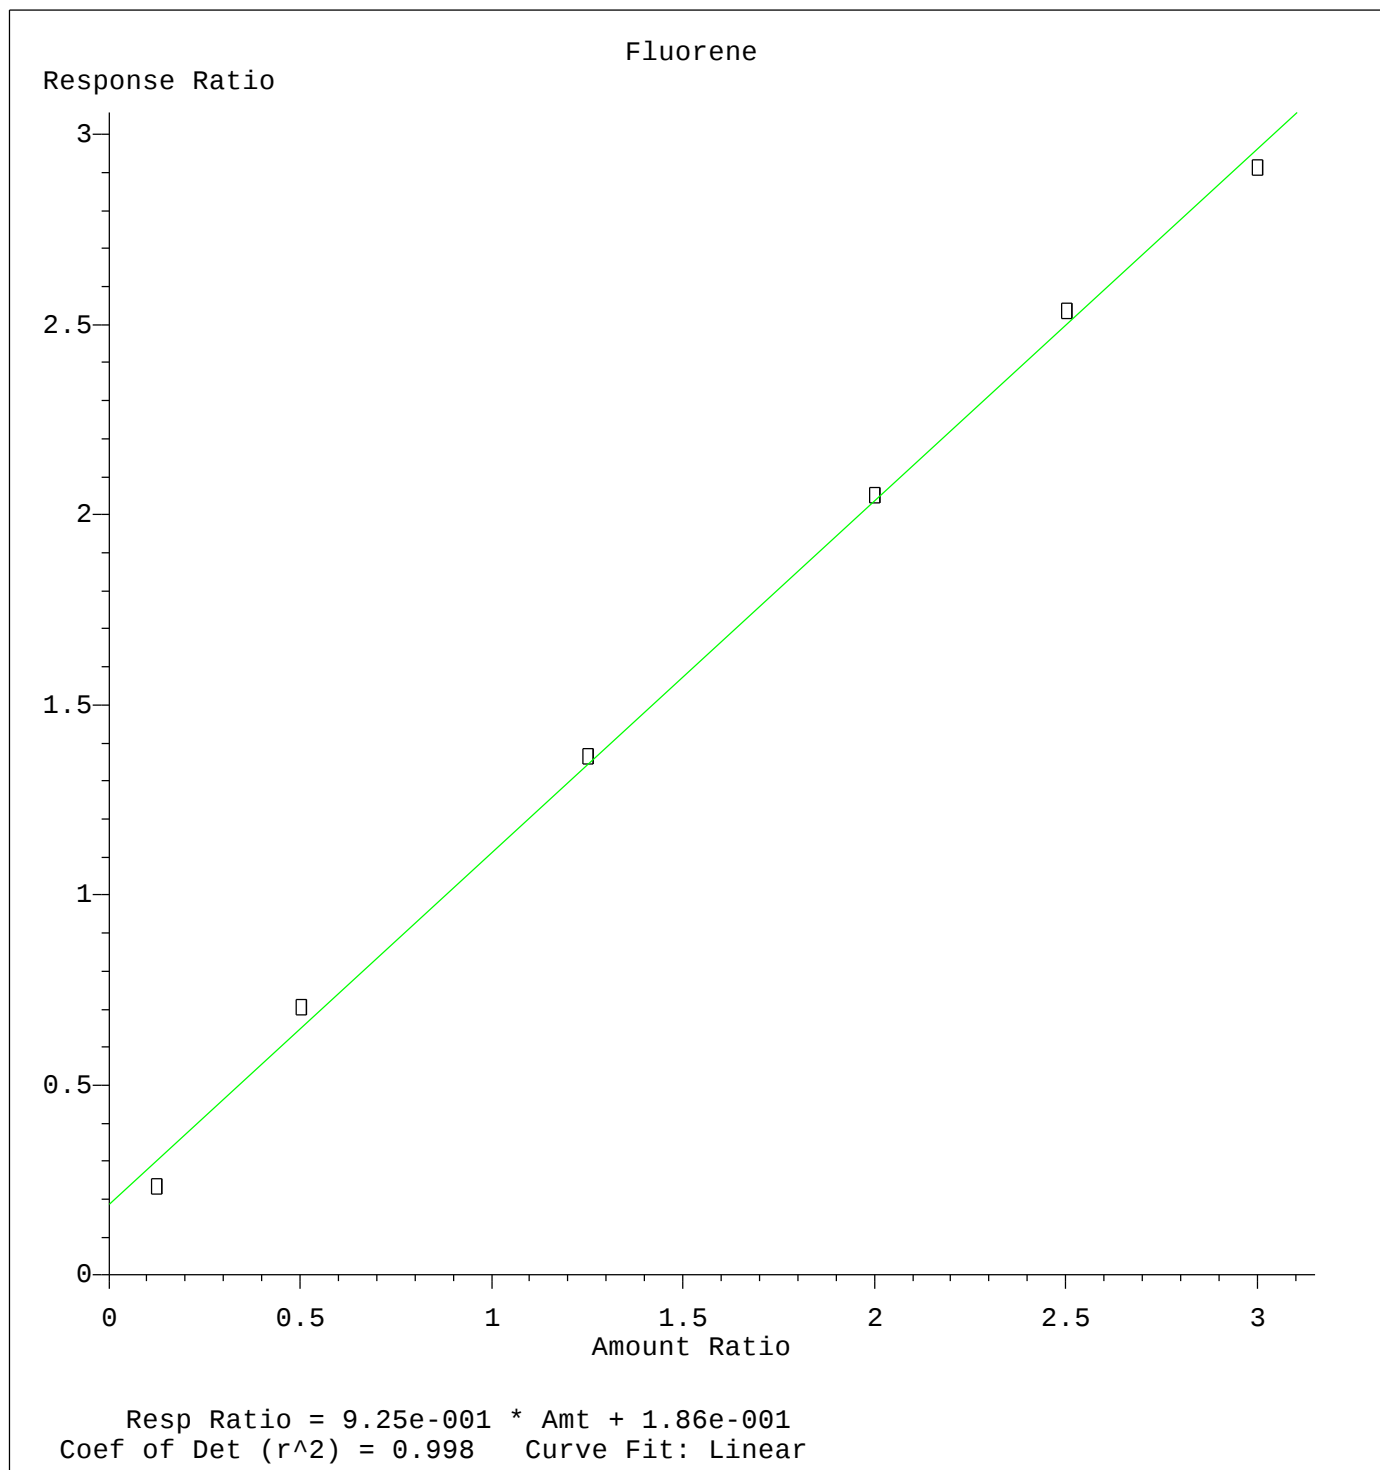

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF041516.M
Calibration Table Last Updated: Fri Apr 15 15:56:31 2016


4-Chlorophenyl-phenylether

Response Ratio

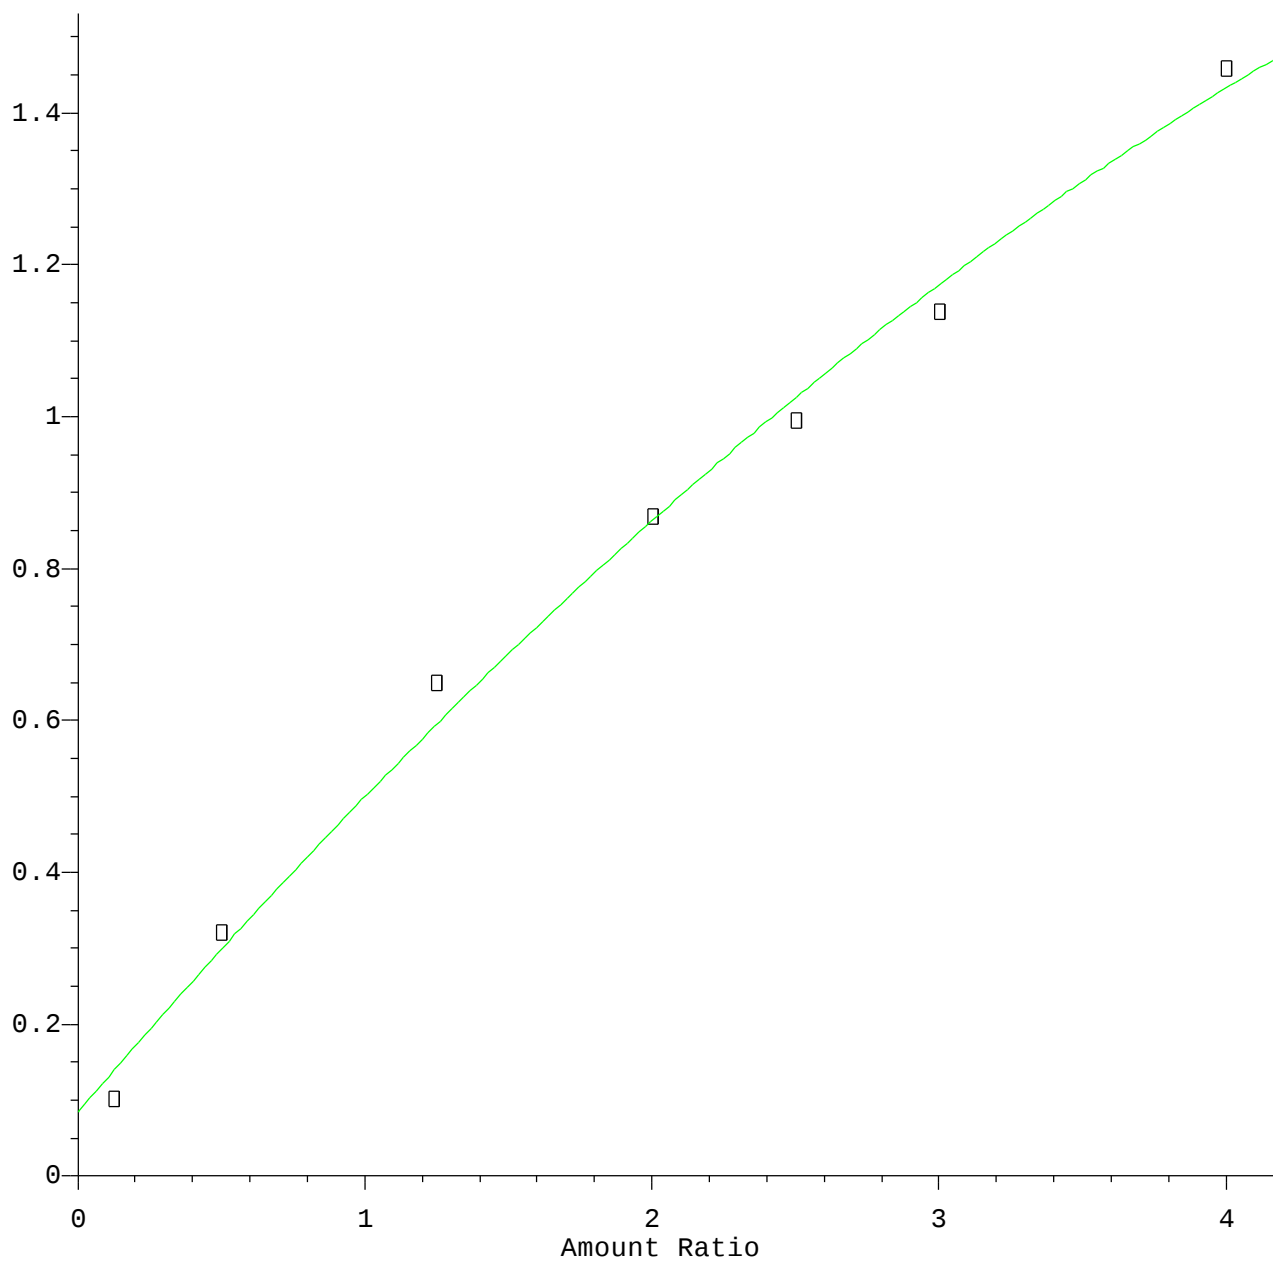


$R = -2.62e-002 A^2 + 4.42e-001 A + 8.43e-002$
Coef of Det (r^2) = 0.994 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF041516.M
Calibration Table Last Updated: Fri Apr 15 15:56:31 2016

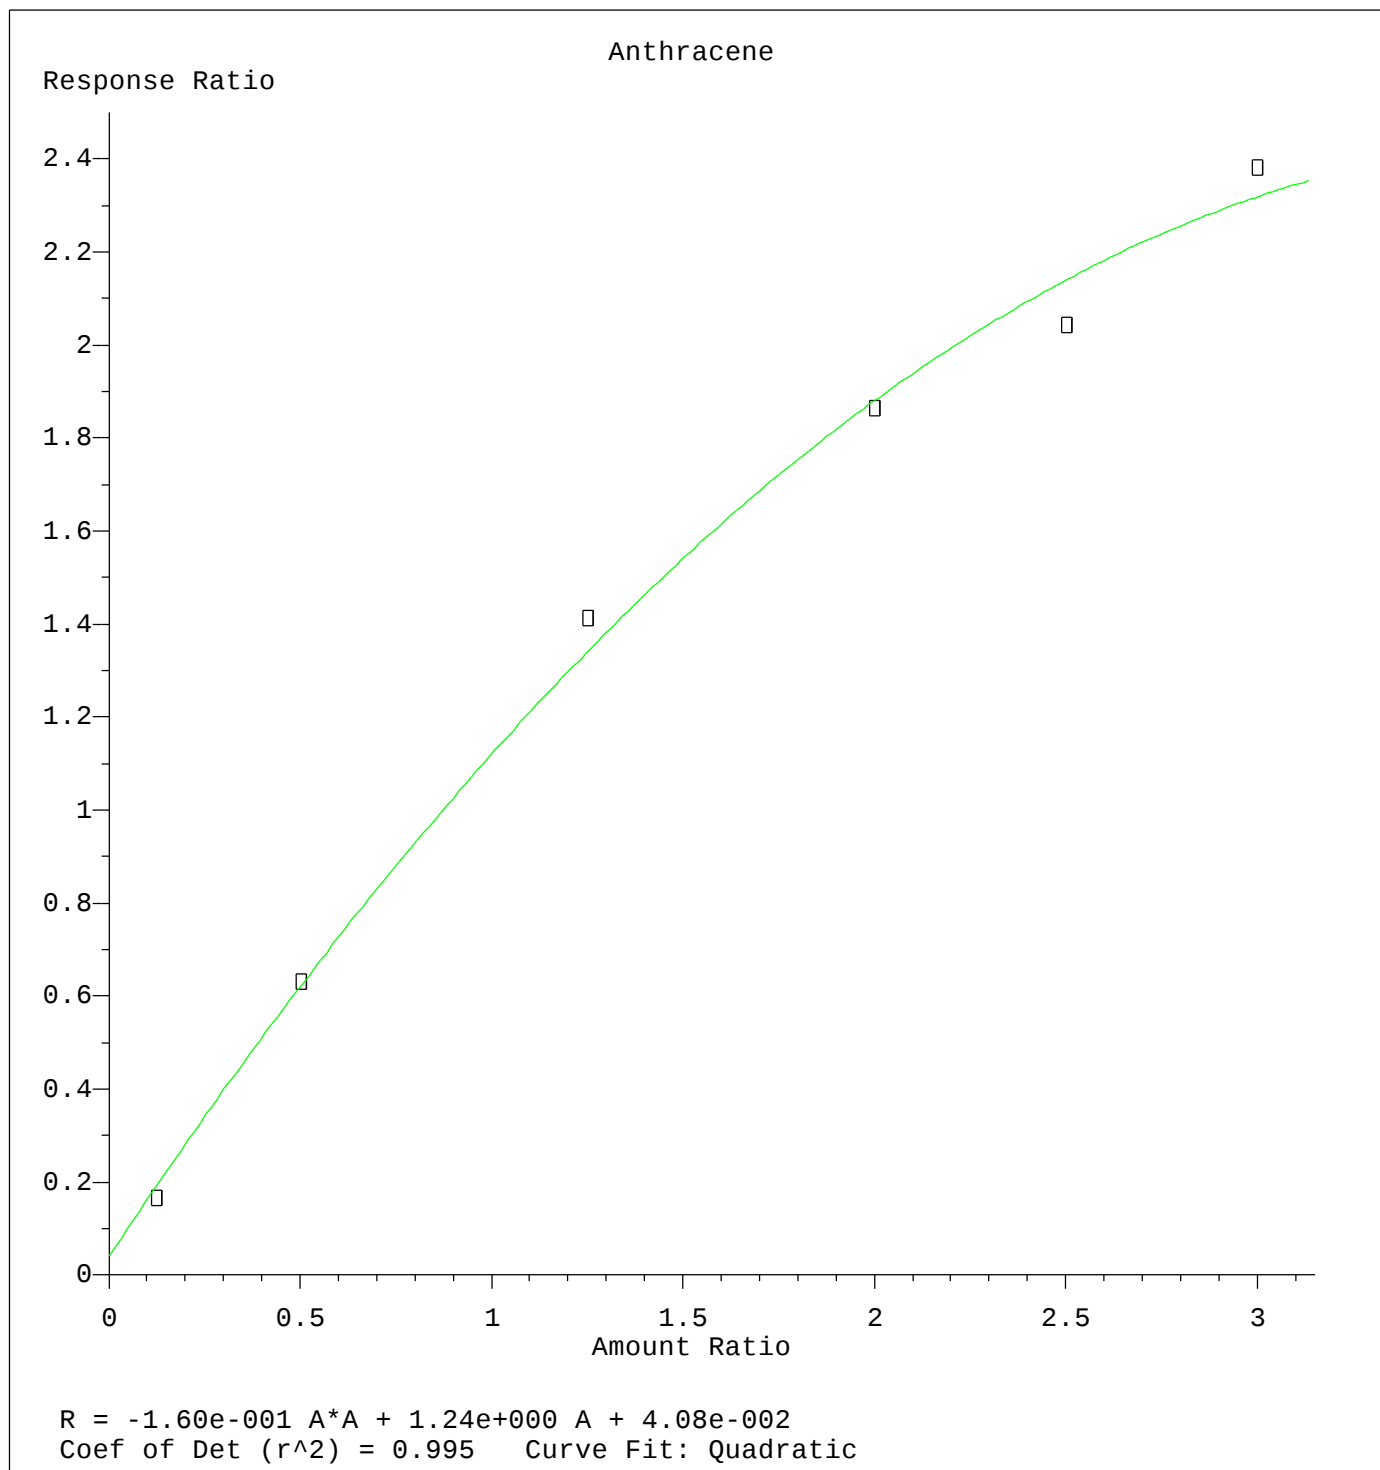

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF041516.M
Calibration Table Last Updated: Fri Apr 15 15:56:31 2016

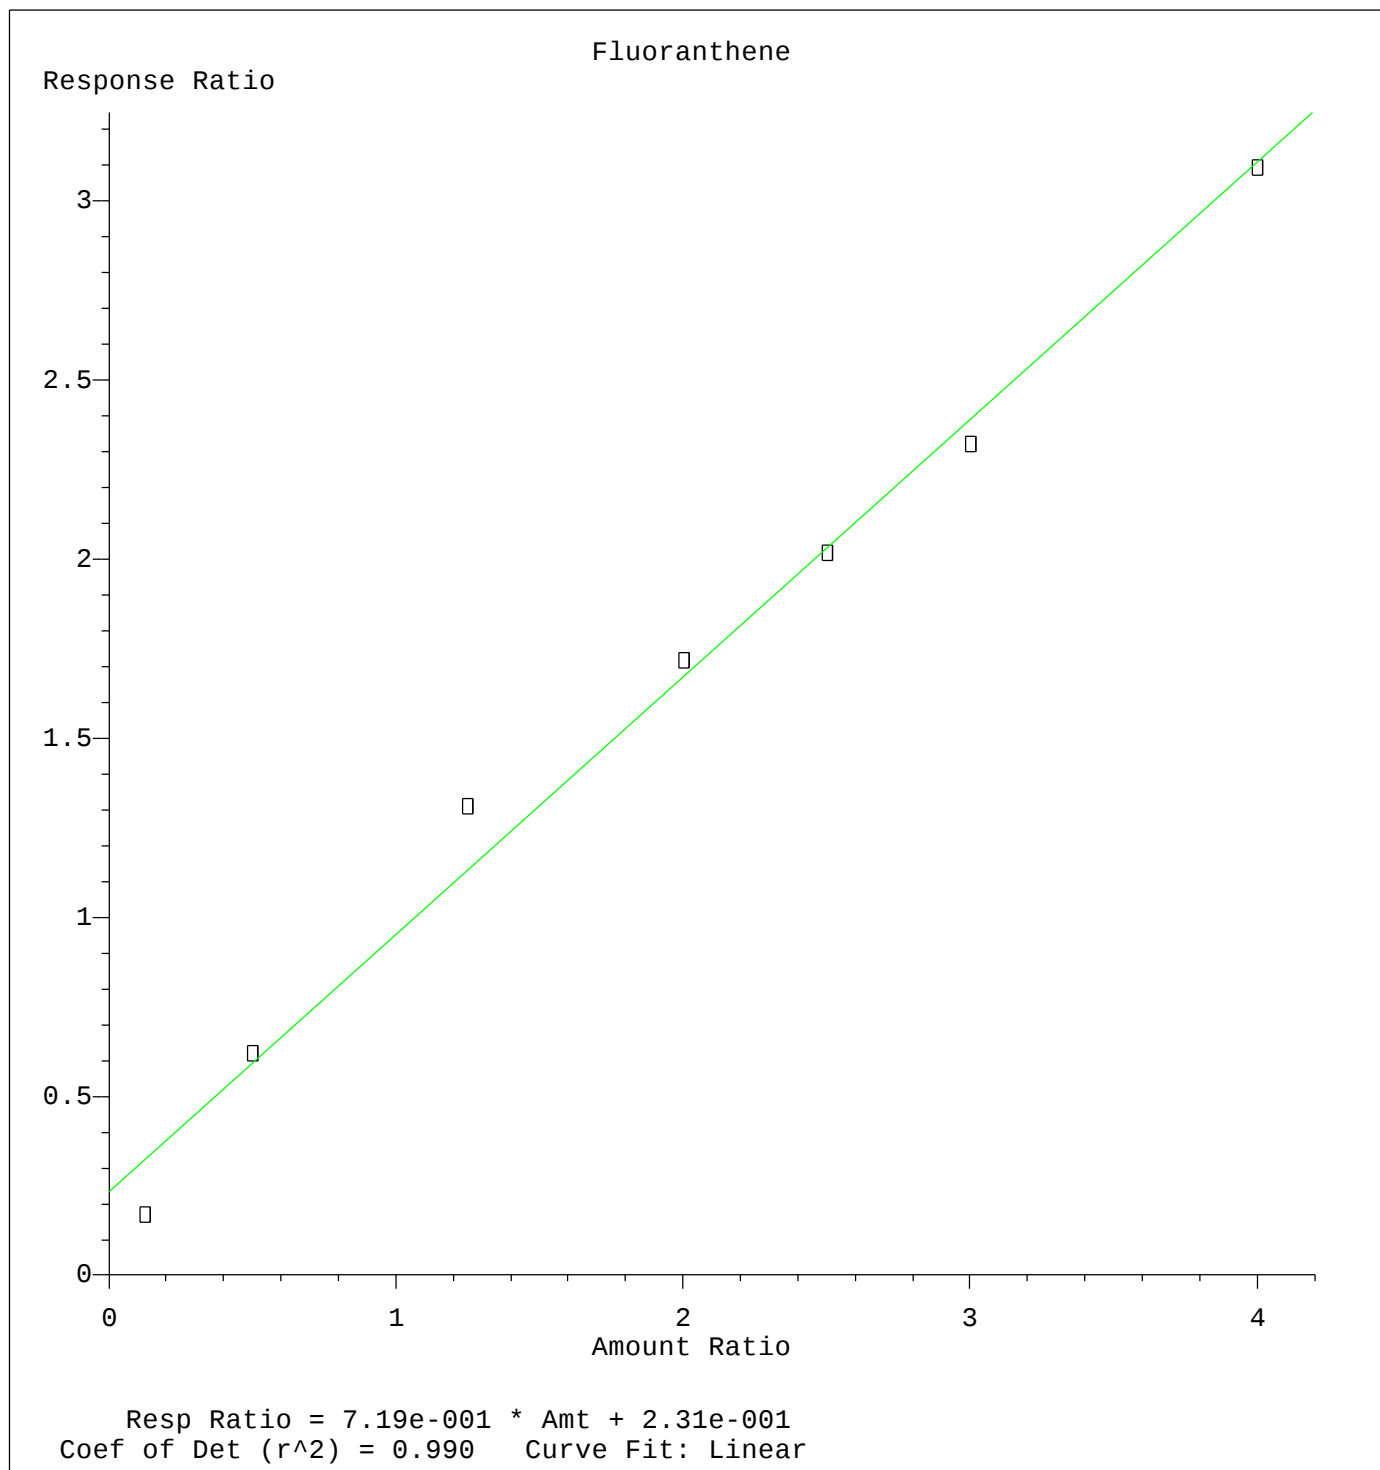

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF041516.M
Calibration Table Last Updated: Fri Apr 15 15:56:31 2016