
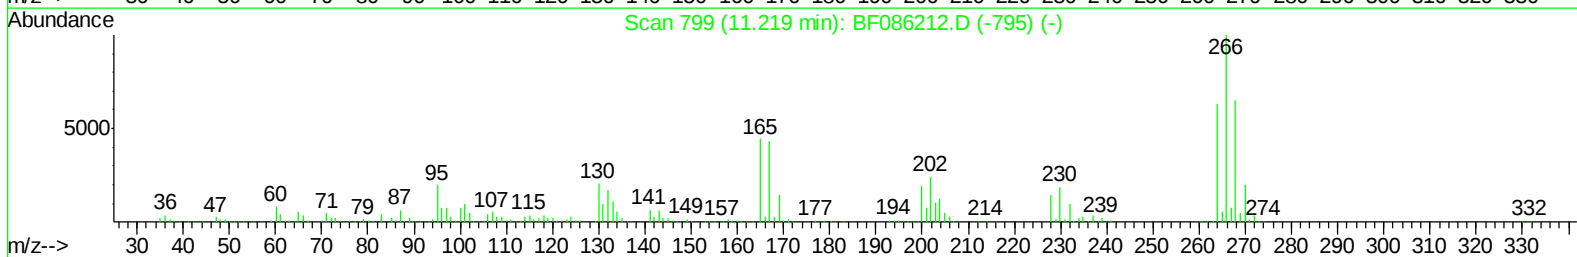
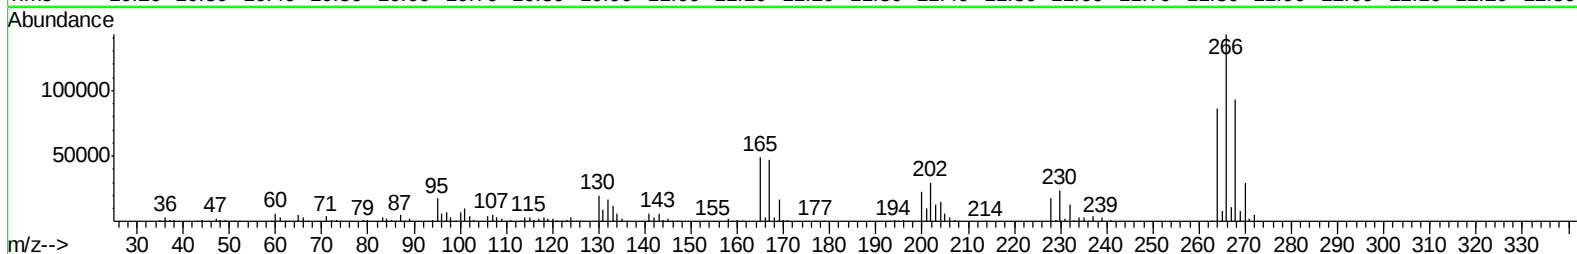


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041516\
Data File : BF086218.D
Acq On : 15 Apr 2016 16:00
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 04:13:40 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF041516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 15 15:56:31 2016
Response via : Initial Calibration

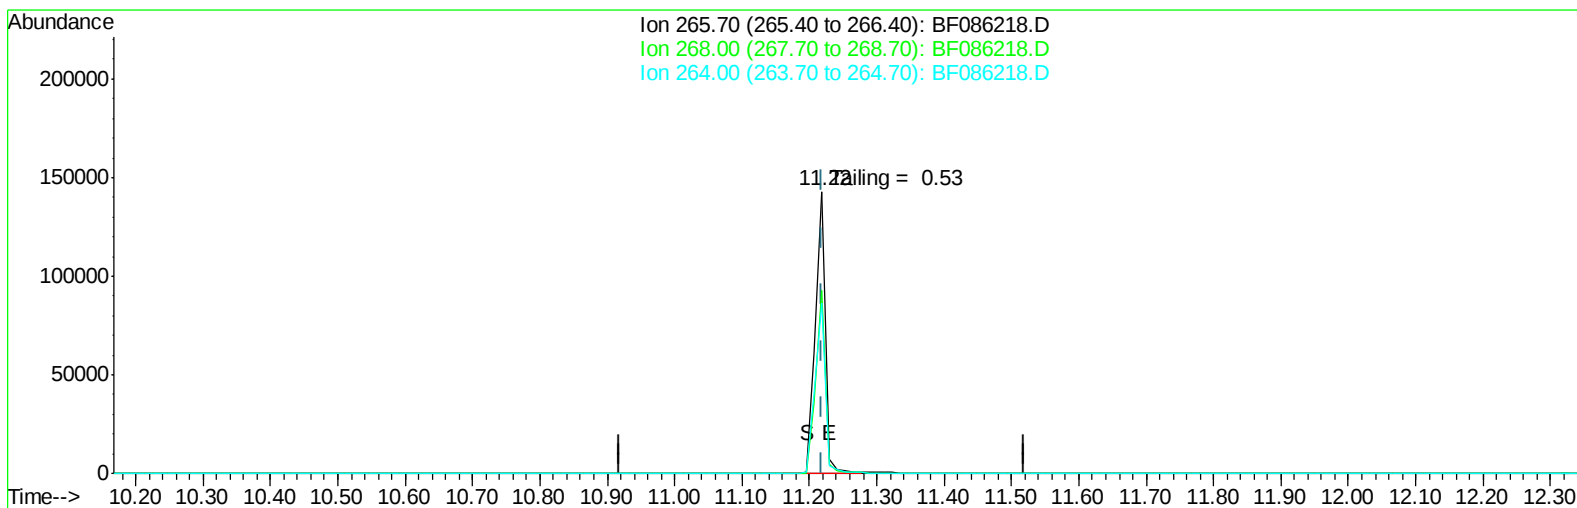

TIC: BF086218.D

(69) Pentachlorophenol (C)




11.219min (-0.000) 12898.70ng

response 149797

Ion	Exp%	Act%
265.70	100	100
268.00	66.20	65.00
264.00	64.10	60.30
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041516\
Data File : BF086218.D
Acq On : 15 Apr 2016 16:00
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 04:13:40 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF041516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 15 15:56:31 2016
Response via : Initial Calibration

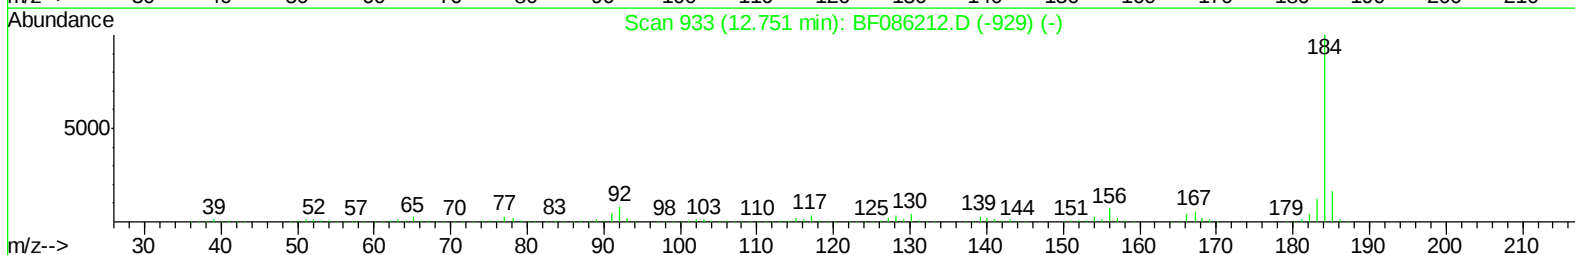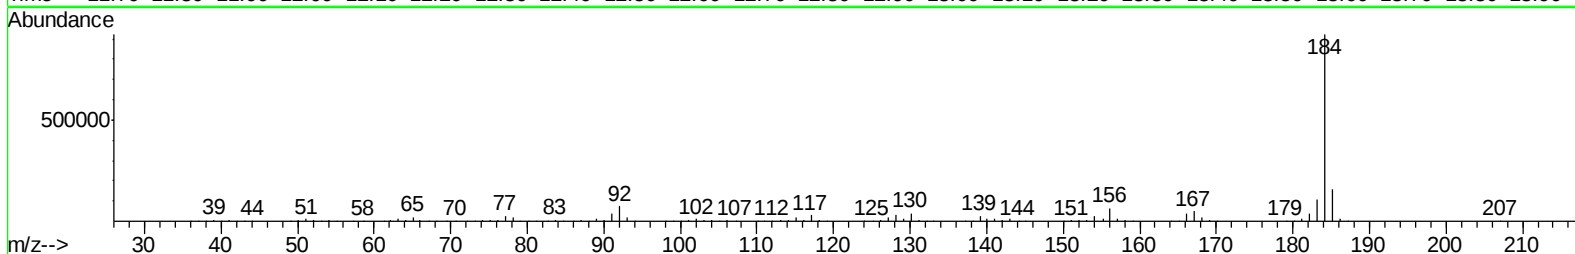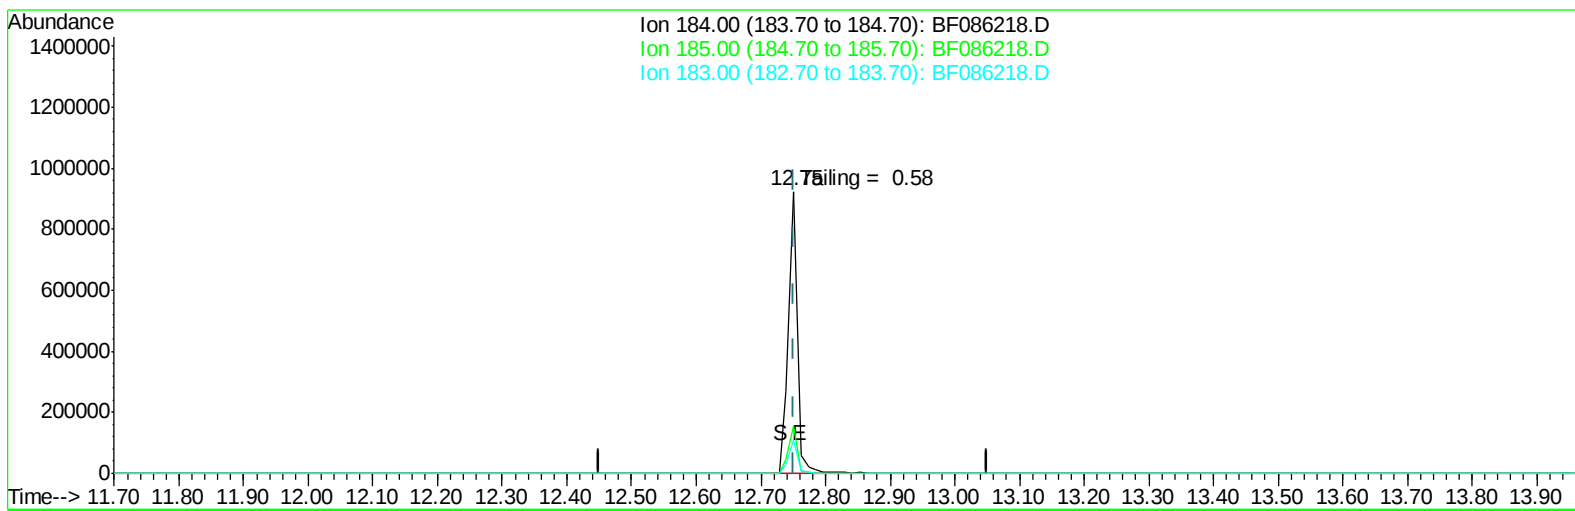

TIC: BF086218.D

(76) Benzidine

12.751min (-0.000) 5595.05ng m

response 891373

Ion	Exp%	Act%
184.00	100	100
185.00	17.70	17.04
183.00	12.20	11.82
0.00	0.00	0.00