
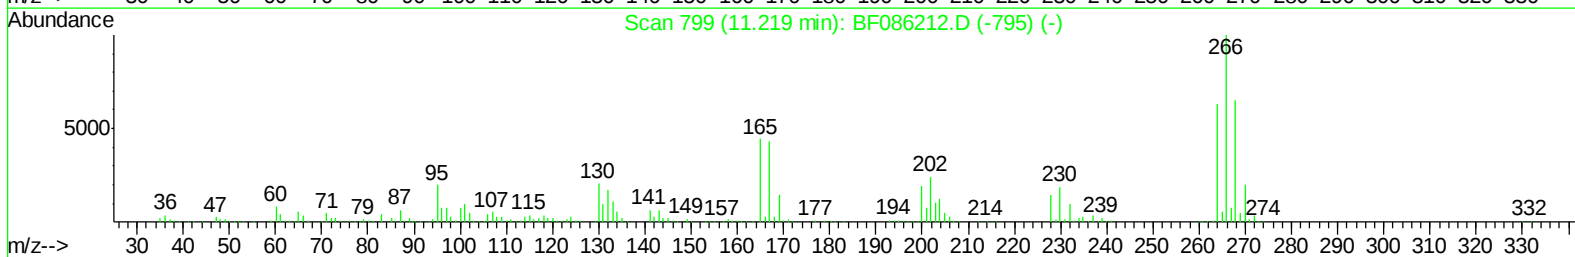
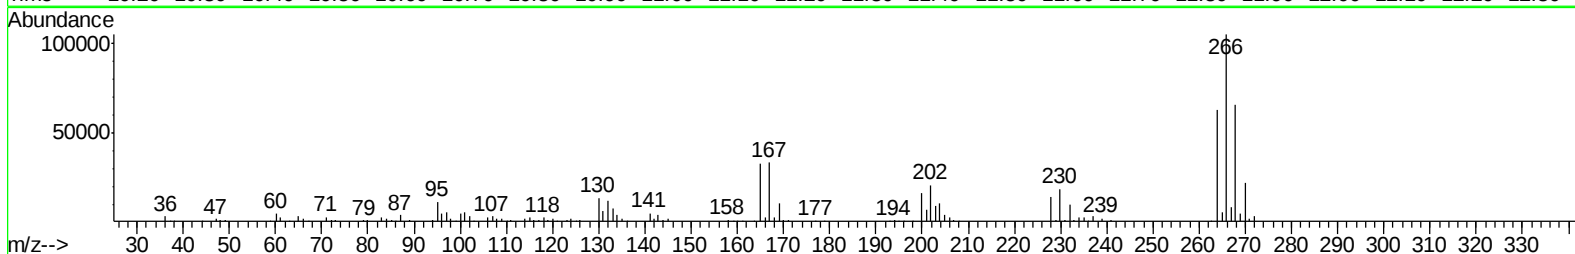


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041516\
Data File : BF086267.D
Acq On : 16 Apr 2016 15:49
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 06:45:15 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF041516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 15 15:56:31 2016
Response via : Initial Calibration

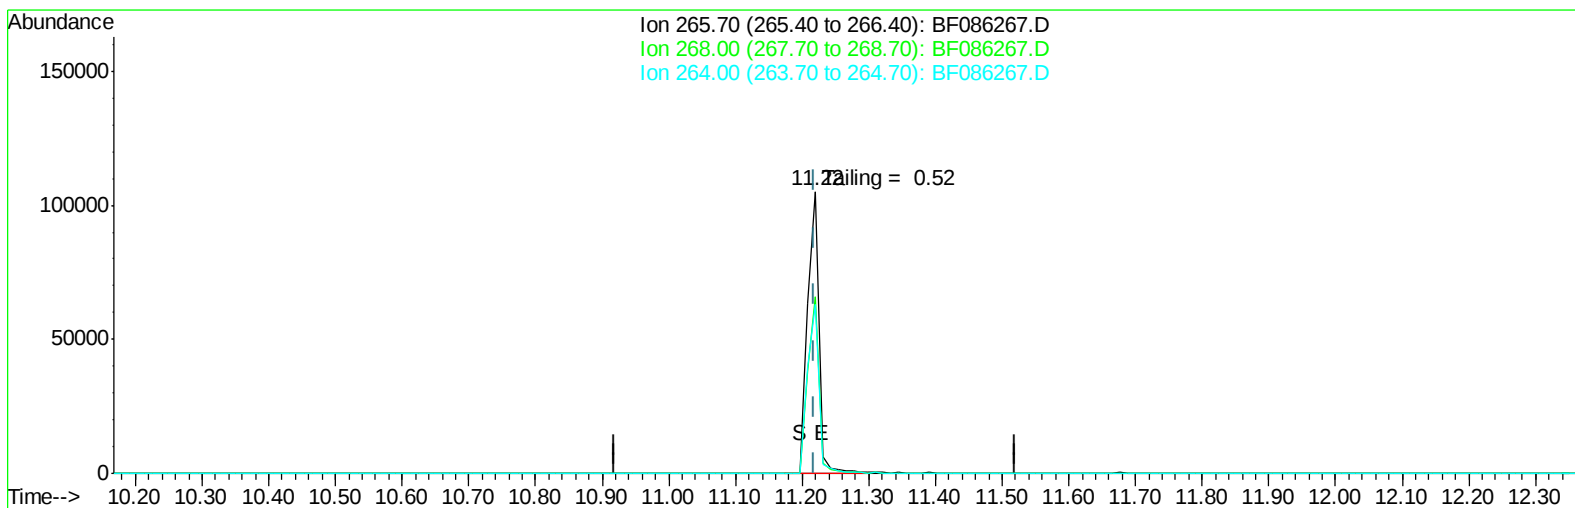

TIC: BF086267.D

(69) Pentachlorophenol (C)




11.219min (-0.000) 20974.72ng

response 125085

Ion	Exp%	Act%
265.70	100	100
268.00	66.20	62.55
264.00	64.10	59.95
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041516\
 Data File : BF086267.D
 Acq On : 16 Apr 2016 15:49
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 06:45:15 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF041516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 15 15:56:31 2016
 Response via : Initial Calibration

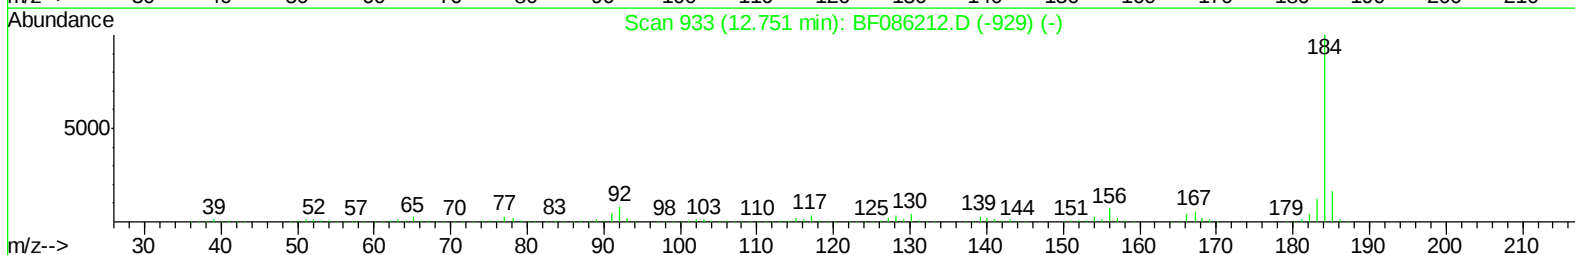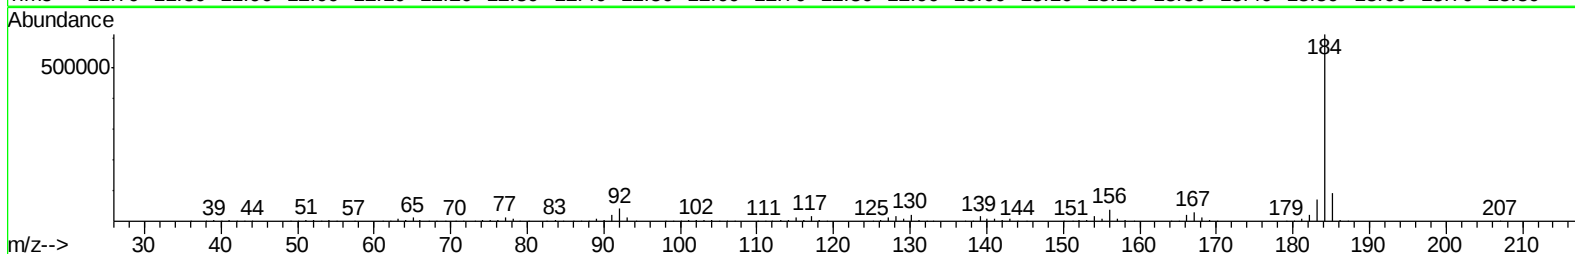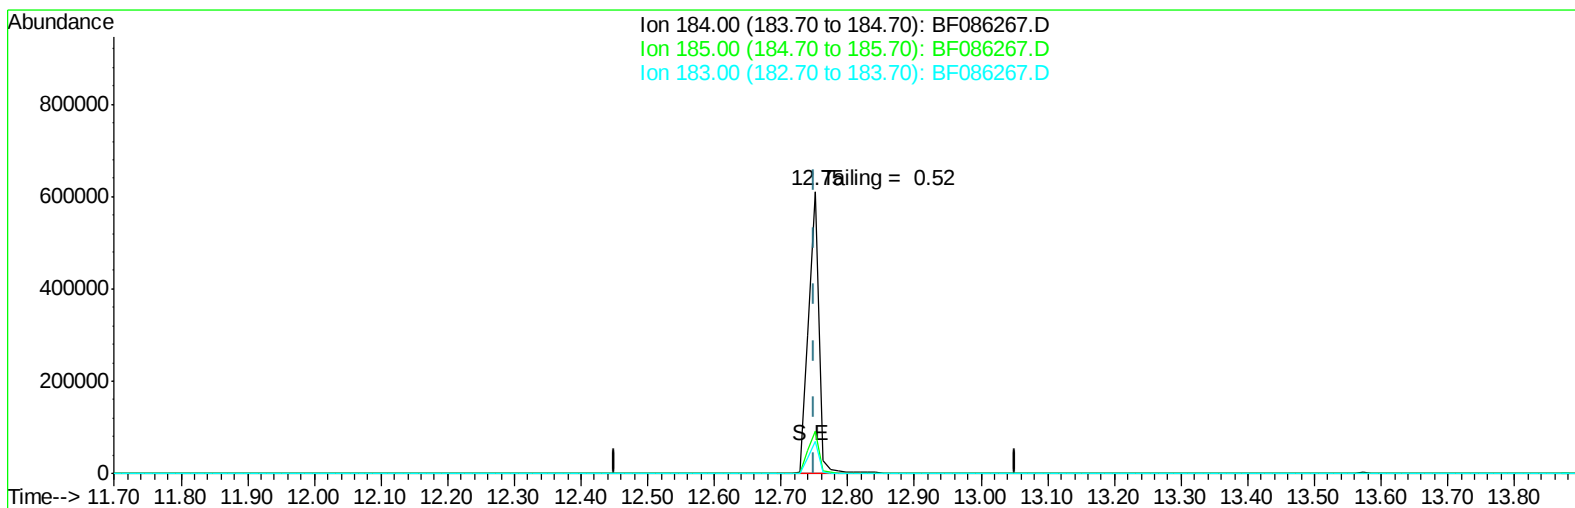

TIC: BF086267.D

(76) Benzidine

12.751min (-0.000) 18020.81ng

response 668287

Ion	Exp%	Act%
184.00	100	100
185.00	17.70	15.07
183.00	12.20	11.45
0.00	0.00	0.00