


Data Path : Z:\HPCHEM1\BNA F\Data\BF041516\
 Data File : BF086208.D
 Acq On : 15 Apr 2016 11:06
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF041516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 15 15:56:31 2016

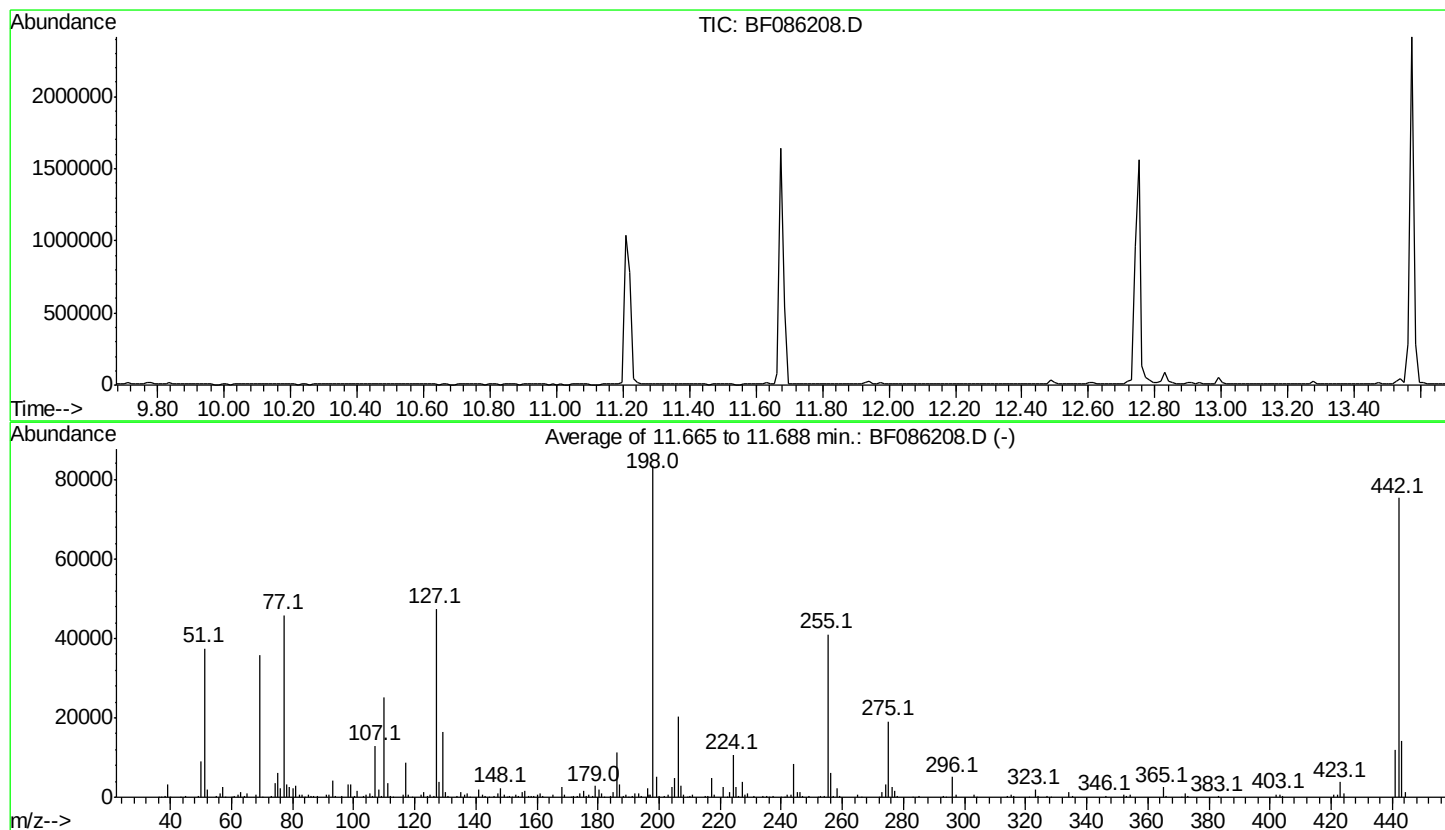

AutoFind: Scans 838, 839, 840; Background Corrected with Scan 835

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.0	37558	PASS
68	69	0.00	2	1.7	601	PASS
69	198	0.00	100	42.8	35733	PASS
70	69	0.00	2	0.4	146	PASS
127	198	10	80	56.9	47518	PASS
197	198	0.00	2	0.7	578	PASS
198	198	100	100	100.0	83512	PASS
199	198	5	9	6.2	5157	PASS
275	198	10	60	22.9	19084	PASS
365	198	1	100	2.9	2438	PASS
441	442	0.01	24	15.7	11865	PASS
442	198	50	100	90.3	75398	PASS
443	442	15	24	18.9	14229	PASS