


Data Path : Z:\HPCHEM1\BNA F\DATA\BF041516\
 Data File : BF086218.D
 Acq On : 15 Apr 2016 16:00
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF041516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 15 15:56:31 2016

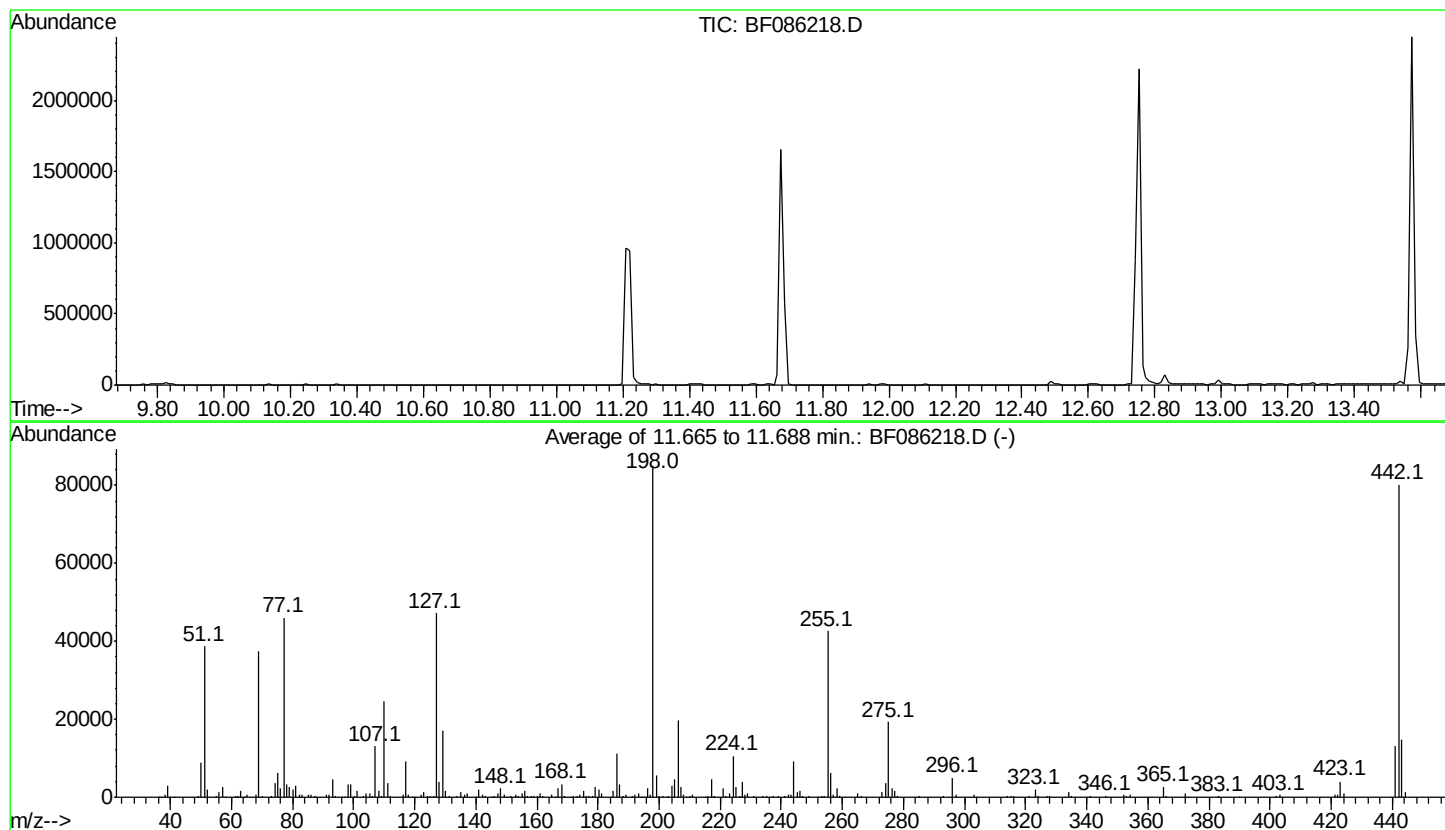

AutoFind: Scans 838, 839, 840; Background Corrected with Scan 835

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.5	38686	PASS
68	69	0.00	2	1.6	603	PASS
69	198	0.00	100	43.9	37327	PASS
70	69	0.00	2	0.6	230	PASS
127	198	10	80	55.5	47198	PASS
197	198	0.00	2	0.9	788	PASS
198	198	100	100	100.0	85091	PASS
199	198	5	9	6.5	5547	PASS
275	198	10	60	22.6	19230	PASS
365	198	1	100	3.2	2752	PASS
441	442	0.01	24	16.4	13156	PASS
442	198	50	100	94.4	80322	PASS
443	442	15	24	18.6	14931	PASS