


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF041516\  
 Data File : BF086267.D  
 Acq On : 16 Apr 2016 15:49  
 Operator : UM/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF041516.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Apr 15 15:56:31 2016

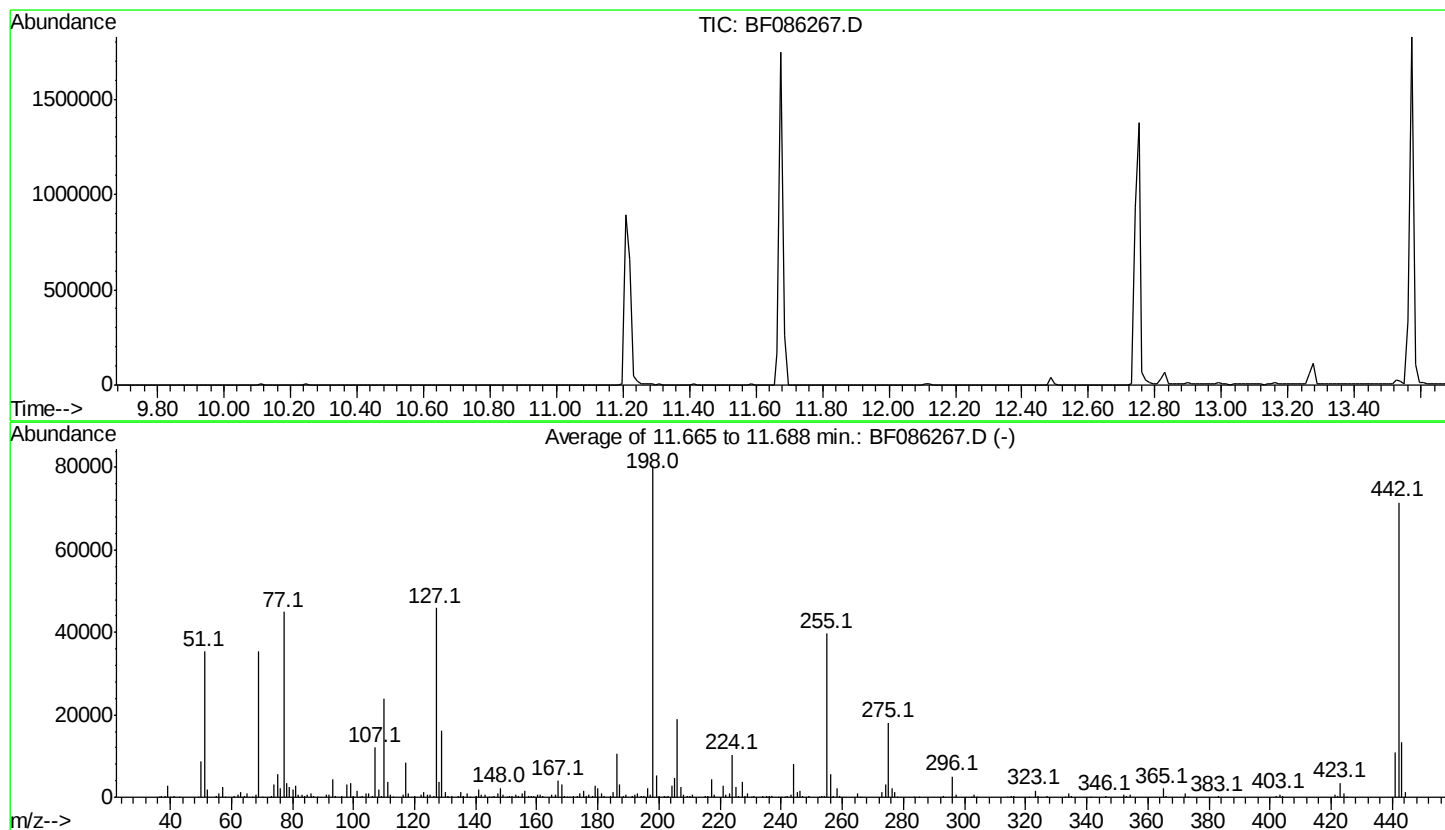

AutoFind: Scans 838, 839, 840; Background Corrected with Scan 835

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 43.9      | 35320   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.8       | 637     | PASS             |
| 69          | 198          | 0.00         | 100          | 43.8      | 35281   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.5       | 162     | PASS             |
| 127         | 198          | 10           | 80           | 57.1      | 45951   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.9       | 727     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 80469   | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 5427    | PASS             |
| 275         | 198          | 10           | 60           | 22.5      | 18067   | PASS             |
| 365         | 198          | 1            | 100          | 2.7       | 2173    | PASS             |
| 441         | 442          | 0.01         | 24           | 15.4      | 11013   | PASS             |
| 442         | 198          | 50           | 100          | 88.8      | 71464   | PASS             |
| 443         | 442          | 15           | 24           | 18.7      | 13346   | PASS             |