

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041521\
 Data File : BF123570.D
 Acq On : 15 Apr 2021 16:28
 Operator : JU/CG
 Sample : PB135656BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB135656BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123570.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.116	3	5	11	rVB	331521	342260	3.33%	0.586%
2	5.481	572	577	580	rBV	5948715	5408281	52.69%	9.253%
3	6.492	743	749	752	rBV	5674599	5575494	54.32%	9.539%
4	6.869	809	813	816	rBV	2065494	1594886	15.54%	2.729%
5	7.028	835	840	843	rBV	6758779	6028855	58.74%	10.314%
6	7.433	903	909	912	rBV	5476308	5417021	52.77%	9.268%
7	8.151	1027	1031	1035	rBV	2373101	2048596	19.96%	3.505%
8	9.233	1210	1215	1218	rBV	8783726	8658002	84.35%	14.812%
9	9.916	1326	1331	1334	rBV	2519450	2211625	21.55%	3.784%
10	10.704	1460	1465	1468	rBV	4818899	4186369	40.79%	7.162%
11	11.404	1580	1584	1587	rBV	2944822	2378877	23.18%	4.070%
12	13.004	1850	1856	1859	rBV	10078191	10264440	100.00%	17.561%
13	14.051	2030	2034	2038	rBV	2534962	2240183	21.82%	3.833%
14	15.539	2281	2287	2292	rBV	1532464	1969978	19.19%	3.370%
15	17.186	2556	2567	2568	rBV6	53409	125837	1.23%	0.215%


Sum of corrected areas: 58450704

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041521\
Data File : BF123570.D
Acq On : 15 Apr 2021 16:28
Operator : JU/CG
Sample : PB135656BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB135656BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

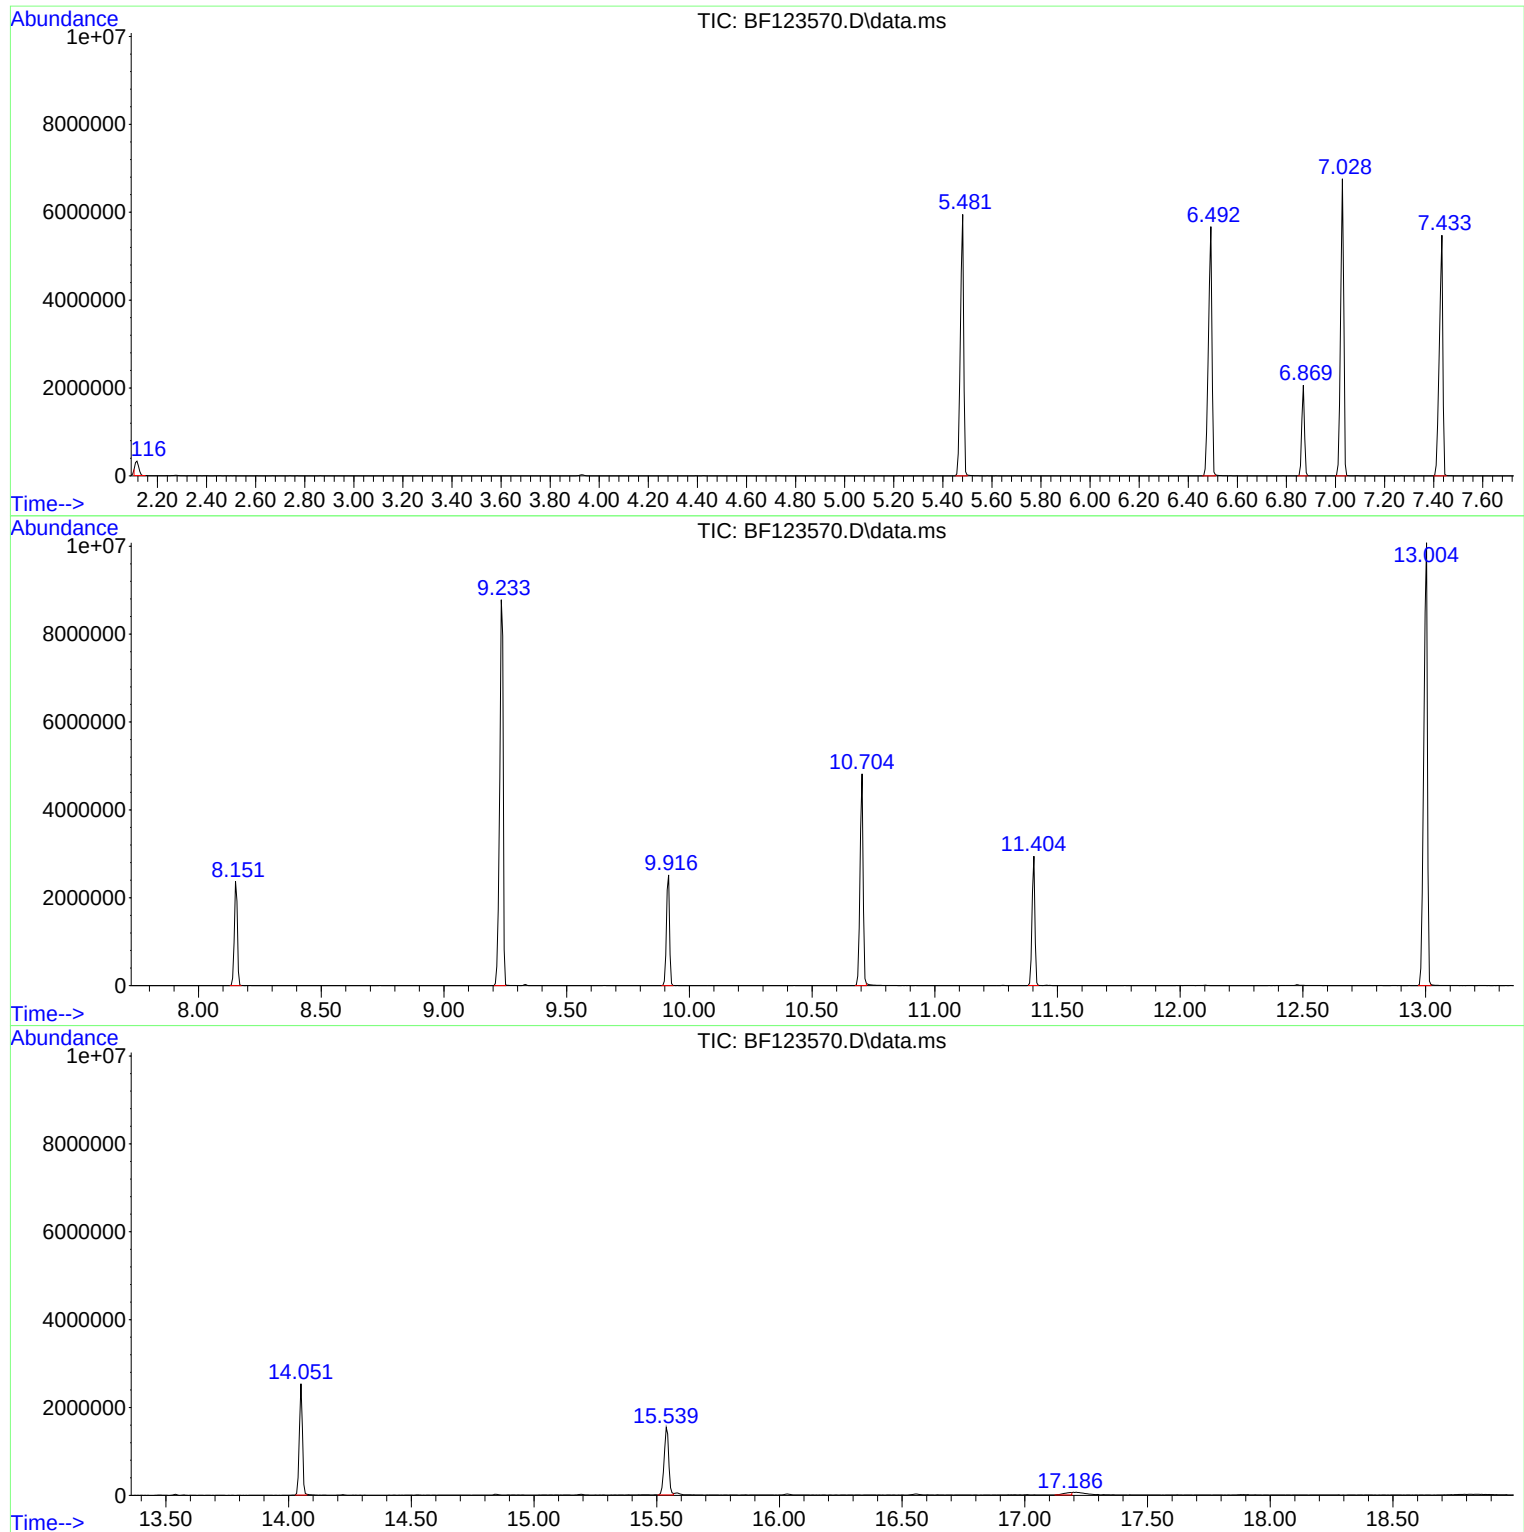

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041521\
Data File : BF123570.D
Acq On : 15 Apr 2021 16:28
Operator : JU/CG
Sample : PB135656BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB135656BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.116	4.29 ng	342260	1,4-Dichlorobenzene-d4	6.869

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			Silane, tetramethyl-	88	C4H12Si	000075-76-3	35
4			3-Pentanol, 2,4-dimethyl-	116	C7H16O	000600-36-2	33
5			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	32

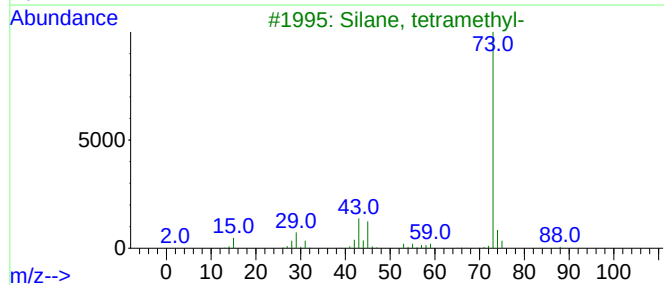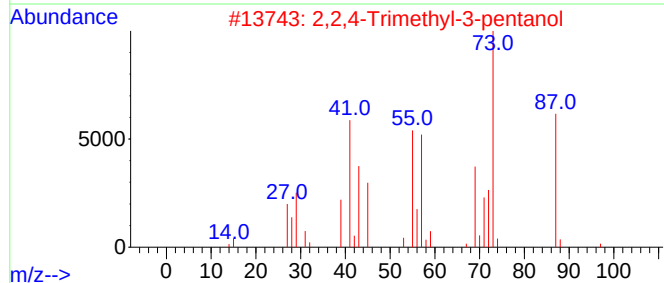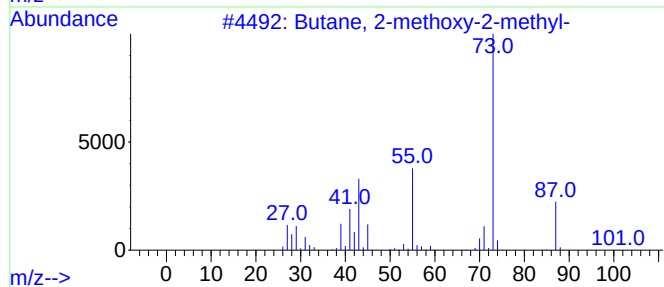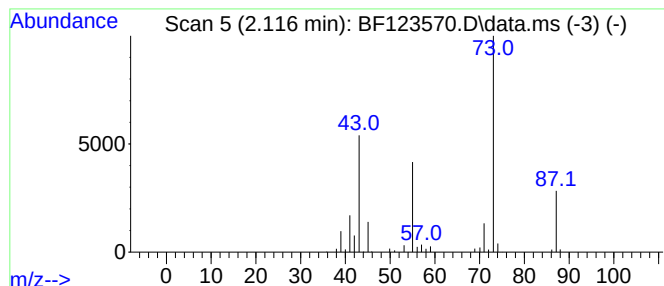

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041521\
Data File : BF123570.D
Acq On : 15 Apr 2021 16:28
Operator : JU/CG
Sample : PB135656BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB135656BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.116	4.3	ng	342260	1	6.869	1594890	20.0