

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041521\
 Data File : BF123578.D
 Acq On : 15 Apr 2021 20:56
 Operator : JU/CG
 Sample : M1990-01RE
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 ELEVATOR-PIT-STANDING-WATER

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123578.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.122	3	6	11	rVB	7718263	9169060	100.00%	13.232%
2	5.475	572	576	588	rBV	2901519	2594725	28.30%	3.744%
3	6.169	691	694	702	rBV	105032	113860	1.24%	0.164%
4	6.481	744	747	750	rBV	1047899	1007310	10.99%	1.454%
5	6.510	750	752	758	rVV	331957	539333	5.88%	0.778%
6	6.569	758	762	769	rVB4	88247	184725	2.01%	0.267%
7	6.669	775	779	781	rBV	122755	114720	1.25%	0.166%
8	6.792	797	800	807	rBV	161626	195325	2.13%	0.282%
9	6.869	809	813	816	rBV	2030070	1717587	18.73%	2.479%
10	7.028	832	840	843	rBV2	7239806	8602201	93.82%	12.414%
11	7.434	899	909	912	rBV	5621154	5765553	62.88%	8.320%
12	7.498	917	920	923	rBV	124847	101750	1.11%	0.147%
13	7.781	964	968	970	rBV	766981	795538	8.68%	1.148%
14	7.804	970	972	983	rVV	729737	1053229	11.49%	1.520%
15	7.892	985	987	990	rVB2	152328	138306	1.51%	0.200%
16	8.151	1027	1031	1034	rBV	2590245	2144525	23.39%	3.095%
17	8.275	1049	1052	1055	rBV2	86474	91856	1.00%	0.133%
18	8.386	1067	1071	1073	rBV	74671	97655	1.07%	0.141%
19	8.422	1073	1077	1083	rVB2	126606	187487	2.04%	0.271%
20	9.233	1210	1215	1218	rBV	9171832	8750389	95.43%	12.627%
21	9.316	1226	1229	1231	rBV	120525	92131	1.00%	0.133%
22	9.622	1278	1281	1285	rBV	262742	209407	2.28%	0.302%
23	9.669	1286	1289	1296	rVB2	133068	153947	1.68%	0.222%
24	9.916	1327	1331	1334	rVB	2472346	2246361	24.50%	3.242%
25	10.045	1350	1353	1362	rVB	213289	209474	2.28%	0.302%
26	10.704	1460	1465	1468	rBV	4357551	3996660	43.59%	5.767%
27	10.845	1487	1489	1496	rVB2	62916	92172	1.01%	0.133%
28	11.404	1580	1584	1587	rBV	2736190	2319550	25.30%	3.347%
29	11.939	1671	1675	1686	rBV	1459195	1538499	16.78%	2.220%
30	12.727	1806	1809	1819	rBV	583154	618681	6.75%	0.893%
31	13.004	1850	1856	1859	rBV	8730905	9033821	98.53%	13.036%
32	13.845	1997	1999	2003	rVB	85001	102557	1.12%	0.148%
33	13.886	2004	2006	2008	rVV	116987	118342	1.29%	0.171%
34	13.939	2009	2015	2029	rVV3	474690	1566823	17.09%	2.261%
35	14.051	2030	2034	2038	rVB	1893544	1685904	18.39%	2.433%
36	14.921	2178	2182	2186	rVB	471133	475376	5.18%	0.686%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041521\
Data File : BF123578.D
Acq On : 15 Apr 2021 20:56
Operator : JU/CG
Sample : M1990-01RE
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ELEVATOR-PIT-STANDING-WATER

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	15.539	2282	2287	2291	rBV	1019315	1260414	13.75%	1.819%
38	15.580	2291	2294	2301	rVB	85426	119121	1.30%	0.172%
39	16.027	2367	2370	2377	rBV	61356	92104	1.00%	0.133%




Sum of corrected areas: 69296478

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041521\
Data File : BF123578.D
Acq On : 15 Apr 2021 20:56
Operator : JU/CG
Sample : M1990-01RE
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ELEVATOR-PIT-STANDING-WATER

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

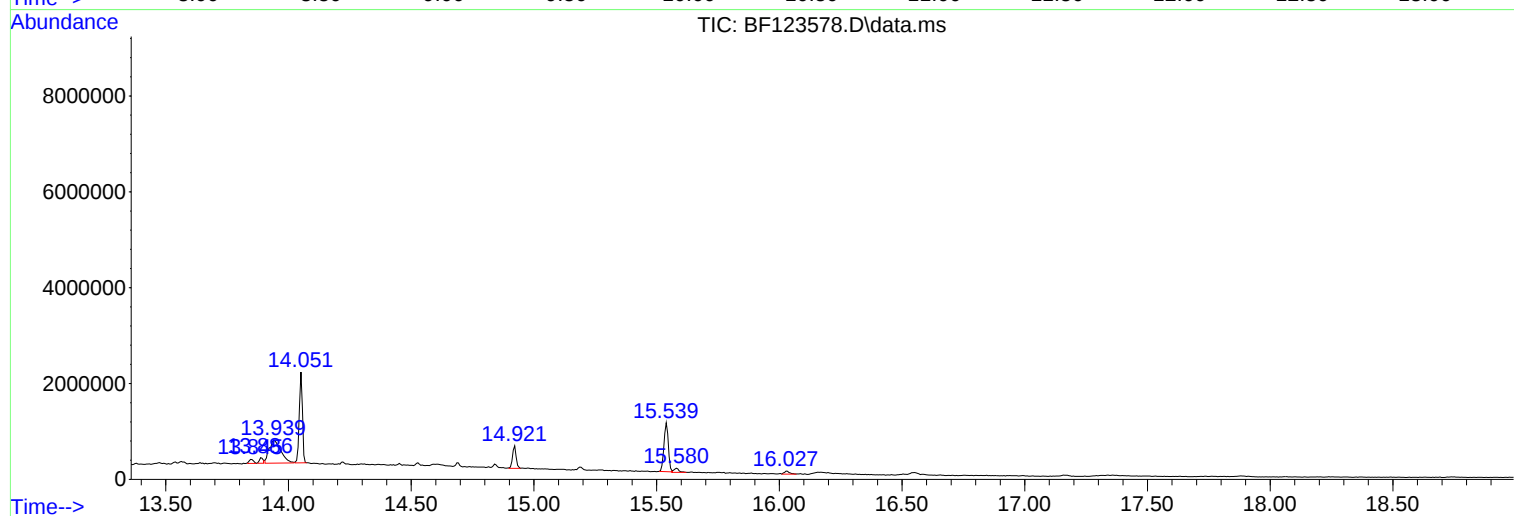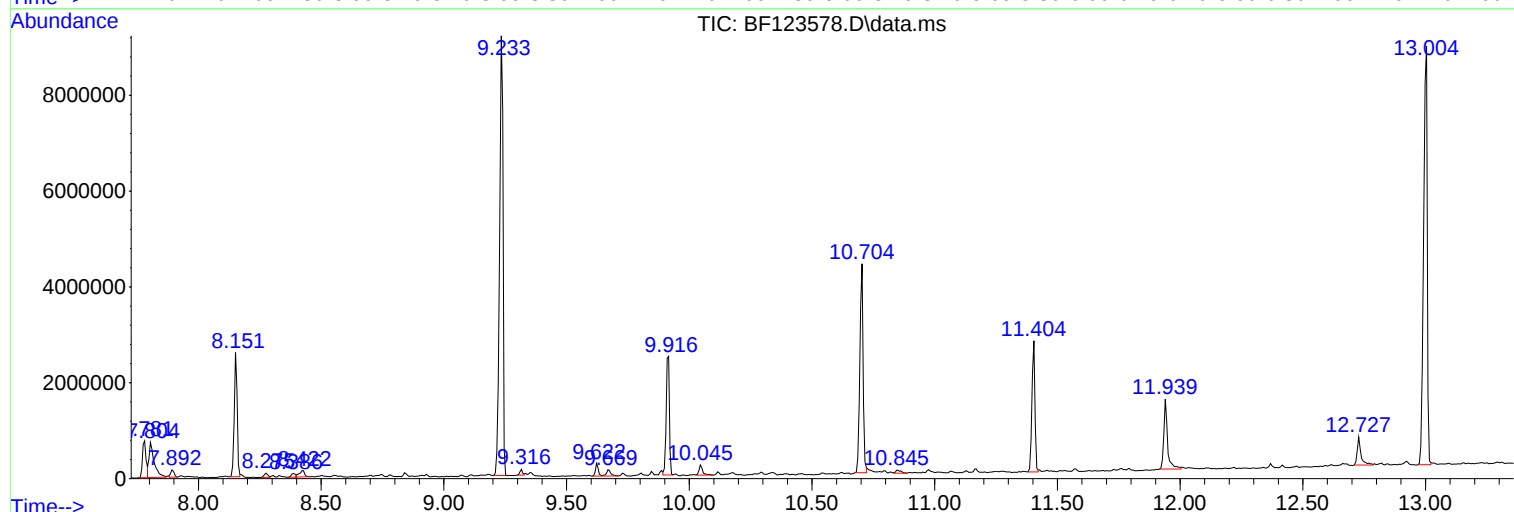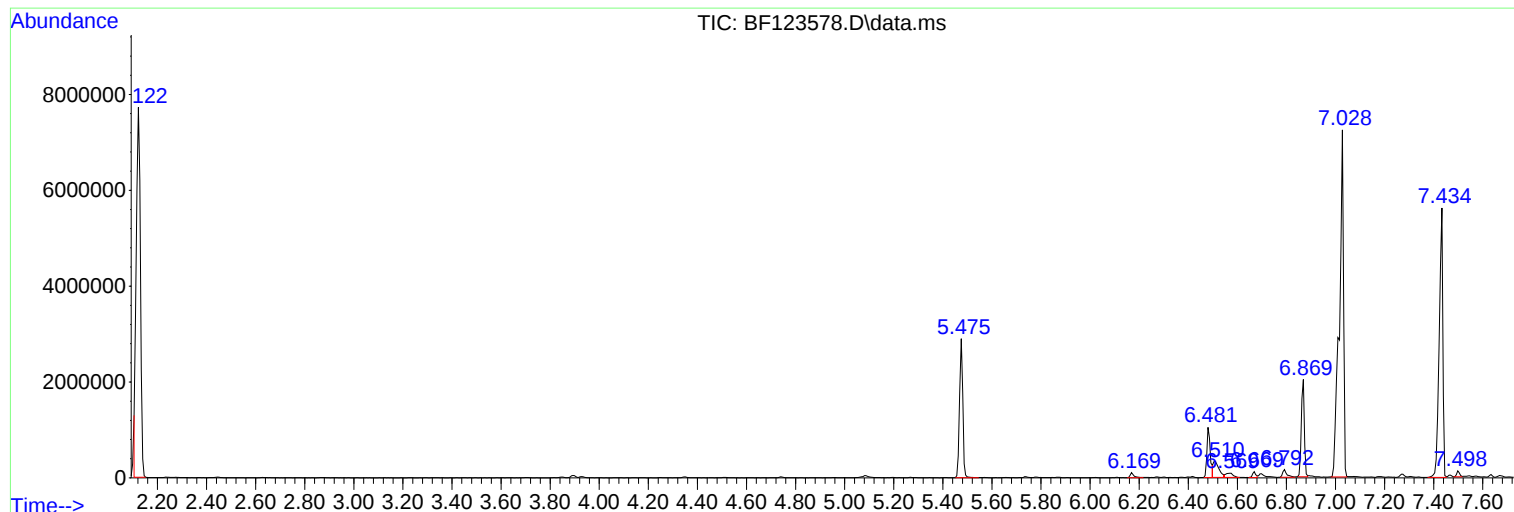

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041521\
Data File : BF123578.D
Acq On : 15 Apr 2021 20:56
Operator : JU/CG
Sample : M1990-01RE
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ELEVATOR-PIT-STANDING-WATER

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041521\
Data File : BF123578.D
Acq On : 15 Apr 2021 20:56
Operator : JU/CG
Sample : M1990-01RE
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ELEVATOR-PIT-STANDING-WATER

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------