

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041521\
 Data File : BF123579.D
 Acq On : 15 Apr 2021 21:28
 Operator : JU/CG
 Sample : M2049-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-09-5.5-6.0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123579.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.187	7	17	24	rVB	2528819	3310599	51.57%	6.665%
2	5.087	501	510	518	rBV	772941	923587	14.39%	1.859%
3	5.487	573	578	581	rBV	5498893	5222983	81.36%	10.515%
4	6.492	744	749	752	rBV	5575621	5688045	88.61%	11.451%
5	6.869	809	813	816	rBV	1805766	1534020	23.90%	3.088%
6	7.428	903	908	911	rBV	4144496	3896972	60.71%	7.845%
7	8.151	1026	1031	1034	rBV	2438660	1959820	30.53%	3.946%
8	9.233	1209	1215	1218	rBV	7293587	6079823	94.71%	12.240%
9	9.622	1278	1281	1285	rBV	221545	170698	2.66%	0.344%
10	9.910	1326	1330	1334	rVB	2291336	2109522	32.86%	4.247%
11	10.704	1460	1465	1468	rBV	3852349	3630661	56.56%	7.309%
12	11.404	1580	1584	1587	rBV	2516072	2221764	34.61%	4.473%
13	12.998	1850	1855	1858	rBV	6993797	6419372	100.00%	12.924%
14	13.845	1994	1999	2002	rBV	79391	107836	1.68%	0.217%
15	13.886	2002	2006	2007	rVV	101459	117204	1.83%	0.236%
16	13.915	2007	2011	2030	rVV4	565048	1411304	21.99%	2.841%
17	14.051	2030	2034	2037	rVB	2198495	1948461	30.35%	3.923%
18	14.221	2059	2063	2068	rVB	114339	107057	1.67%	0.216%
19	14.527	2110	2115	2118	rBV	133559	134102	2.09%	0.270%
20	14.710	2142	2146	2159	rVB	457076	600767	9.36%	1.209%
21	14.839	2165	2168	2173	rVB	120834	116483	1.81%	0.235%
22	15.186	2223	2227	2232	rBV	117322	138645	2.16%	0.279%
23	15.539	2279	2287	2291	rBV	1217704	1548580	24.12%	3.118%
24	15.580	2291	2294	2298	rVB	80833	95719	1.49%	0.193%
25	16.027	2366	2370	2376	rBV2	66761	99956	1.56%	0.201%
26	16.545	2452	2458	2465	rVB4	35485	77895	1.21%	0.157%




Sum of corrected areas: 49671875

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041521\
Data File : BF123579.D
Acq On : 15 Apr 2021 21:28
Operator : JU/CG
Sample : M2049-08
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-09-5.5-6.0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

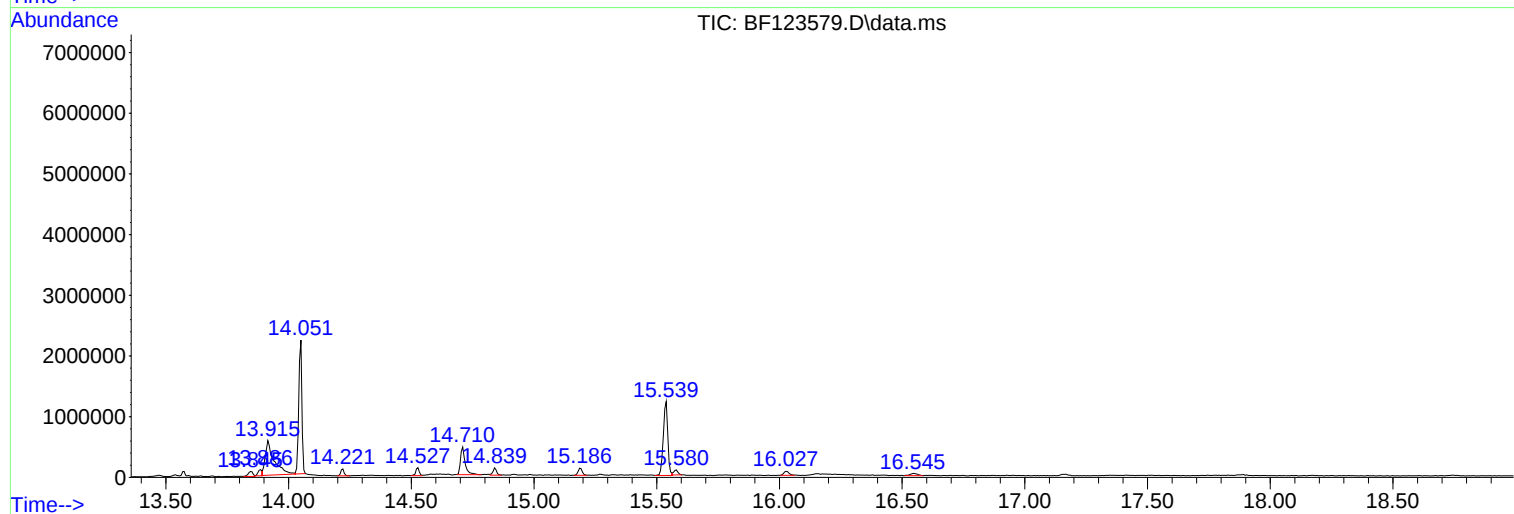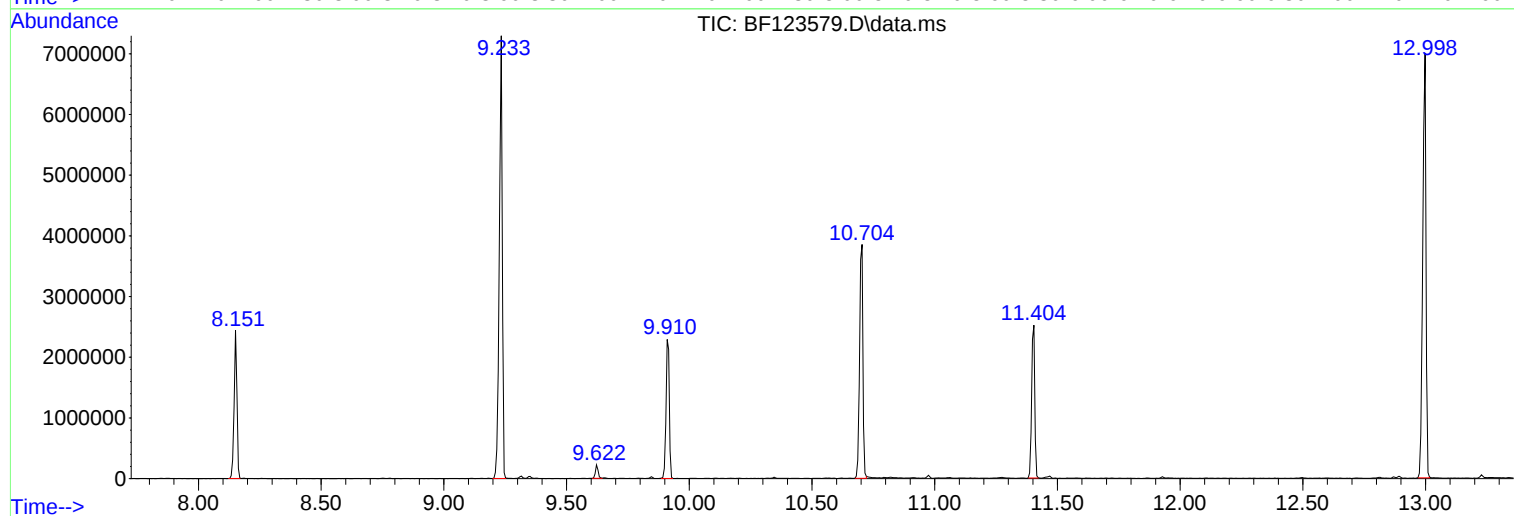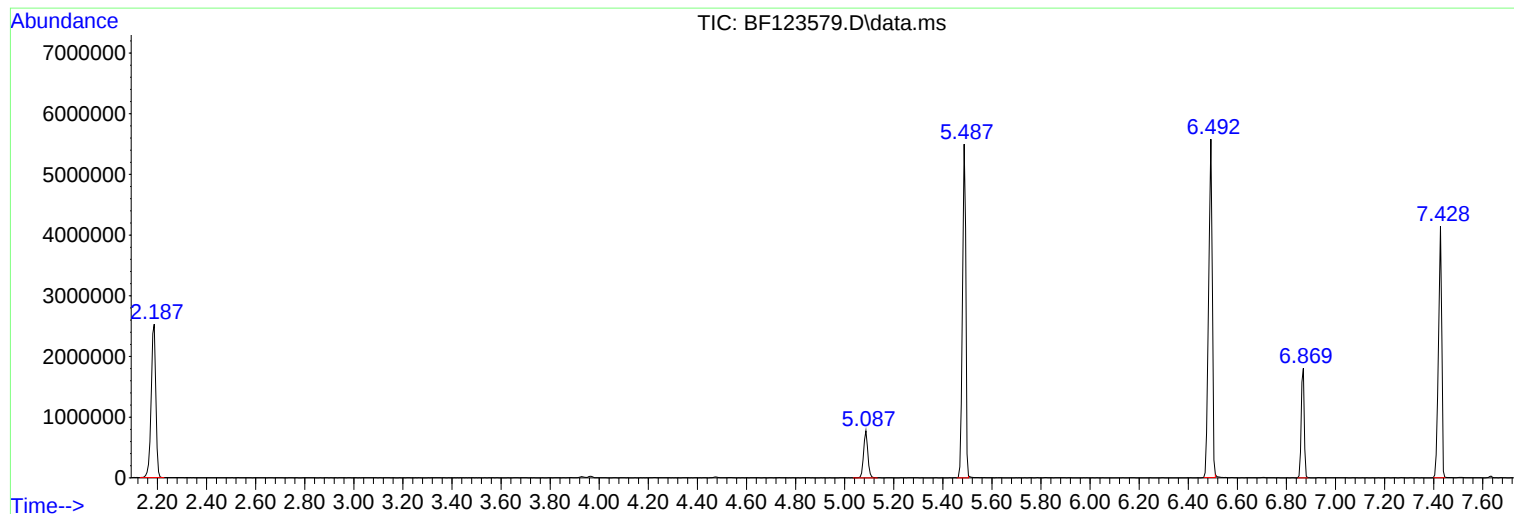

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041521\
Data File : BF123579.D
Acq On : 15 Apr 2021 21:28
Operator : JU/CG
Sample : M2049-08
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-09-5.5-6.0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041521\
Data File : BF123579.D
Acq On : 15 Apr 2021 21:28
Operator : JU/CG
Sample : M2049-08
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-09-5.5-6.0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc