


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041521\
 Data File : BF123561.D
 Acq On : 15 Apr 2021 10:26
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 16 10:31:33 2021

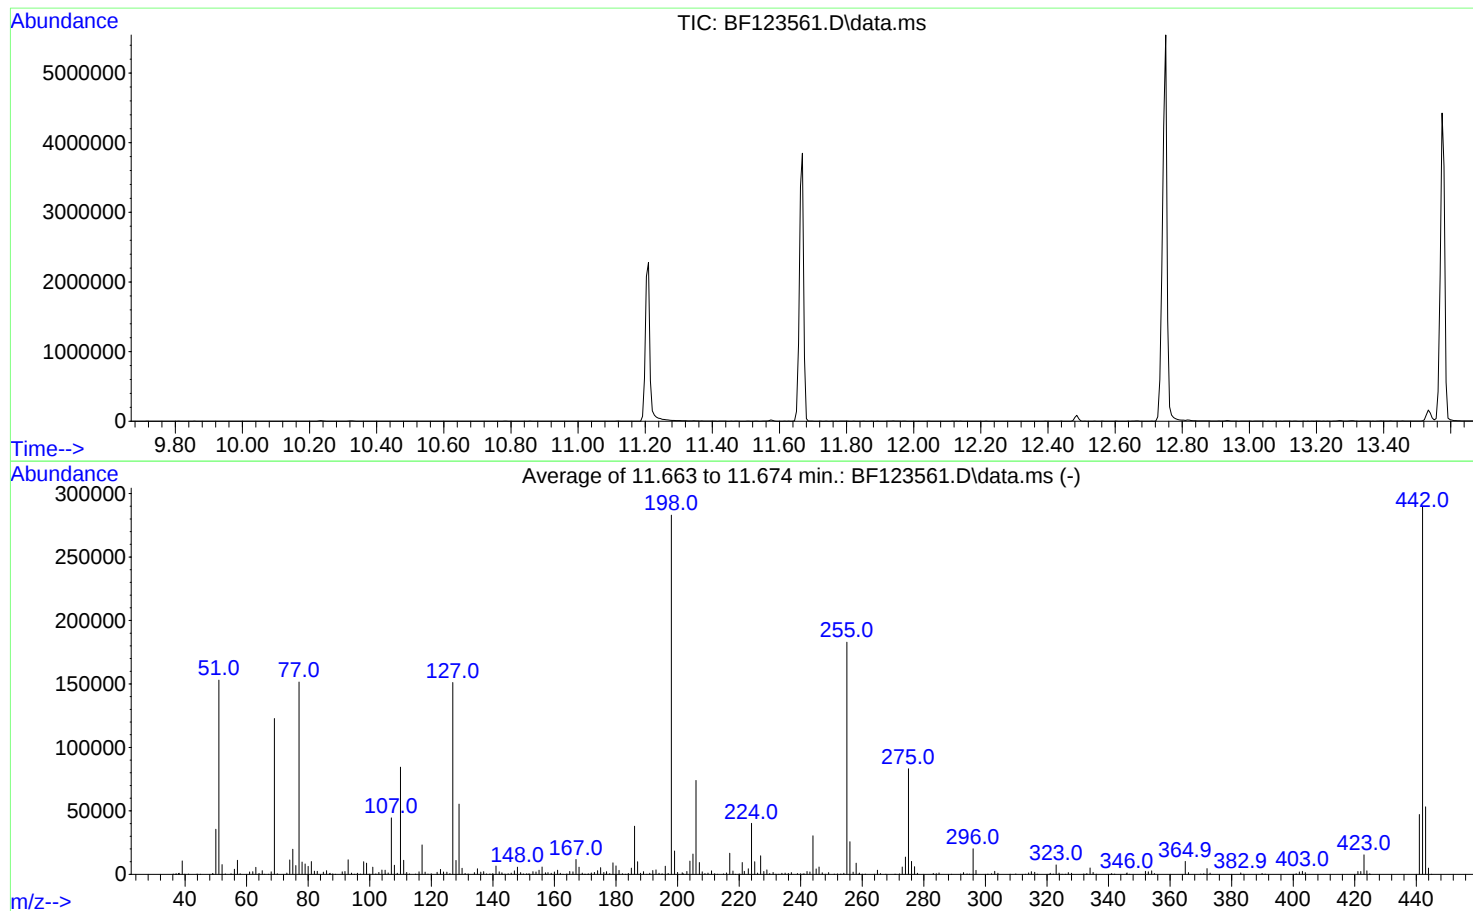

AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.1	153069	PASS
68	69	0.00	2	1.6	2015	PASS
69	198	0.00	100	43.4	122741	PASS
70	69	0.00	2	0.5	554	PASS
127	198	10	80	53.4	151147	PASS
197	198	0.00	2	0.3	708	PASS
198	198	100	100	100.0	283029	PASS
199	198	5	9	6.5	18385	PASS
275	198	10	60	29.4	83192	PASS
365	198	1	100	3.6	10209	PASS
441	198	0.01	100	16.7	47187	PASS
442	442	50	100	100.0	289792	PASS
443	442	15	24	18.3	53147	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/15/2021	BNA_F	<u>BF123561.D</u>
Compound Name	Response	Retention Time
DDT	686569	13.574
DDD	3955	13.268
DDE	1224	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5179	691748	0.75

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041521\
 Data File : BF123561.D
 Acq On : 15 Apr 2021 10:26
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 19 01:29:19 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 16 10:31:33 2021
 Response via : Initial Calibration

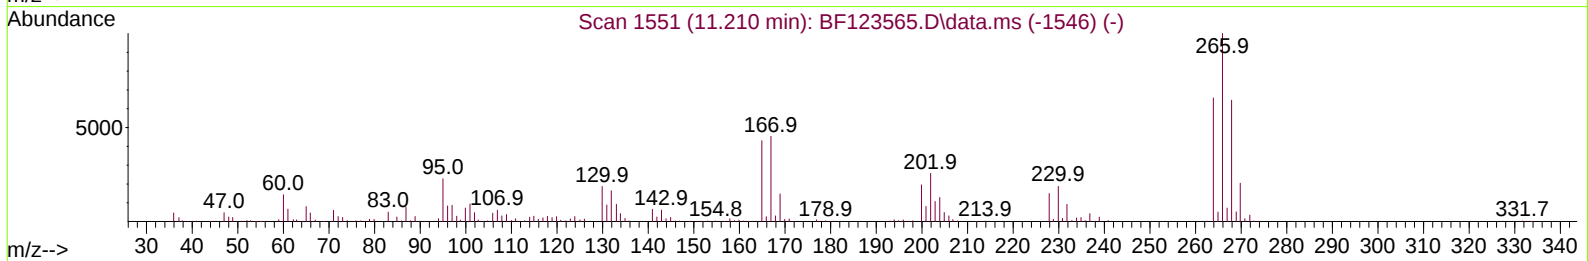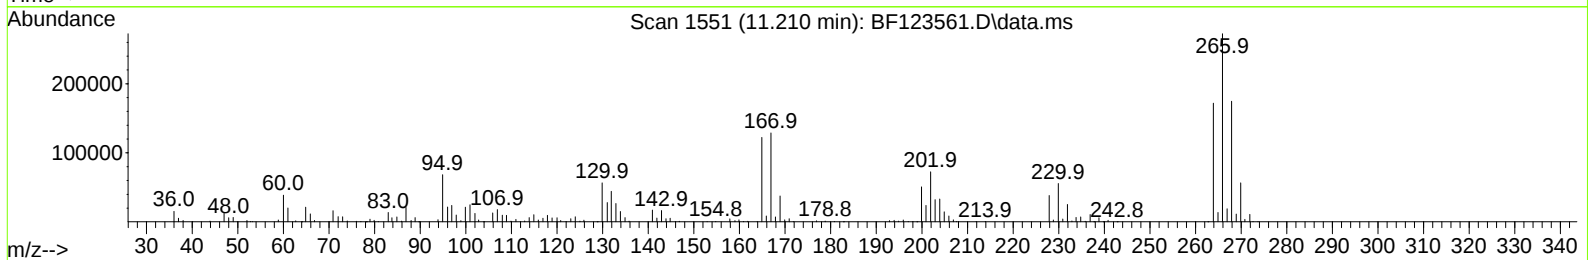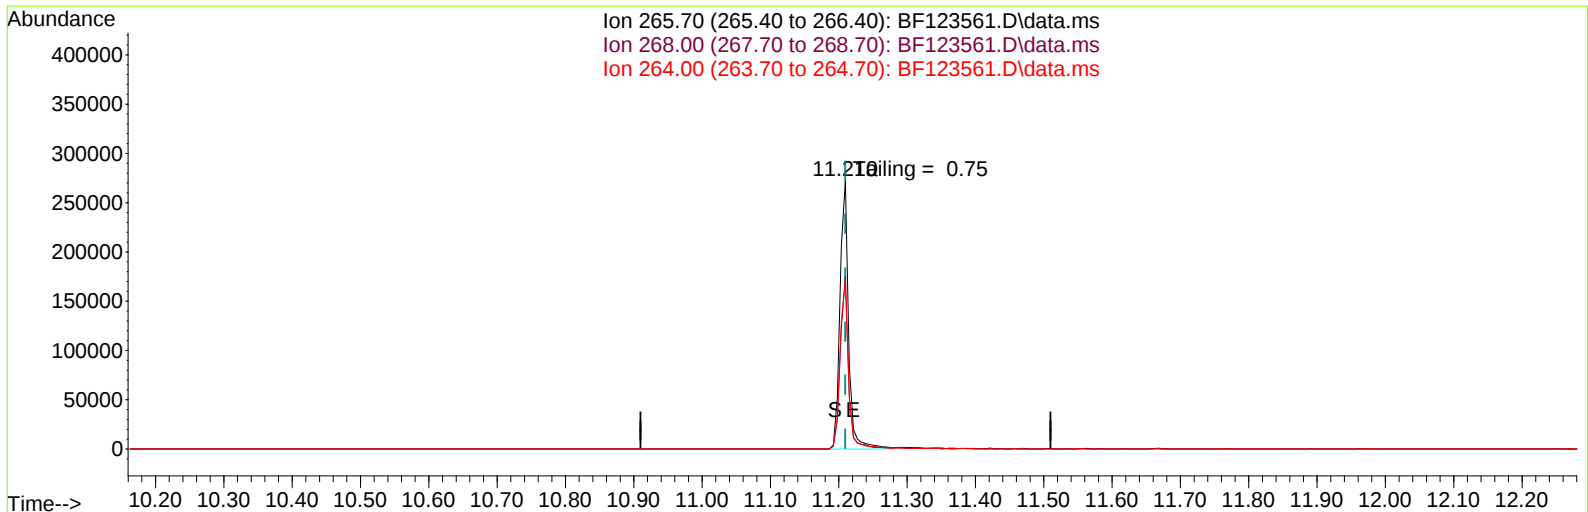

TIC: BF123561.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.000) 220281.24 ng




response 240018

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.17
264.00	65.70	63.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041521\
 Data File : BF123561.D
 Acq On : 15 Apr 2021 10:26
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 19 01:29:19 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 16 10:31:33 2021
 Response via : Initial Calibration

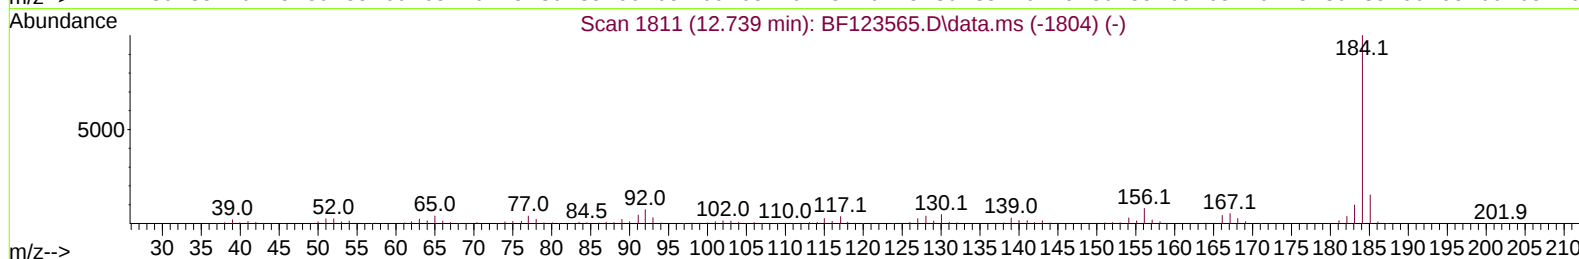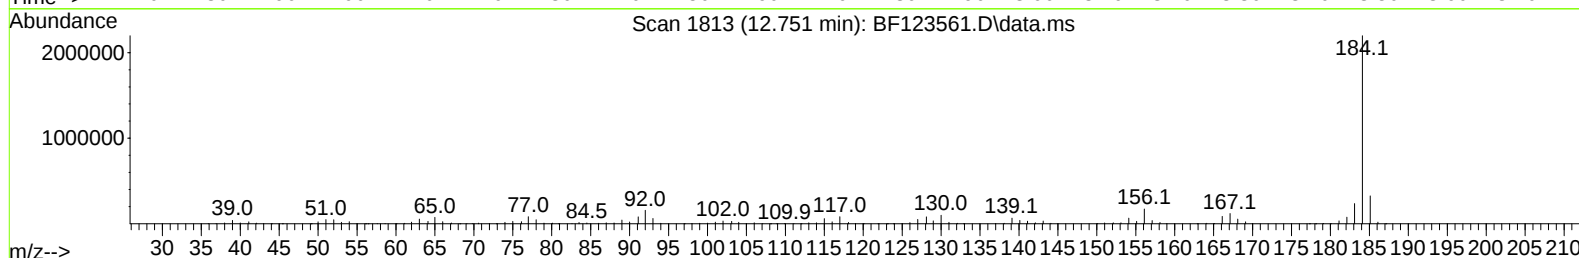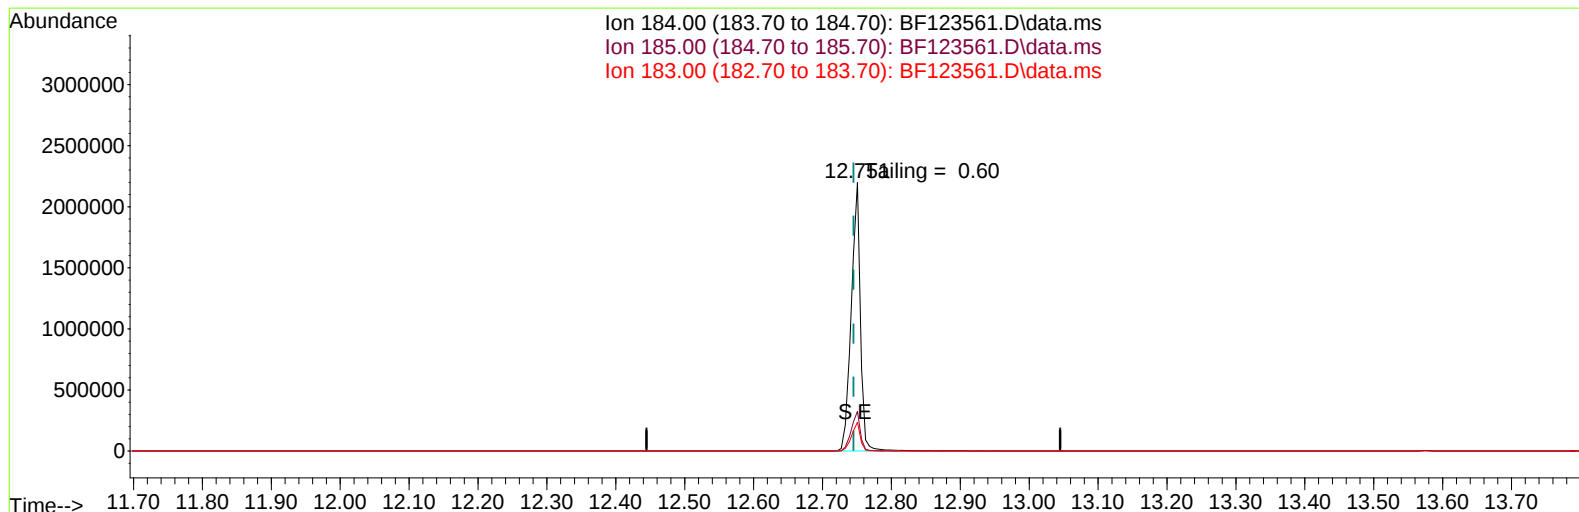

TIC: BF123561.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 7551.19 ng m

response 2010821

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.79
183.00	9.80	10.77
0.00	0.00	0.00