

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041522\
 Data File : BF127798.D
 Acq On : 15 Apr 2022 11:20
 Operator : CG\JU
 Sample : PB144095TB
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB144095TB

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127798.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.587	555	561	564	rBV	4356191	4946663	77.28%	12.904%
2	6.575	722	729	732	rBV	4023216	4988430	77.93%	13.013%
3	6.945	788	792	796	rBV	1313205	1098674	17.16%	2.866%
4	7.510	882	888	891	rBV	2709837	3425832	53.52%	8.936%
5	8.228	1005	1010	1014	rBV	1310709	1409815	22.03%	3.678%
6	9.310	1187	1194	1197	rBV	5776349	6057984	94.64%	15.803%
7	9.992	1303	1310	1313	rBV	1657731	1648962	25.76%	4.301%
8	10.780	1437	1444	1448	rBV	3714938	3900224	60.93%	10.174%
9	11.480	1557	1563	1567	rBV	2000593	1725541	26.96%	4.501%
10	13.074	1826	1834	1837	rBV	6286045	6400779	100.00%	16.697%
11	14.127	2009	2013	2016	rBV	1627458	1431993	22.37%	3.735%
12	15.645	2263	2271	2279	rBV	809083	1101599	17.21%	2.874%
13	17.668	2602	2615	2617	rBV6	69064	198784	3.11%	0.519%




Sum of corrected areas: 38335280

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041522\
Data File : BF127798.D
Acq On : 15 Apr 2022 11:20
Operator : CG\JU
Sample : PB144095TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144095TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

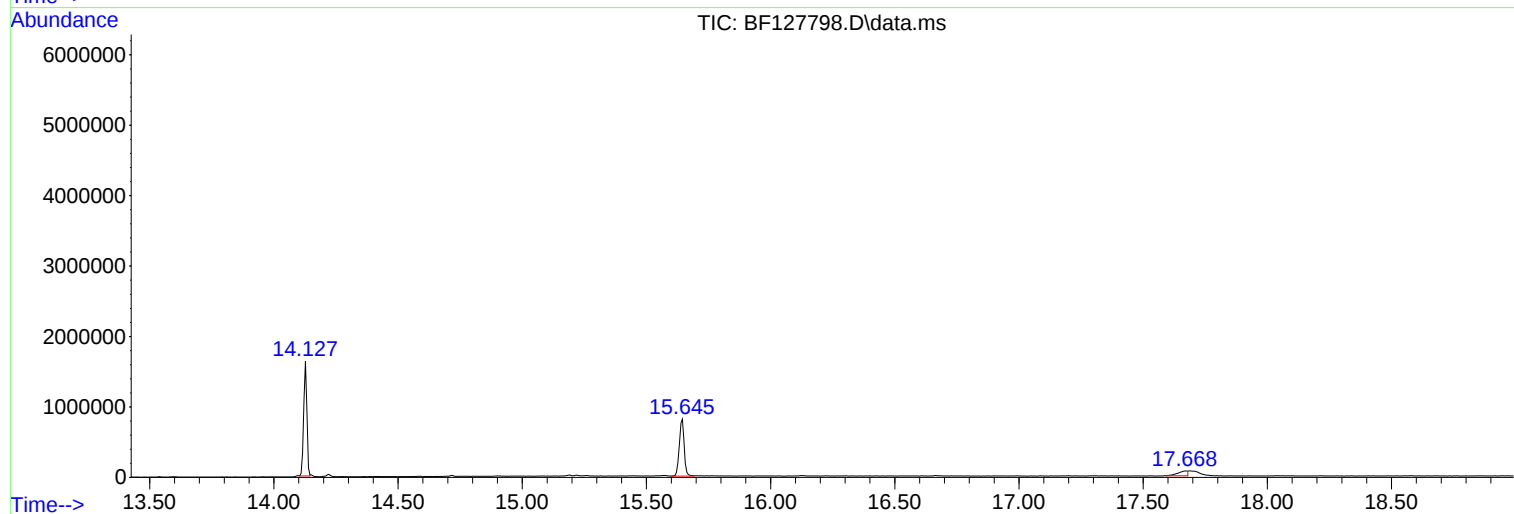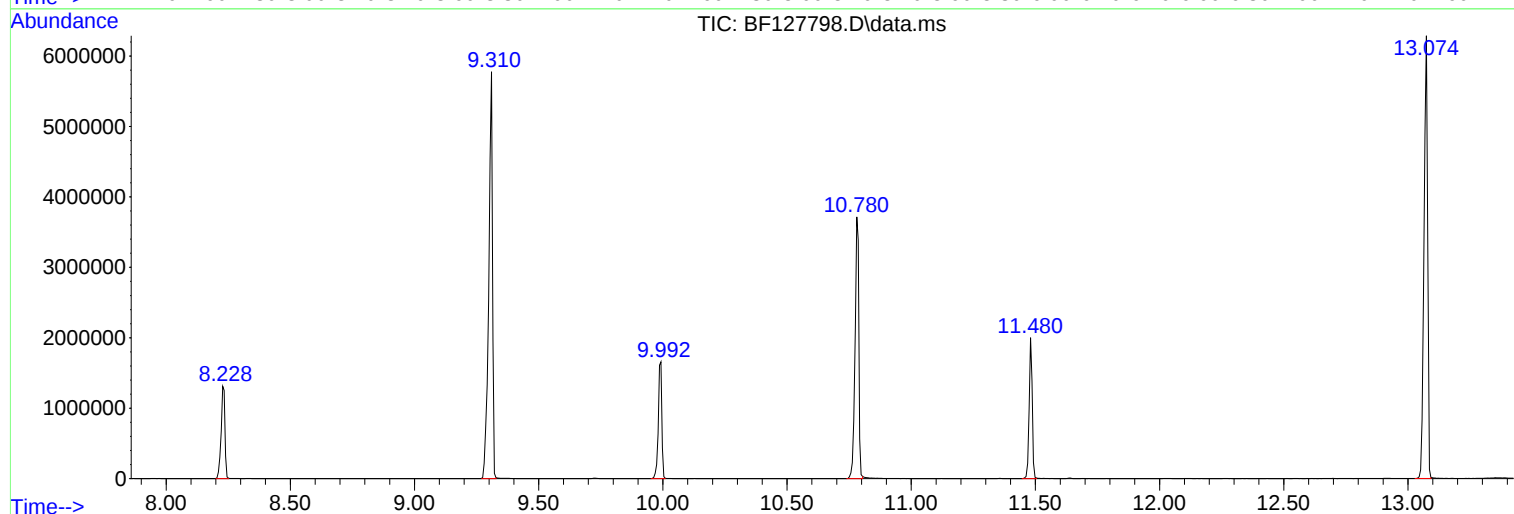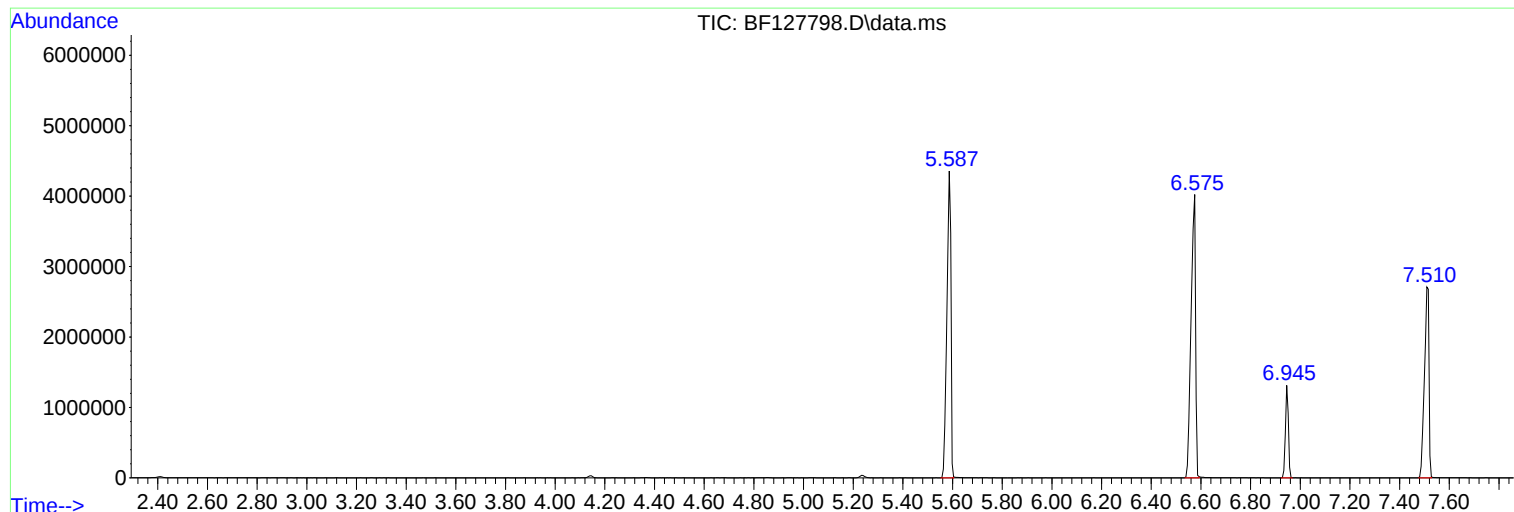

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041522\
Data File : BF127798.D
Acq On : 15 Apr 2022 11:20
Operator : CG\JU
Sample : PB144095TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144095TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041522\
Data File : BF127798.D
Acq On : 15 Apr 2022 11:20
Operator : CG\JU
Sample : PB144095TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144095TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------