

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041522\
 Data File : BF127801.D
 Acq On : 15 Apr 2022 14:08
 Operator : CG\JU
 Sample : N2432-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DUP220414

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127801.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.581	554	560	563	rBV	4011874	4384346	76.65%	12.651%
2	6.575	722	729	732	rBV	3886791	4487978	78.46%	12.950%
3	6.945	788	792	796	rBV	1166629	923799	16.15%	2.666%
4	7.510	882	888	891	rBV	2825280	3079044	53.83%	8.884%
5	8.228	1006	1010	1014	rBV	1263595	1203557	21.04%	3.473%
6	9.310	1188	1194	1197	rBV	4966708	5508425	96.30%	15.894%
7	9.992	1304	1310	1313	rBV	1457182	1465788	25.63%	4.229%
8	10.780	1438	1444	1448	rBV	3458561	3773323	65.97%	10.888%
9	11.480	1558	1563	1567	rBV	1751532	1565674	27.37%	4.518%
10	13.074	1829	1834	1837	rBV	5770276	5720034	100.00%	16.505%
11	13.968	1982	1986	1996	rBV2	160256	283883	4.96%	0.819%
12	14.127	2009	2013	2017	rVB	1405259	1254776	21.94%	3.621%
13	15.645	2266	2271	2280	rVB2	791297	1006437	17.59%	2.904%


Sum of corrected areas: 34657064

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041522\
Data File : BF127801.D
Acq On : 15 Apr 2022 14:08
Operator : CG\JU
Sample : N2432-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DUP220414

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

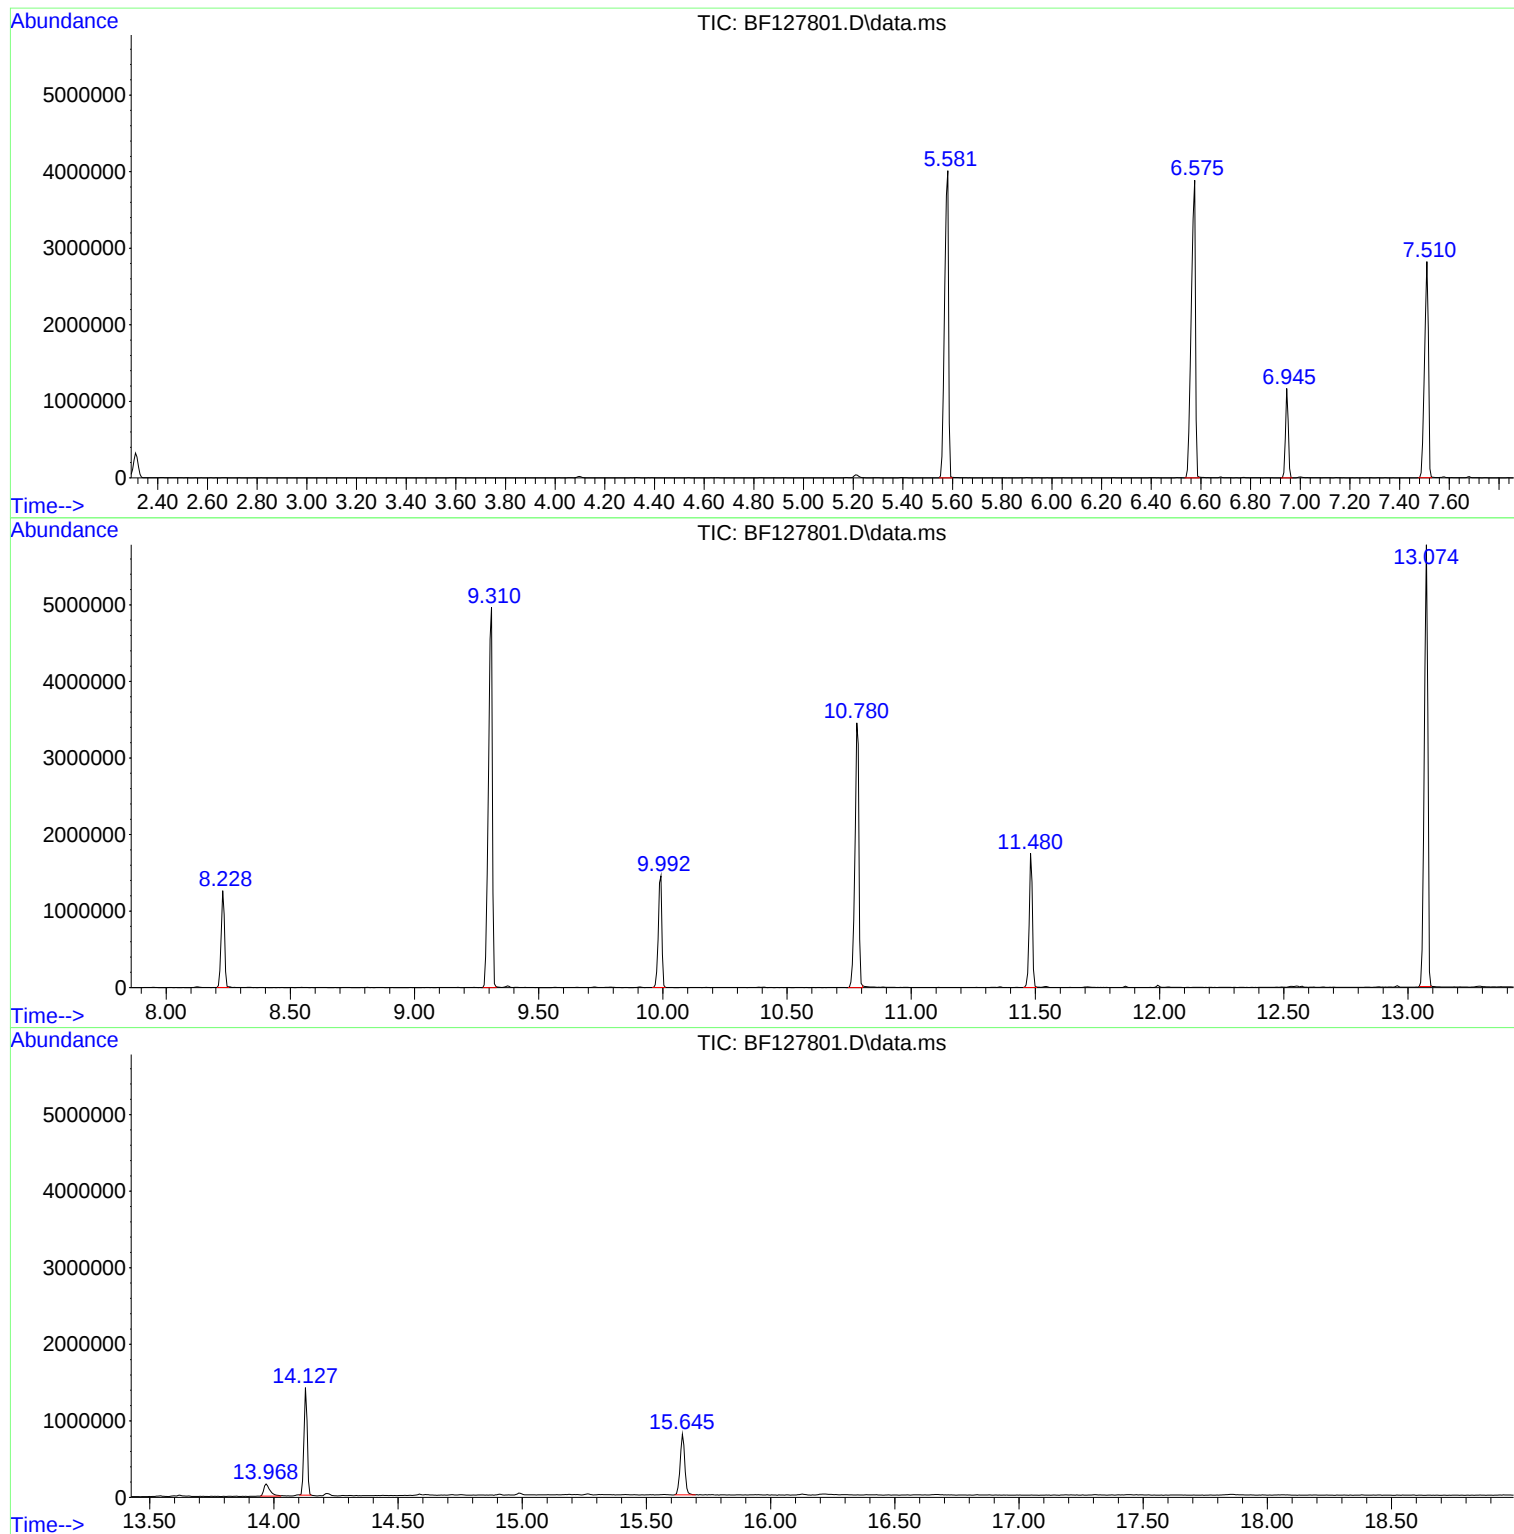

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041522\
Data File : BF127801.D
Acq On : 15 Apr 2022 14:08
Operator : CG\JU
Sample : N2432-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DUP220414










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Behenic alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.968	4.52 ng	283883	Chrysene-d12	14.127

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Behenic alcohol	326	C22H46O	000661-19-8	94
2			n-Tetracosanol-1	354	C24H50O	000506-51-4	91
3			1-Docosene	308	C22H44	001599-67-3	91
4			n-Heptadecanol-1	256	C17H36O	001454-85-9	90
5			n-Nonadecanol-1	284	C19H40O	001454-84-8	90

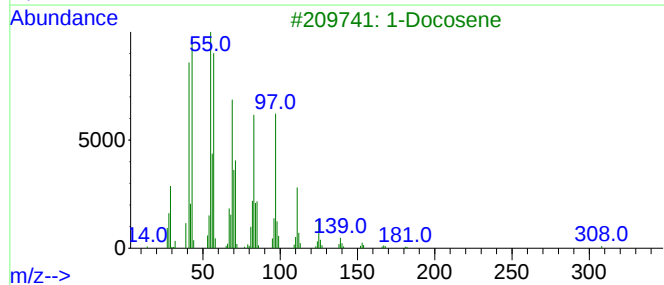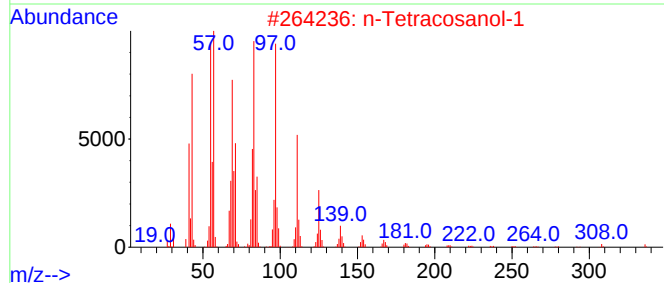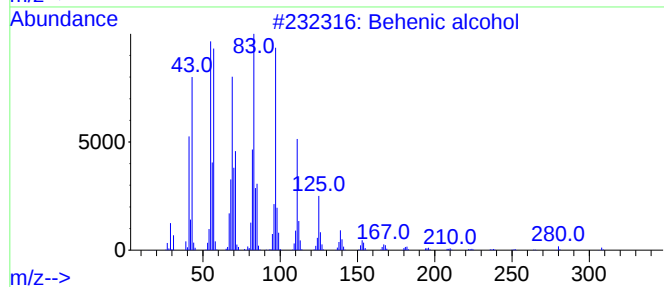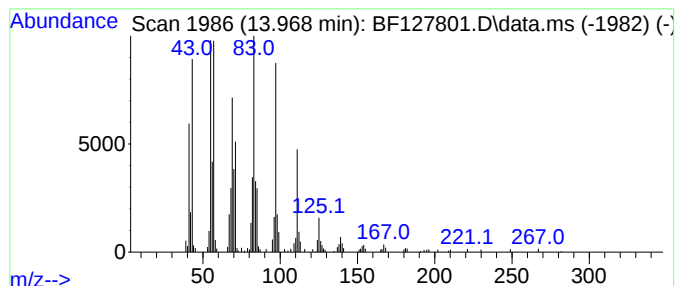

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041522\
Data File : BF127801.D
Acq On : 15 Apr 2022 14:08
Operator : CG\JU
Sample : N2432-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DUP220414

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Behenic alcohol	13.968	4.5	ng	283883	5	14.127	1254780	20.0