

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041522\
 Data File : BF127802.D
 Acq On : 15 Apr 2022 14:36
 Operator : CG\JU
 Sample : N2432-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-6075

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127802.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.581	554	560	563	rBV	3631569	4065410	77.97%	13.095%
2	6.575	722	729	732	rBV	3580308	4221036	80.95%	13.596%
3	6.946	789	792	796	rVB	1060668	862971	16.55%	2.780%
4	7.510	882	888	891	rBV	2621190	2918947	55.98%	9.402%
5	8.228	1006	1010	1014	rBV	1143821	1124442	21.56%	3.622%
6	9.310	1188	1194	1197	rBV	5287255	5214340	100.00%	16.796%
7	9.987	1305	1309	1313	rBV	1428885	1337724	25.65%	4.309%
8	10.781	1439	1444	1447	rBV	3455833	3328657	63.84%	10.722%
9	11.481	1559	1563	1567	rBV	1658209	1357889	26.04%	4.374%
10	13.075	1829	1834	1837	rBV	4521332	4638681	88.96%	14.941%
11	13.969	1982	1986	1997	rBV2	124055	229396	4.40%	0.739%
12	14.127	2009	2013	2017	rBV	929078	833554	15.99%	2.685%
13	15.645	2265	2271	2278	rBV	687348	912855	17.51%	2.940%




Sum of corrected areas: 31045902

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041522\
Data File : BF127802.D
Acq On : 15 Apr 2022 14:36
Operator : CG\JU
Sample : N2432-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-6075

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

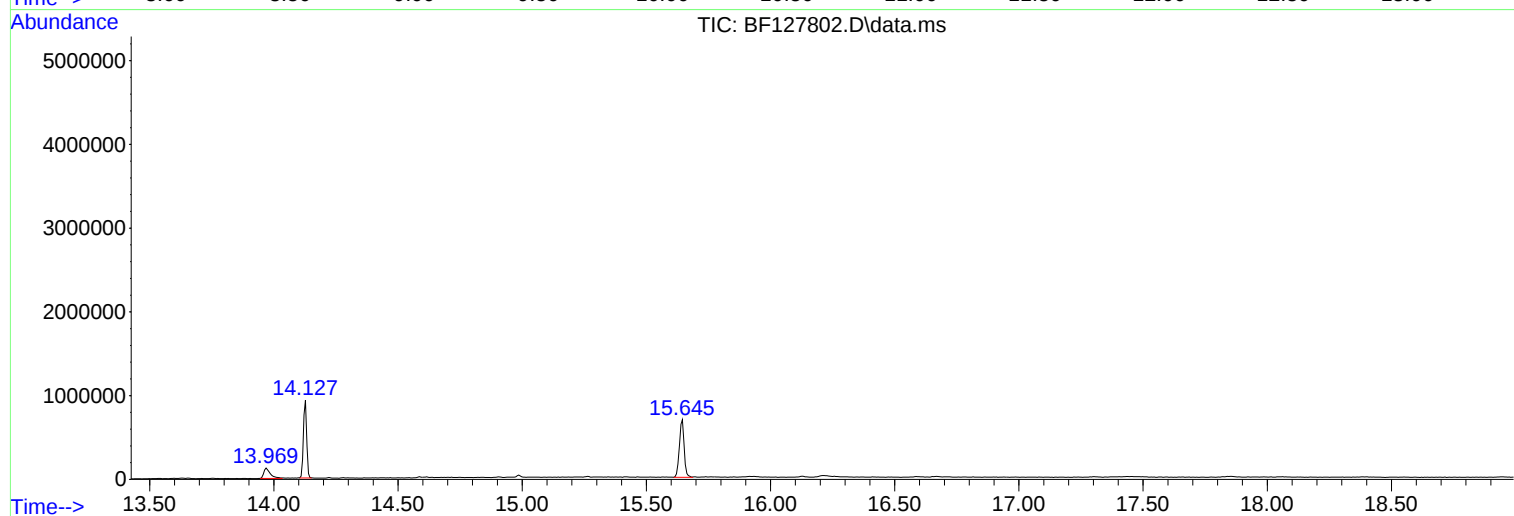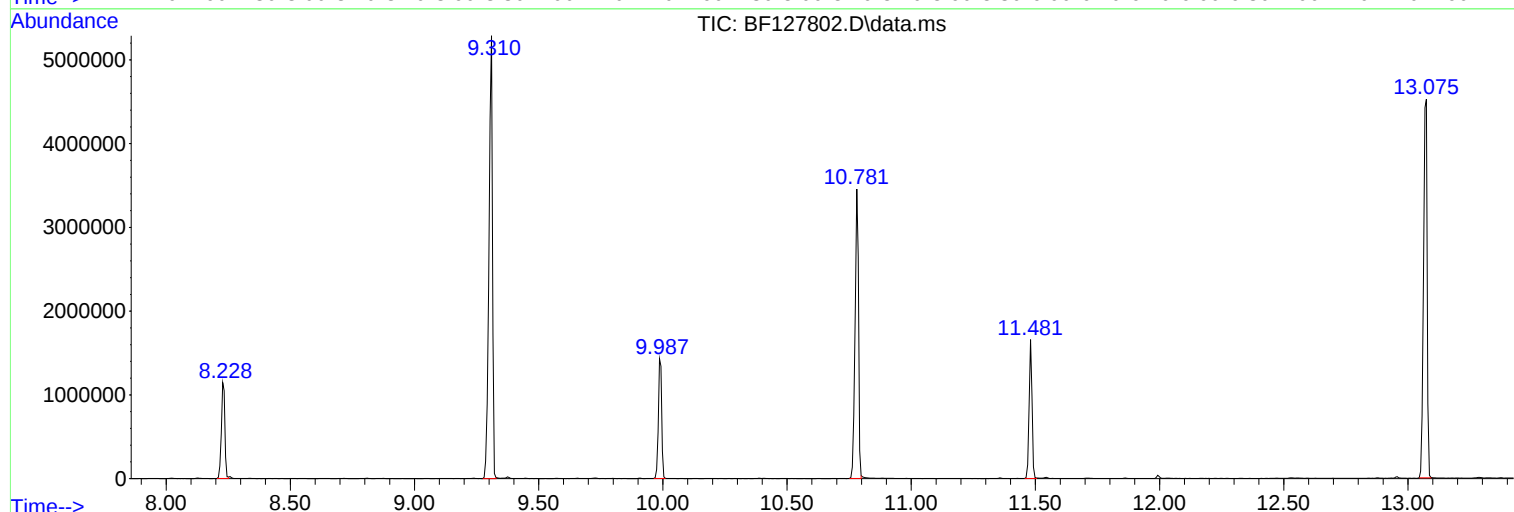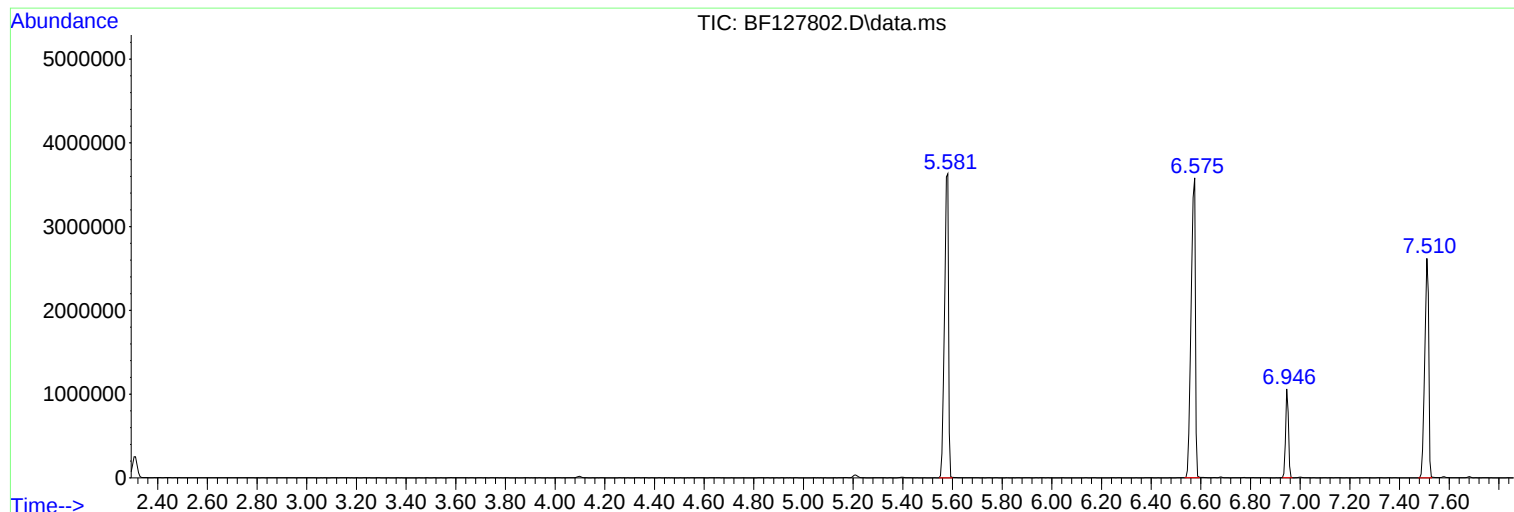

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041522\
Data File : BF127802.D
Acq On : 15 Apr 2022 14:36
Operator : CG\JU
Sample : N2432-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-6075










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 n-Tetracosanol-1 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.969	5.50 ng	229396	Chrysene-d12	14.127

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			n-Tetracosanol-1	354	C24H50O	000506-51-4	94
2			Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	94
3			Behenic alcohol	326	C22H46O	000661-19-8	94
4			3-Eicosene, (E)-	280	C20H40	074685-33-9	91
5			2- Chloropropionic acid, hexadec...	332	C19H37ClO2	086711-81-1	91

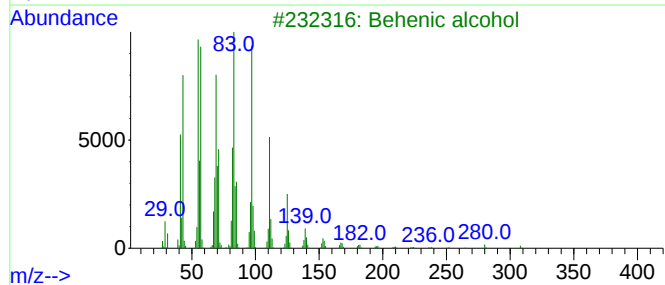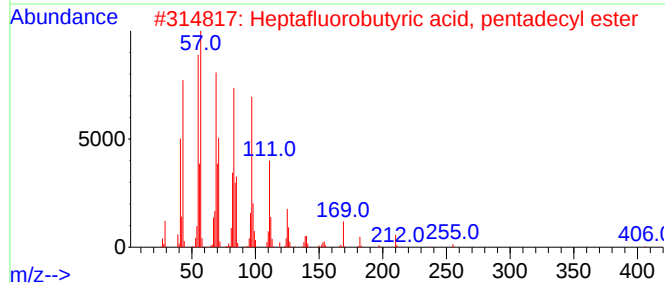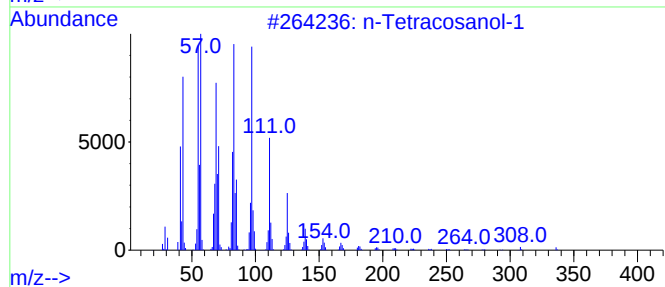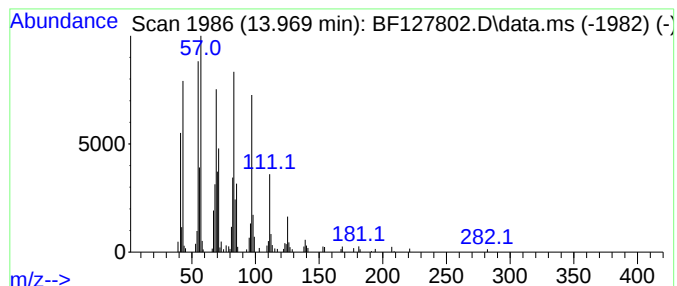

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041522\
Data File : BF127802.D
Acq On : 15 Apr 2022 14:36
Operator : CG\JU
Sample : N2432-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-6075

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
n-Tetracosanol-1	13.969	5.5	ng	229396	5	14.127	833554	20.0