

Data Path : Z:\HPCHEM1\BNA_F\Data\BF041615\
 Data File : BF078564.D
 Acq On : 16 Apr 2015 14:32
 Operator : TP/IZ
 Sample : G1889-03
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FK-GF-01-014-B

Quant Time: Apr 16 16:45:57 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 16 16:17:35 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.68	152	28840	20.00	ng	0.00
21) Naphthalene-d8	8.27	136	118345	20.00	ng	0.00
38) Acenaphthene-d10	10.42	164	62612	20.00	ng	0.00
63) Phenanthrene-d10	12.24	188	122937	20.00	ng	0.00
75) Chrysene-d12	15.49	240	132716	20.00	ng	0.00
86) Perylene-d12	17.20	264	139347	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	4.91	112	139969	80.02	ng	0.01
7) Phenol-d6	6.30	99	181783	82.93	ng	0.00
23) Nitrobenzene-d5	7.39	82	107795	55.21	ng	0.00
41) 2,4,6-Tribromophenol	11.39	330	46233	89.03	ng	0.00
44) 2-Fluorobiphenyl	9.62	172	189423	43.24	ng	0.00
78) Terphenyl-d14	14.23	244	235092	40.03	ng	0.00
Target Compounds						
49) Dimethylphthalate	10.14	163	22087	4.70	ng	# 96
74) Fluoranthene	13.73	202	19441	2.59	ng	95
77) Pyrene	14.00	202	18118	2.17	ng	# 93
87) Benzo(b)fluoranthene	16.77	252	20145	2.34	ng	# 86
88) Benzo(k)fluoranthene	16.77	252	20148	2.63	ng	# 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\Data\BF041615\
Data File : BF078564.D
Acq On : 16 Apr 2015 14:32
Operator : TP/IZ
Sample : G1889-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-GF-01-014-B

Quant Time: Apr 16 16:45:57 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 16 16:17:35 2015
Response via : Initial Calibration

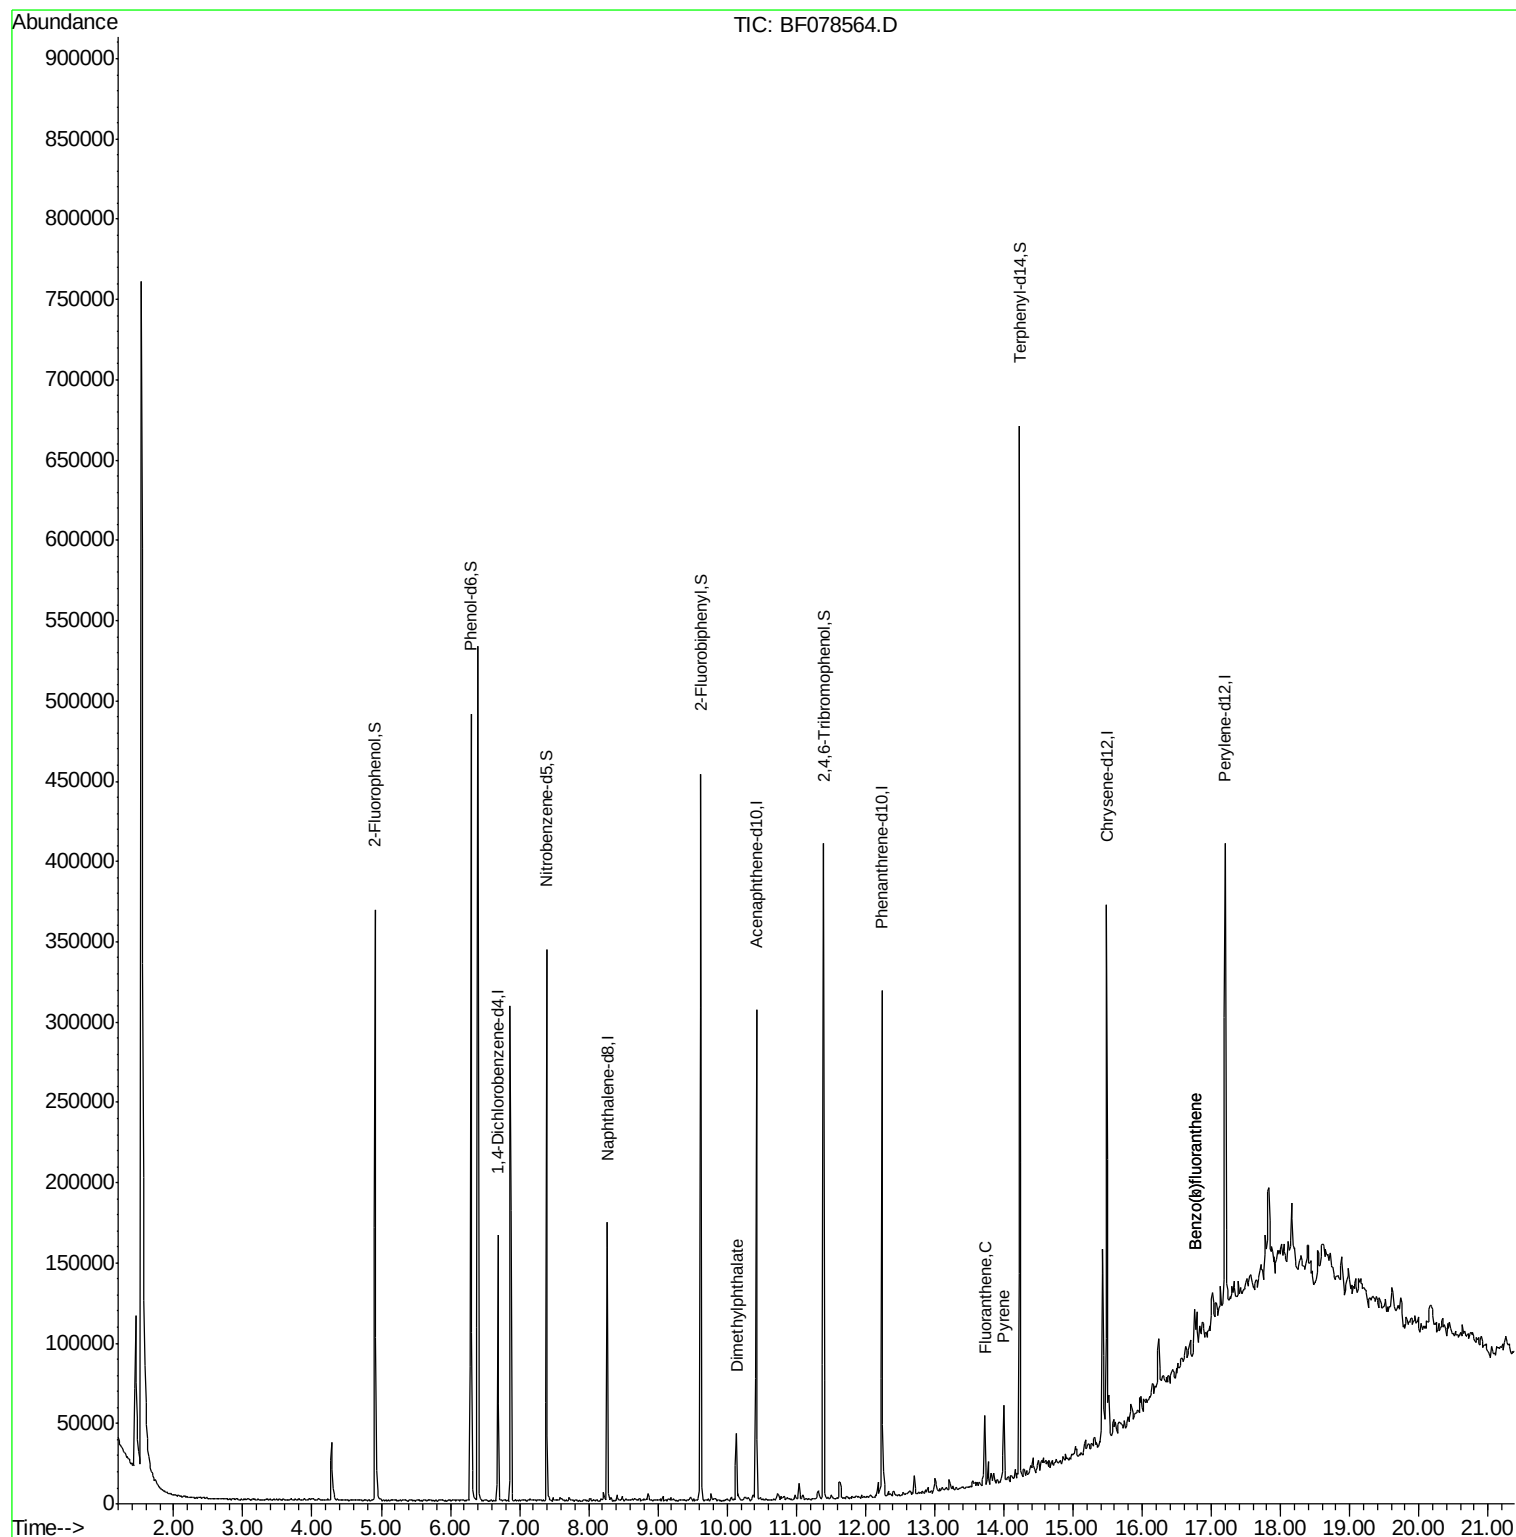

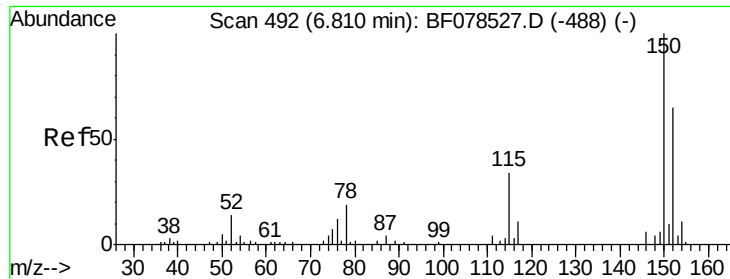


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.68 min Scan# 481
Delta R.T. 0.00 min
Lab File: BF078564.D
Acq: 16 Apr 2015 14:32

Instrument :
BNA_F
ClientSampleId :
FK-GF-01-014-B

Tgt Ion:152 Resp: 28840
Ion Ratio Lower Upper
152 100
150 158.5 125.9 188.9
115 62.3 52.7 79.1

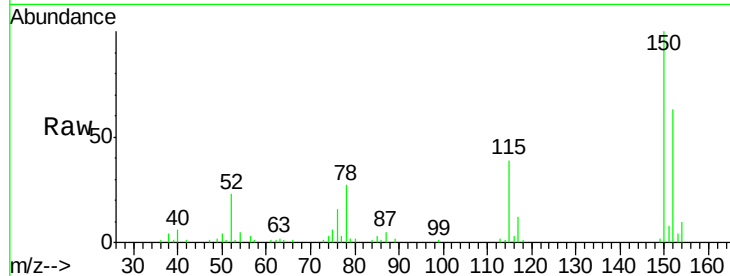


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

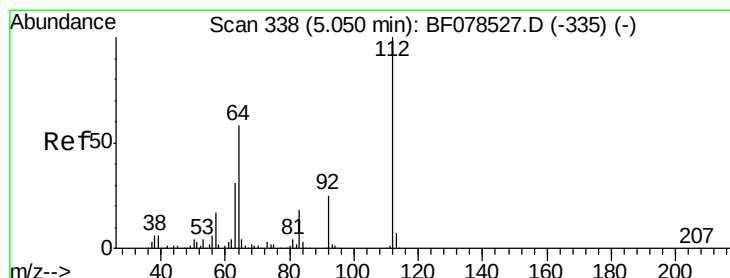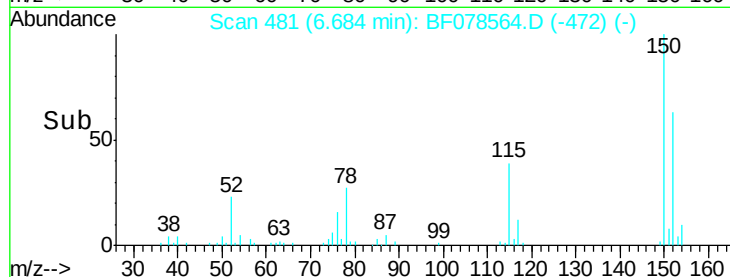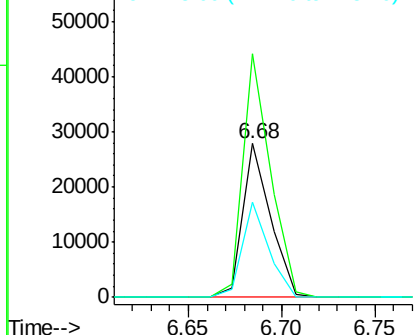



#5


2-Fluorophenol
Concen: 80.02 ng
RT: 4.91 min Scan# 326
Delta R.T. 0.01 min
Lab File: BF078564.D
Acq: 16 Apr 2015 14:32

Tgt Ion:112 Resp: 139969
Ion Ratio Lower Upper
112 100
64 53.3 39.9 59.9
63 27.5 20.2 30.4

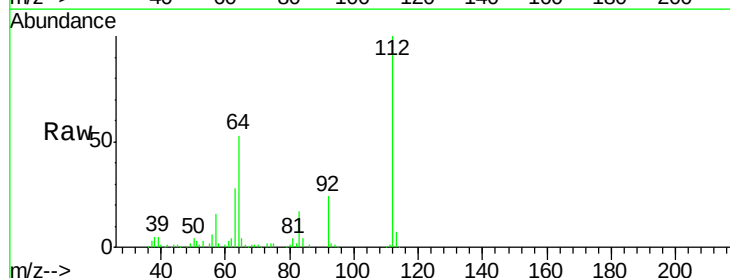

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

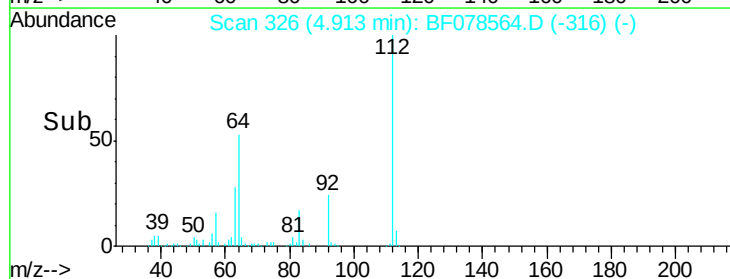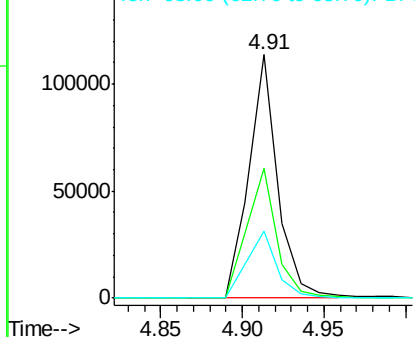

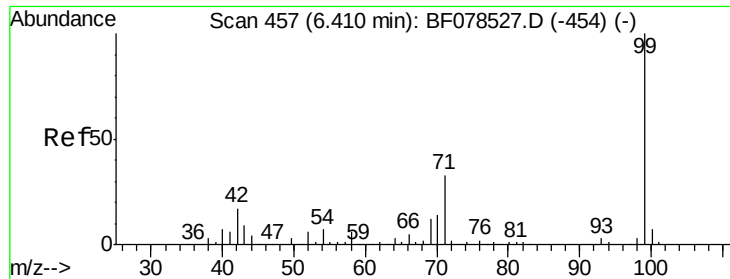

#7

Phenol-d6

Concen: 82.93 ng

RT: 6.30 min Scan# 447

Delta R.T. 0.00 min

Lab File: BF078564.D

Acq: 16 Apr 2015 14:32

Instrument :

BNA_F

ClientSampleId :

FK-GF-01-014-B


Tgt Ion: 99 Resp: 181783

Ion Ratio Lower Upper

99 100

42 17.4 14.8 22.2

71 32.9 26.6 39.8

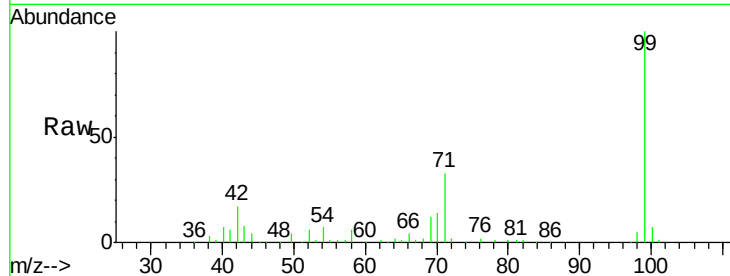

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

250000

200000

150000



100000

50000

0

6.25 6.30 6.35

Time-->

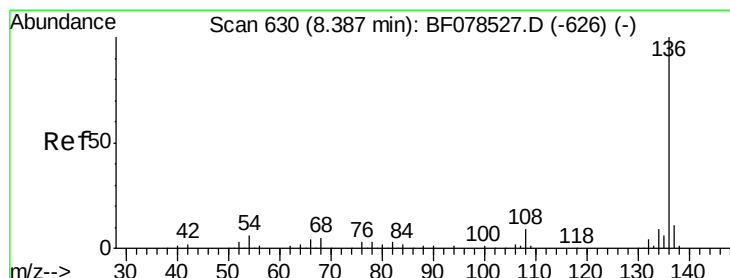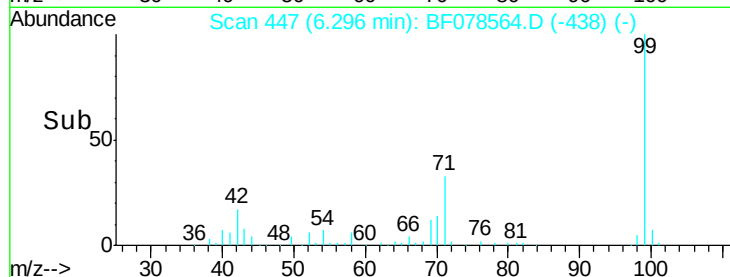

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.27 min Scan# 620

Delta R.T. 0.00 min

Lab File: BF078564.D

Acq: 16 Apr 2015 14:32

Tgt Ion: 136 Resp: 118345


Ion Ratio Lower Upper

136 100

137 10.0 9.0 13.4

54 5.3 7.0 10.6#

68 4.7 5.4 8.2#

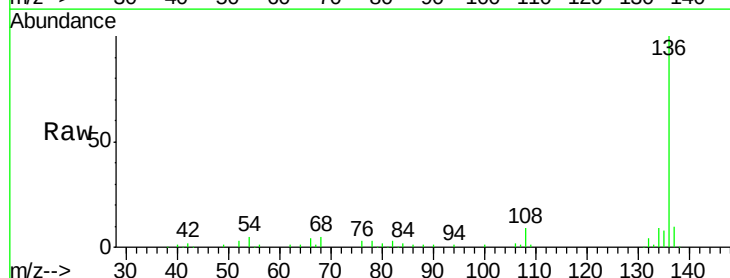

Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0


100000


50000

0

8.20 8.25 8.30 8.35

Time-->

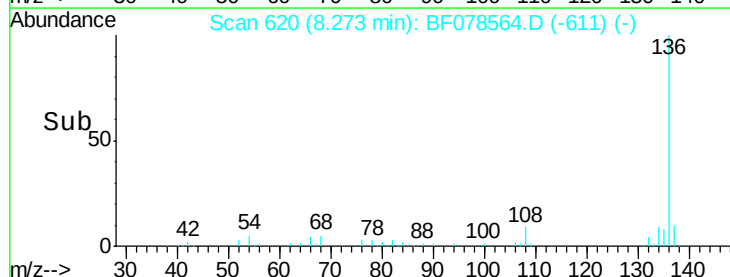


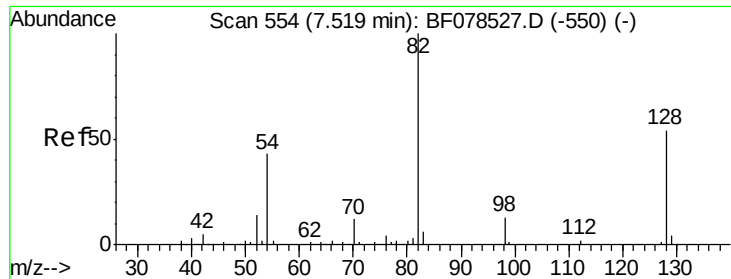




#23
 Nitrobenzene-d5
 Concen: 55.21 ng
 RT: 7.39 min Scan# 543
 Delta R.T. 0.00 min
 Lab File: BF078564.D
 Acq: 16 Apr 2015 14:32

Instrument :
 BNA_F
 ClientSampleId :
 FK-GF-01-014-B

Tgt Ion: 82 Resp: 107795
 Ion Ratio Lower Upper
 82 100
 128 45.7 31.8 47.8
 54 49.0 41.5 62.3

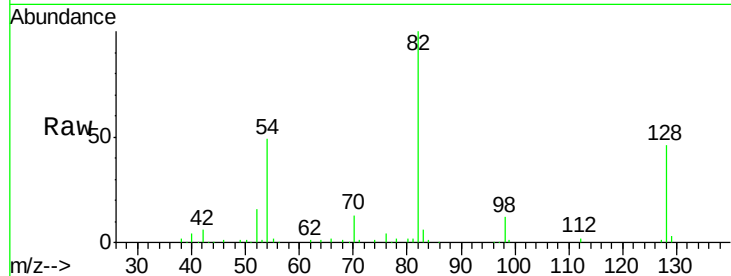


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): B
 Ion 54.00 (53.70 to 54.70): BF0

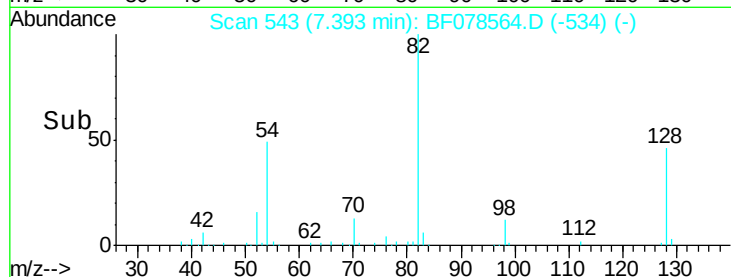
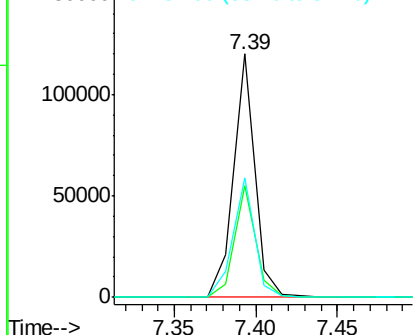



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.42 min Scan# 808
 Delta R.T. 0.00 min
 Lab File: BF078564.D
 Acq: 16 Apr 2015 14:32

Tgt Ion: 164 Resp: 62612
 Ion Ratio Lower Upper
 164 100
 162 101.9 82.2 123.2
 160 44.1 34.7 52.1



Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

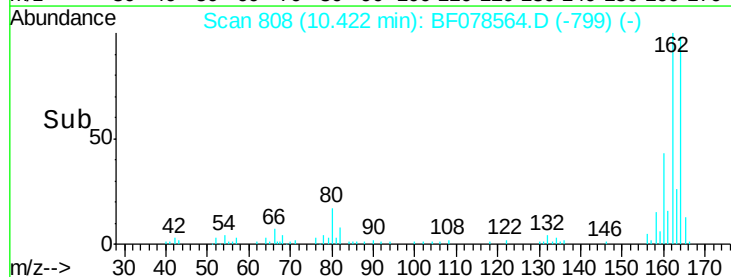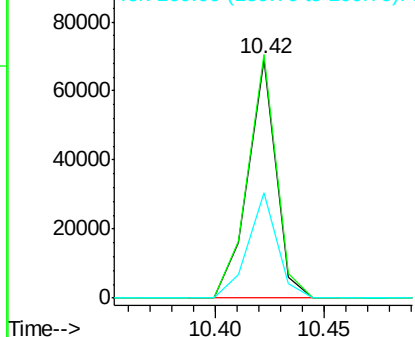


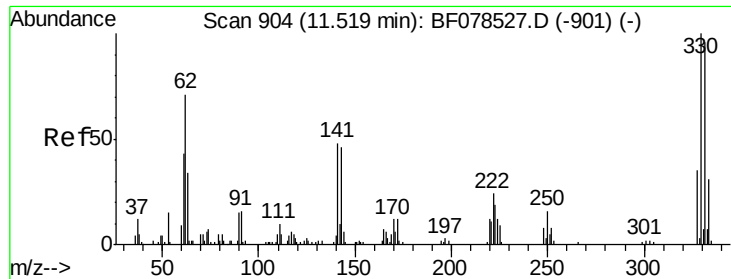




#41
 2,4,6-Tribromophenol
 Concen: 89.03 ng
 RT: 11.39 min Scan# 893
 Delta R.T. 0.00 min
 Lab File: BF078564.D
 Acq: 16 Apr 2015 14:32

Instrument :
 BNA_F
 ClientSampleId :
 FK-GF-01-014-B

Tgt Ion:330 Resp: 46233
 Ion Ratio Lower Upper
 330 100
 332 95.1 78.6 117.8
 141 40.0 31.2 46.8




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

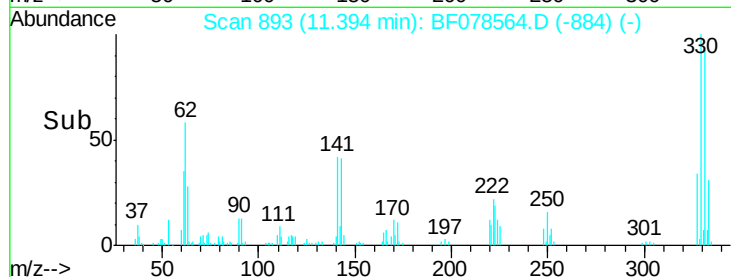
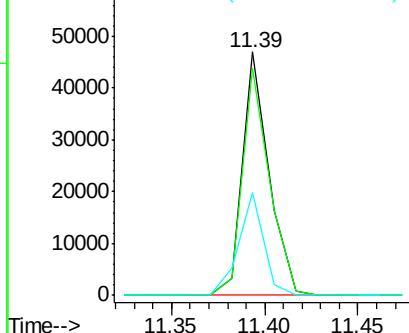



#44
 2-Fluorobiphenyl
 Concen: 43.24 ng
 RT: 9.62 min Scan# 738
 Delta R.T. 0.00 min
 Lab File: BF078564.D
 Acq: 16 Apr 2015 14:32

Tgt Ion:172 Resp: 189423
 Ion Ratio Lower Upper
 172 100
 171 35.6 28.6 42.8
 170 23.1 18.5 27.7



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

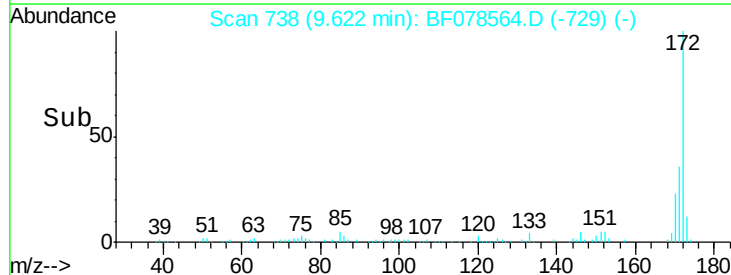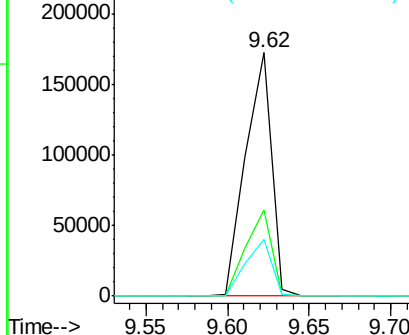

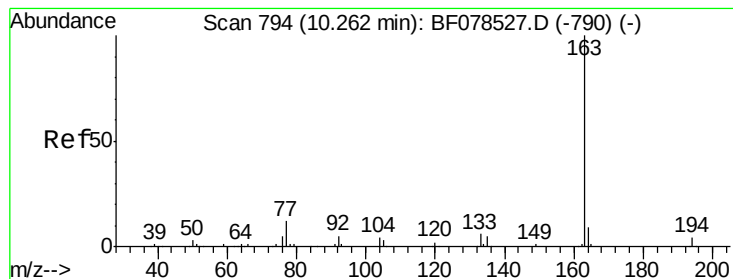

#49

Dimethylphthalate

Concen: 4.70 ng

RT: 10.14 min Scan# 783

Delta R.T. 0.00 min

Lab File: BF078564.D

Acq: 16 Apr 2015 14:32

Instrument :

BNA_F

ClientSampleId :

FK-GF-01-014-B


Tgt Ion:163 Resp: 22087

Ion Ratio Lower Upper

163 100

194 3.8 2.3 3.5#




164 9.2 8.6 13.0

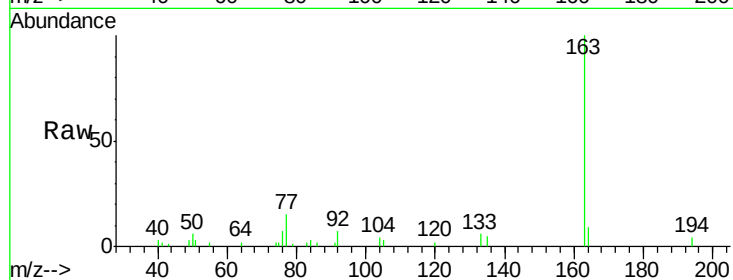

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

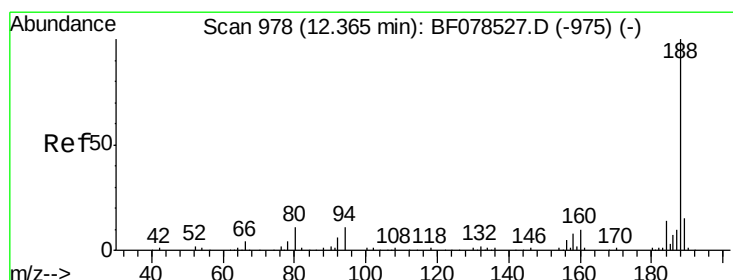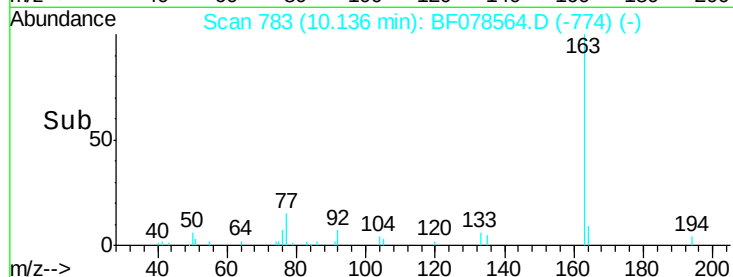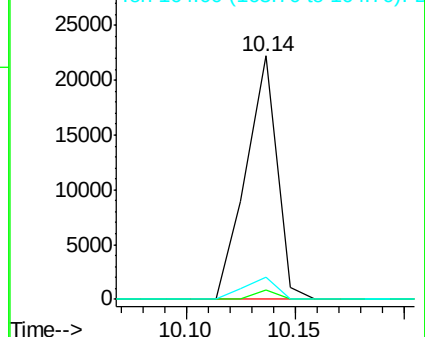

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 12.24 min Scan# 967

Delta R.T. 0.00 min

Lab File: BF078564.D

Acq: 16 Apr 2015 14:32


Tgt Ion:188 Resp: 122937

Ion Ratio Lower Upper

188 100

94 9.1 9.0 13.4



80 9.9 9.5 14.3

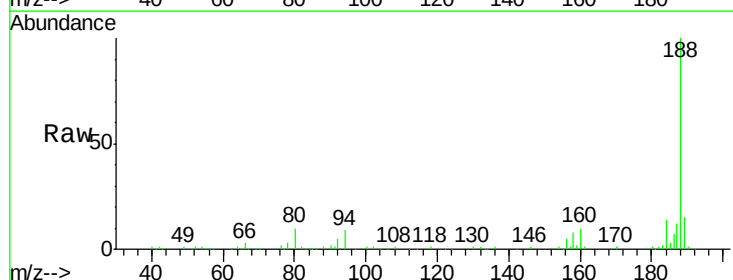


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0



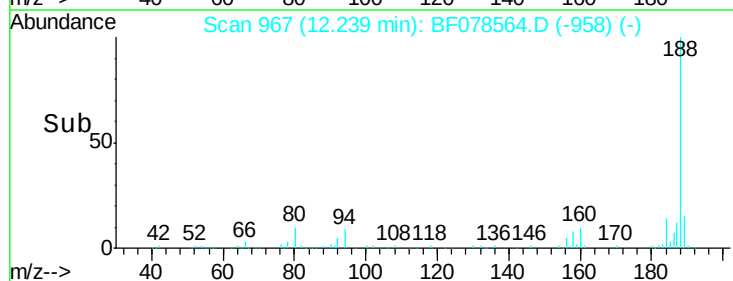
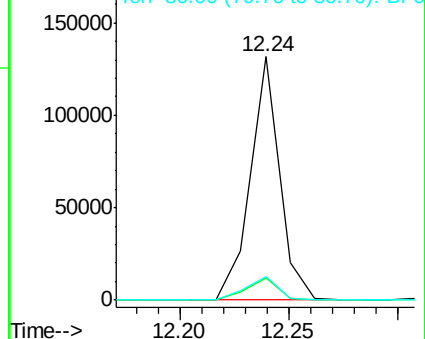


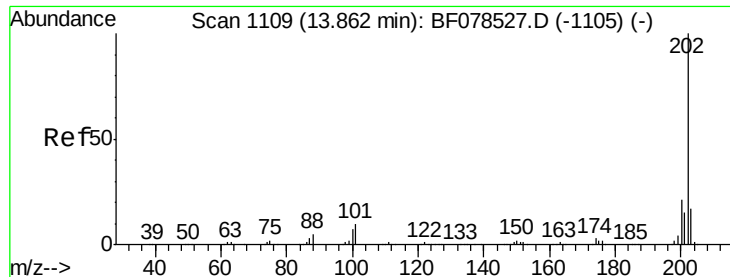

#74
Fluoranthene
Concen: 2.59 ng
RT: 13.73 min Scan# 1097
Delta R.T. 0.00 min
Lab File: BF078564.D
Acq: 16 Apr 2015 14:32




Instrument :
BNA_F
ClientSampleId :
FK-GF-01-014-B


Tgt Ion: 202 Resp: 19441
Ion Ratio Lower Upper
202 100
101 12.0 0.0 35.2
203 17.3 0.0 38.5

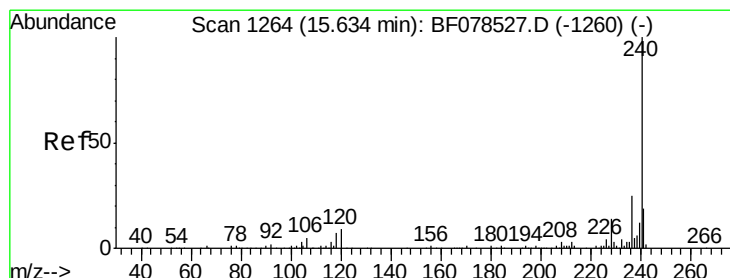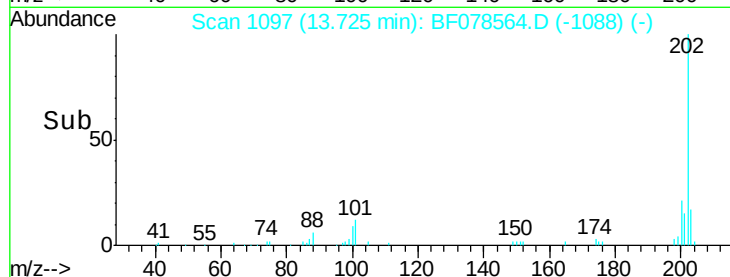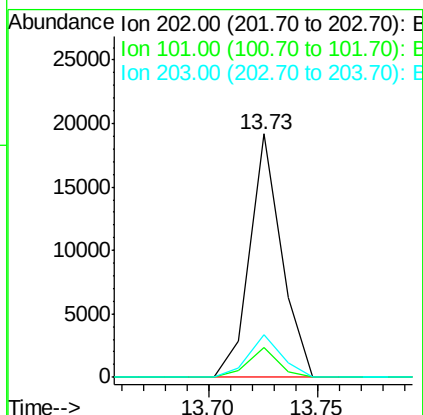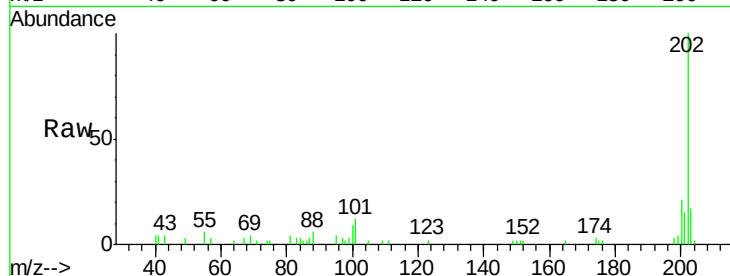

#75
Chrysene-d12
Concen: 20.00 ng
RT: 15.49 min Scan# 1251
Delta R.T. 0.00 min
Lab File: BF078564.D
Acq: 16 Apr 2015 14:32

Tgt Ion: 240 Resp: 132716
Ion Ratio Lower Upper
240 100
120 14.4 7.1 10.7#
236 25.5 21.4 32.2


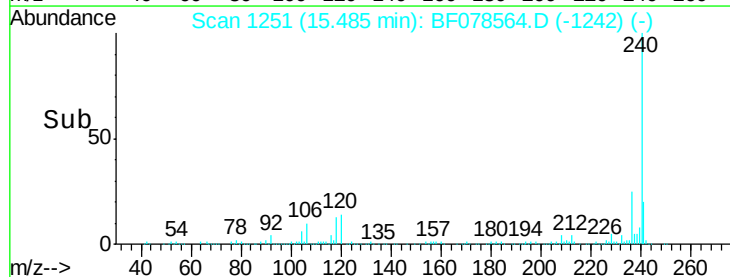
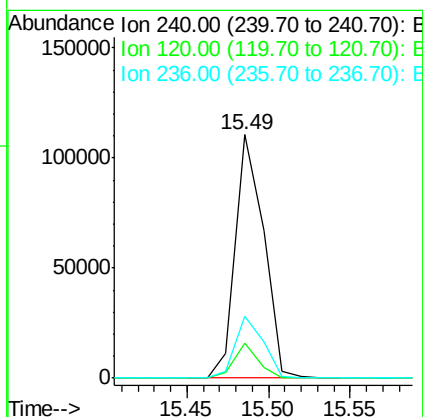
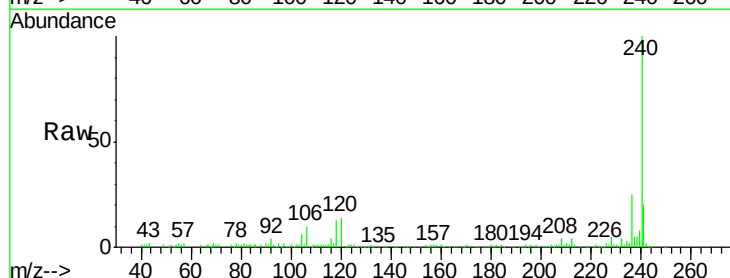


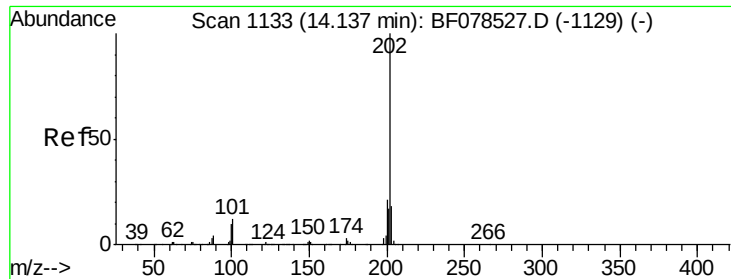

#77
 Pyrene
 Concen: 2.17 ng
 RT: 14.00 min Scan# 1121
 Delta R.T. 0.00 min
 Lab File: BF078564.D
 Acq: 16 Apr 2015 14:32




Instrument :
 BNA_F
 ClientSampleId :
 FK-GF-01-014-B


Tgt Ion	Ratio	Lower	Upper
202	100		
200	22.8	16.3	24.5
203	20.8	13.8	20.6#

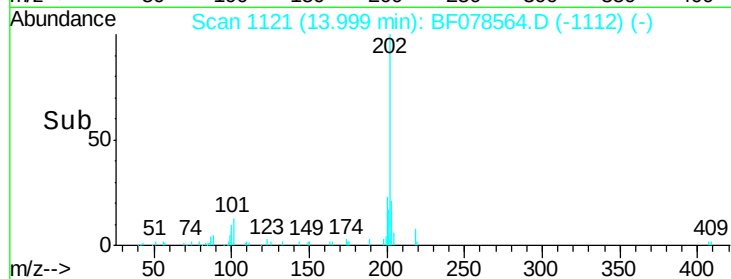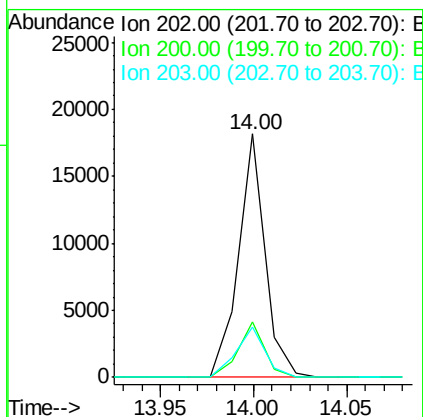

#78
 Terphenyl-d14
 Concen: 40.03 ng
 RT: 14.23 min Scan# 1141
 Delta R.T. 0.00 min
 Lab File: BF078564.D
 Acq: 16 Apr 2015 14:32

Tgt Ion	Ratio	Lower	Upper
244	100		
212	6.8	5.0	7.4
122	12.7	7.1	10.7#

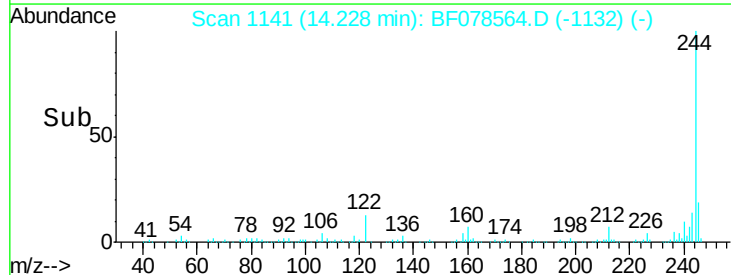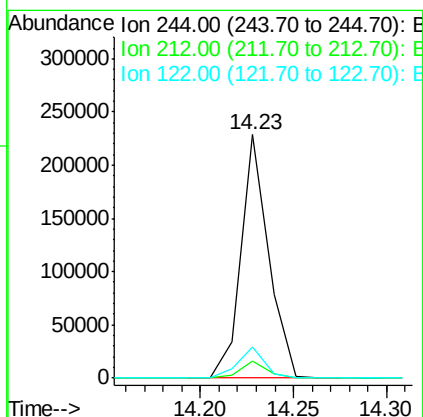


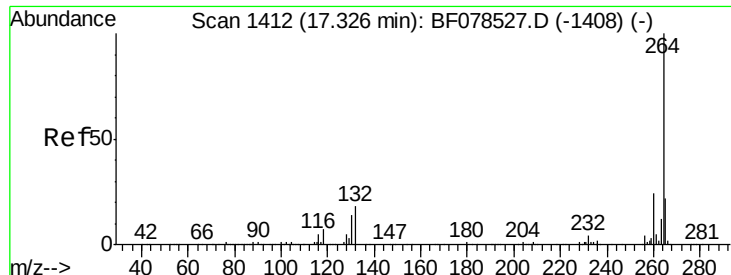




#86
Perylene-d12
Concen: 20.00 ng
RT: 17.20 min Scan# 1401
Delta R.T. 0.01 min
Lab File: BF078564.D
Acq: 16 Apr 2015 14:32

Instrument :
BNA_F
ClientSampleId :
FK-GF-01-014-B

Tgt Ion:264 Resp: 139347
Ion Ratio Lower Upper
264 100
260 23.7 18.6 27.8
265 21.8 17.0 25.6

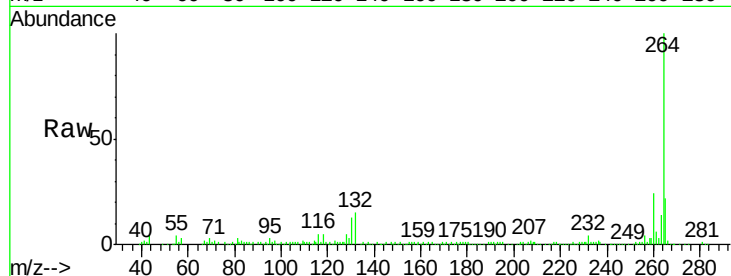


Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

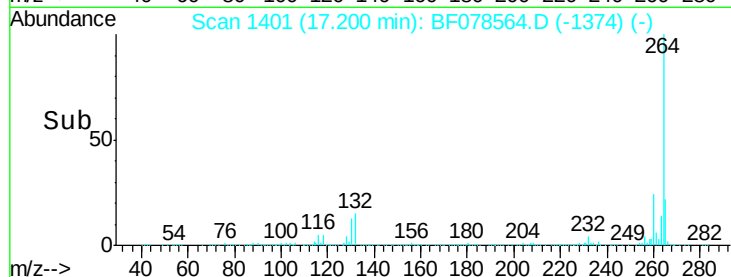
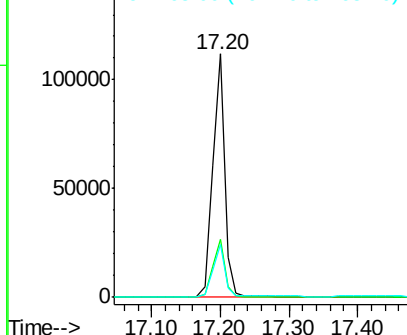



#87
Benzo(b)fluoranthene
Concen: 2.34 ng
RT: 16.77 min Scan# 1363
Delta R.T. 0.01 min
Lab File: BF078564.D
Acq: 16 Apr 2015 14:32

Tgt Ion:252 Resp: 20145
Ion Ratio Lower Upper
252 100
253 24.7 17.2 25.8
125 20.6 7.0 10.4#



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

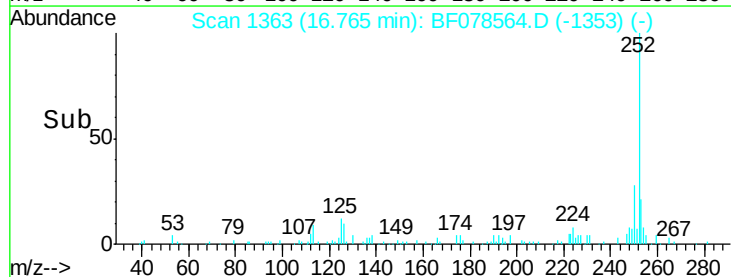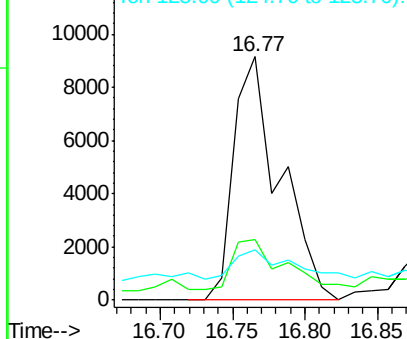


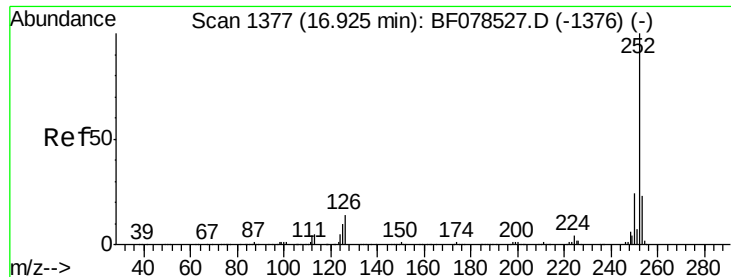

#88
 Benzo(k)fluoranthene
 Concen: 2.63 ng
 RT: 16.77 min Scan# 1363
 Delta R.T. -0.02 min
 Lab File: BF078564.D
 Acq: 16 Apr 2015 14:32

Instrument :
 BNA_F
 ClientSampleId :
 FK-GF-01-014-B

Tgt Ion:	252	Resp:	20148
Ion	Ratio	Lower	Upper
252	100		
253	24.7	17.5	26.3
125	20.6	11.6	17.4



Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

