
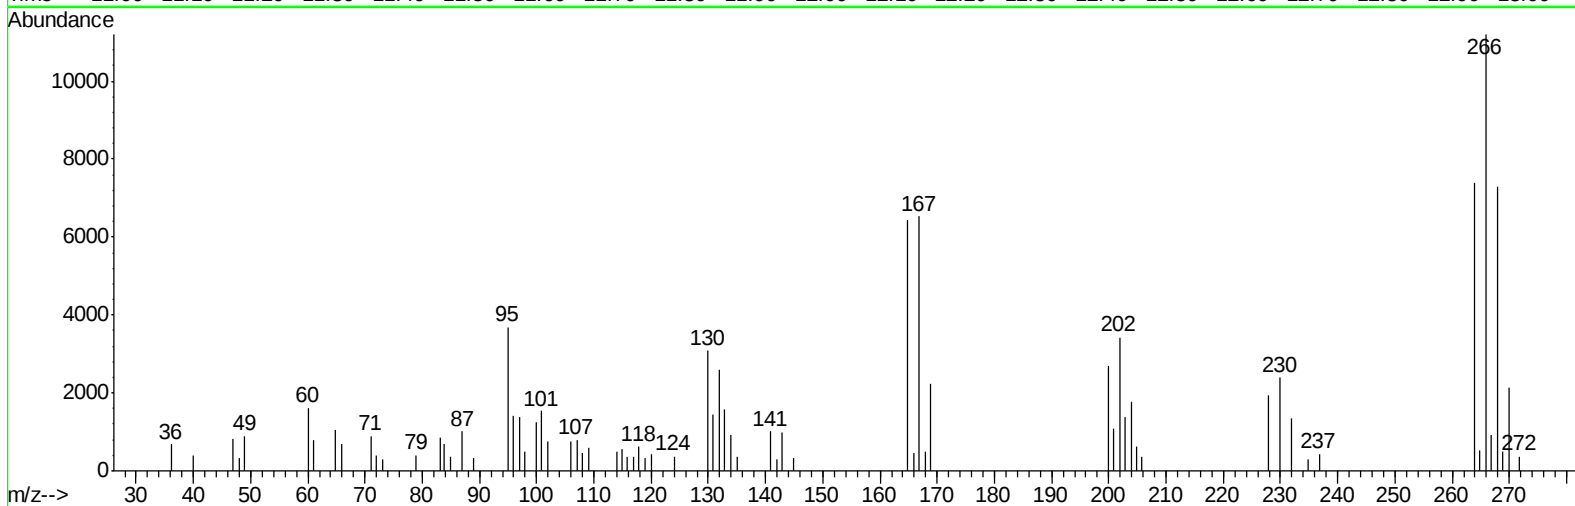


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041615\
Data File : BF078585.D
Acq On : 17 Apr 2015 1:39
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 17 09:25:47 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 17 03:45:36 2015
Response via : Initial Calibration

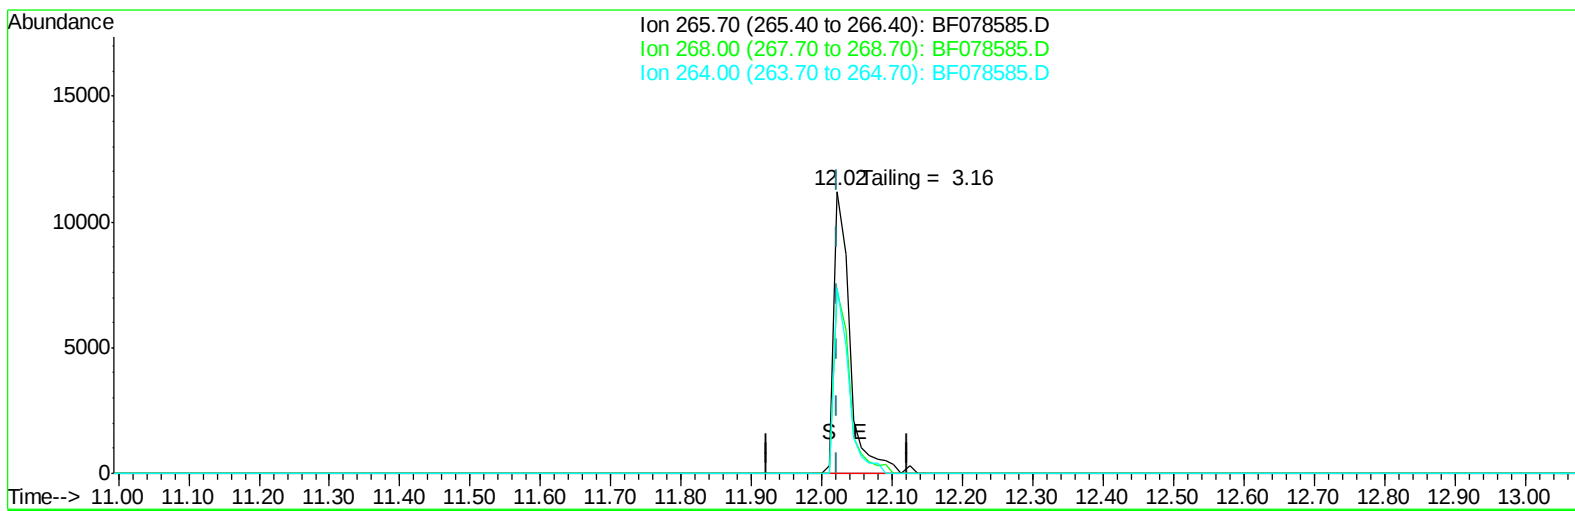

TIC: BF078585.D

(69) Pentachlorophenol (C)



12.022min (-0.000) 0.00ng

response 16878

Ion	Exp%	Act%
265.70	100	100
268.00	62.60	65.13
264.00	62.50	65.99
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041615\
Data File : BF078585.D
Acq On : 17 Apr 2015 1:39
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 17 09:25:47 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 17 03:45:36 2015
Response via : Initial Calibration

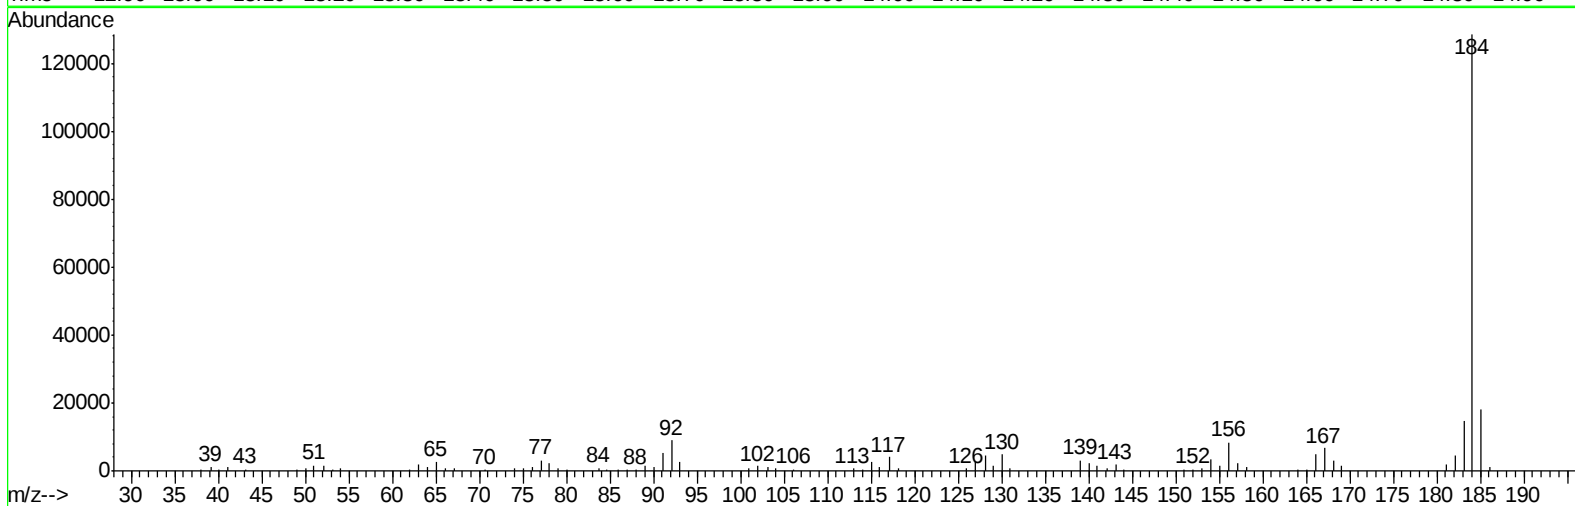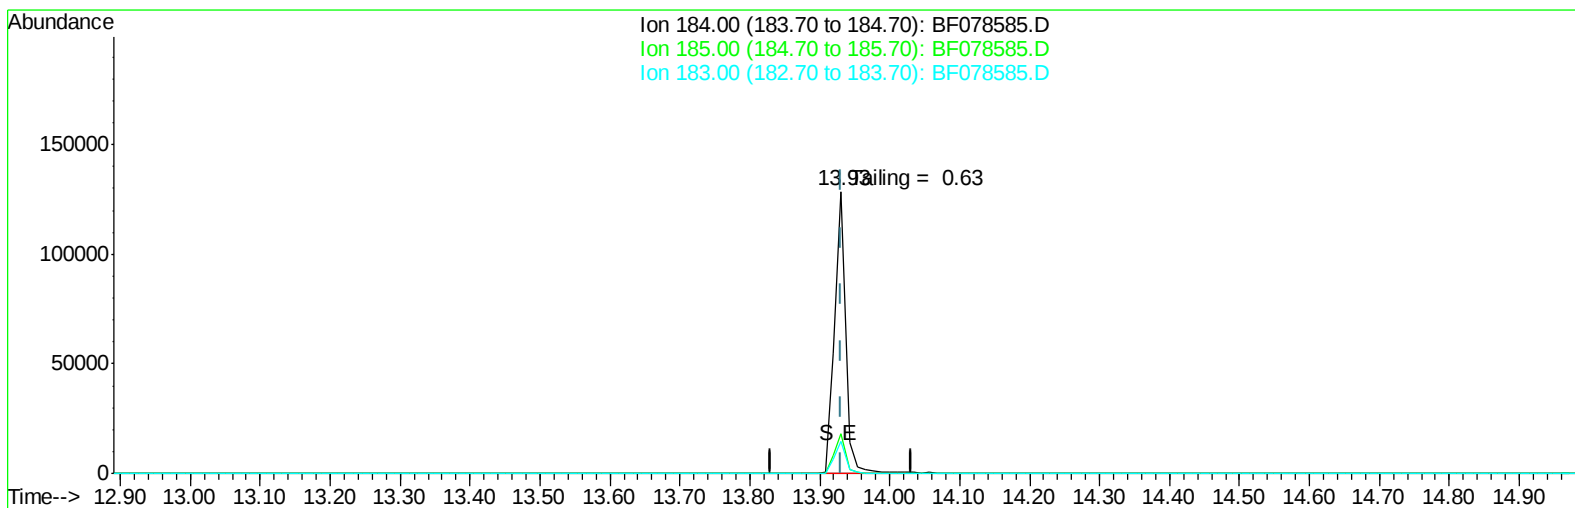

TIC: BF078585.D

(76) Benzidine

13.931min (-0.000) 0.00ng

response 140594

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.21
183.00	11.90	11.41
0.00	0.00	0.00