

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041615\
 Data File : BF078573.D
 Acq On : 16 Apr 2015 18:51
 Operator : TP/IZ
 Sample : G1891-07 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-71S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.530	28	30	53	rVB	763230	1539453	100.00%	33.892%
2	4.924	324	327	332	rBV	21027	32394	2.10%	0.713%
3	6.307	445	448	454	rVB	25470	36943	2.40%	0.813%
4	6.399	454	456	459	rBV	34968	39560	2.57%	0.871%
5	6.685	479	481	484	rVB	158933	168803	10.97%	3.716%
6	6.867	495	497	500	rBV	25198	32877	2.14%	0.724%
7	7.393	541	543	546	rBV	24013	22437	1.46%	0.494%
8	8.273	617	620	622	rBV	246089	261333	16.98%	5.753%
9	9.622	736	738	740	rBV	50797	54664	3.55%	1.203%
10	10.422	806	808	810	rBV	352252	325668	21.15%	7.170%
11	11.394	891	893	896	rBV	28110	28029	1.82%	0.617%
12	12.239	965	967	969	rBV	372773	386874	25.13%	8.517%
13	12.331	973	975	978	rVB	17261	16941	1.10%	0.373%
14	12.994	1031	1033	1035	rBV	14247	15551	1.01%	0.342%
15	13.725	1095	1097	1100	rVB	87693	90122	5.85%	1.984%
16	14.000	1119	1121	1123	rBV	100540	99753	6.48%	2.196%
17	14.114	1129	1131	1134	rBV	24346	25993	1.69%	0.572%
18	14.228	1139	1141	1143	rVB	90805	82184	5.34%	1.809%
19	14.423	1154	1158	1160	rBV	12680	19915	1.29%	0.438%
20	15.428	1240	1246	1248	rBV3	12012	36580	2.38%	0.805%
21	15.486	1248	1251	1253	rBV	407289	505280	32.82%	11.124%
22	16.743	1358	1361	1368	rBV	42939	112615	7.32%	2.479%
23	17.051	1385	1388	1390	rBV	26142	35821	2.33%	0.789%
24	17.109	1391	1393	1396	rVB	35217	48176	3.13%	1.061%
25	17.177	1396	1399	1405	rBV	388269	524246	34.05%	11.542%


Sum of corrected areas: 4542212

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041615\
Data File : BF078573.D
Acq On : 16 Apr 2015 18:51
Operator : TP/IZ
Sample : G1891-07 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-71S

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

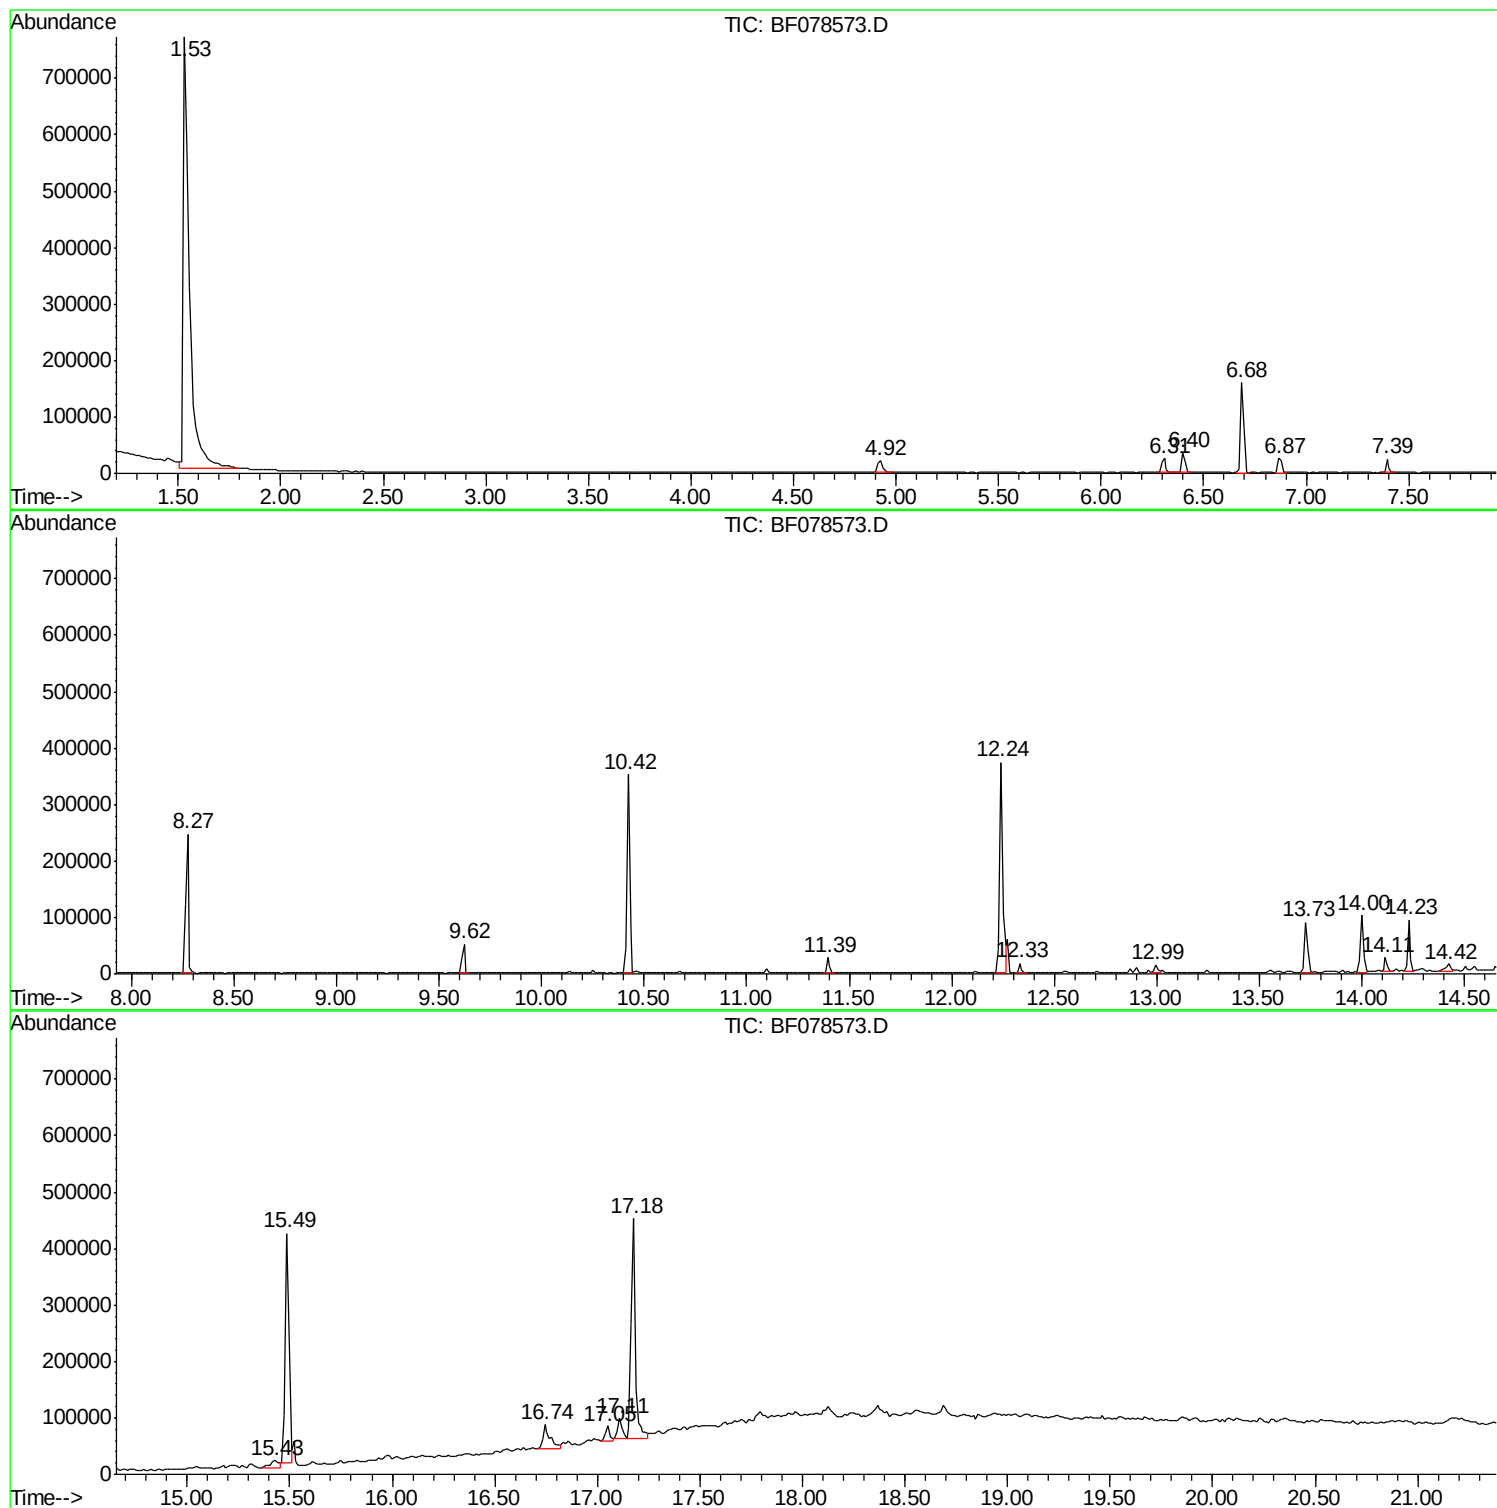

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041615\
Data File : BF078573.D
Acq On : 16 Apr 2015 18:51
Operator : TP/IZ
Sample : G1891-07 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-71S










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.40 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.40	4.69 ng	39560	1,4-Dichlorobenzene-d4	6.68

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	37
2			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3			4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
4			Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	9

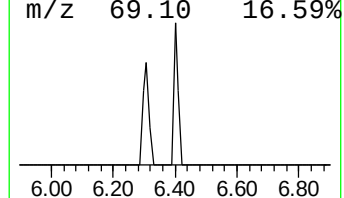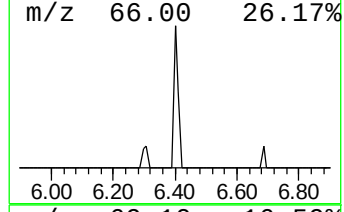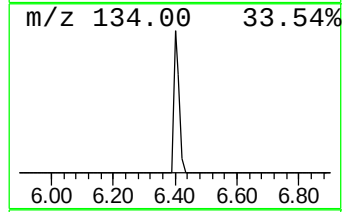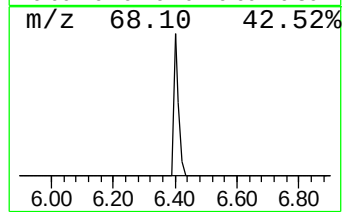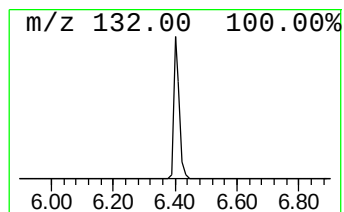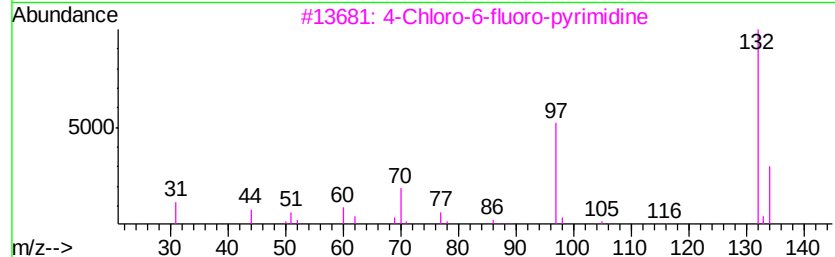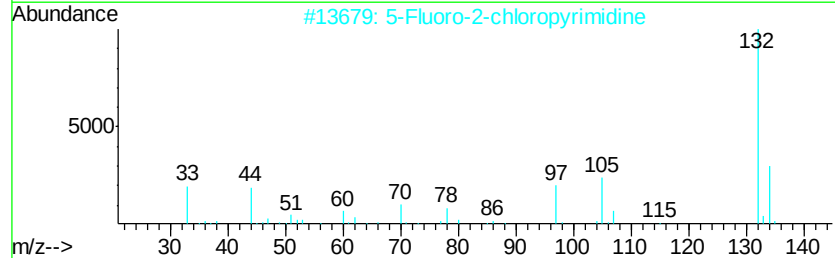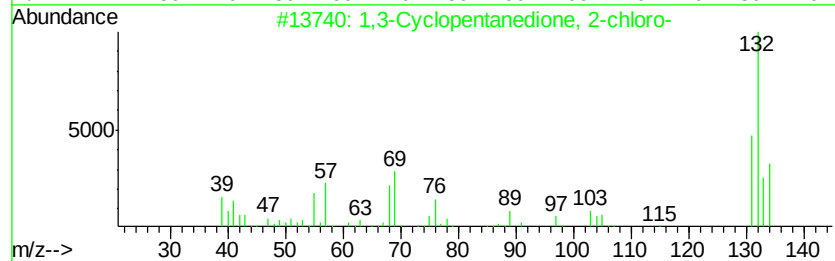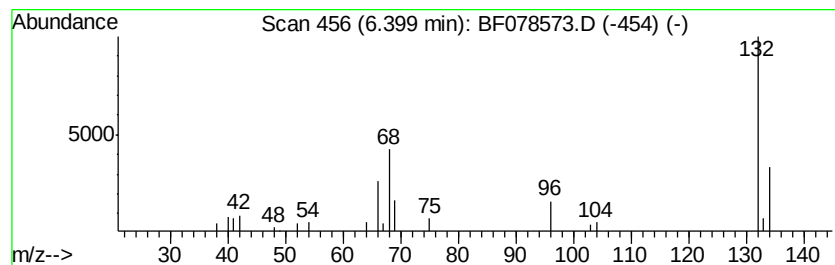

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041615\
Data File : BF078573.D
Acq On : 16 Apr 2015 18:51
Operator : TP/IZ
Sample : G1891-07 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-71S

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.40	6.40	4.7	ng	39560	1	6.68	168803	20.0