


Data Path : Z:\HPCHEM1\BNA_F\Data\BF041615\
 Data File : BF078561.D
 Acq On : 16 Apr 2015 12:24
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 31 14:58:34 2015

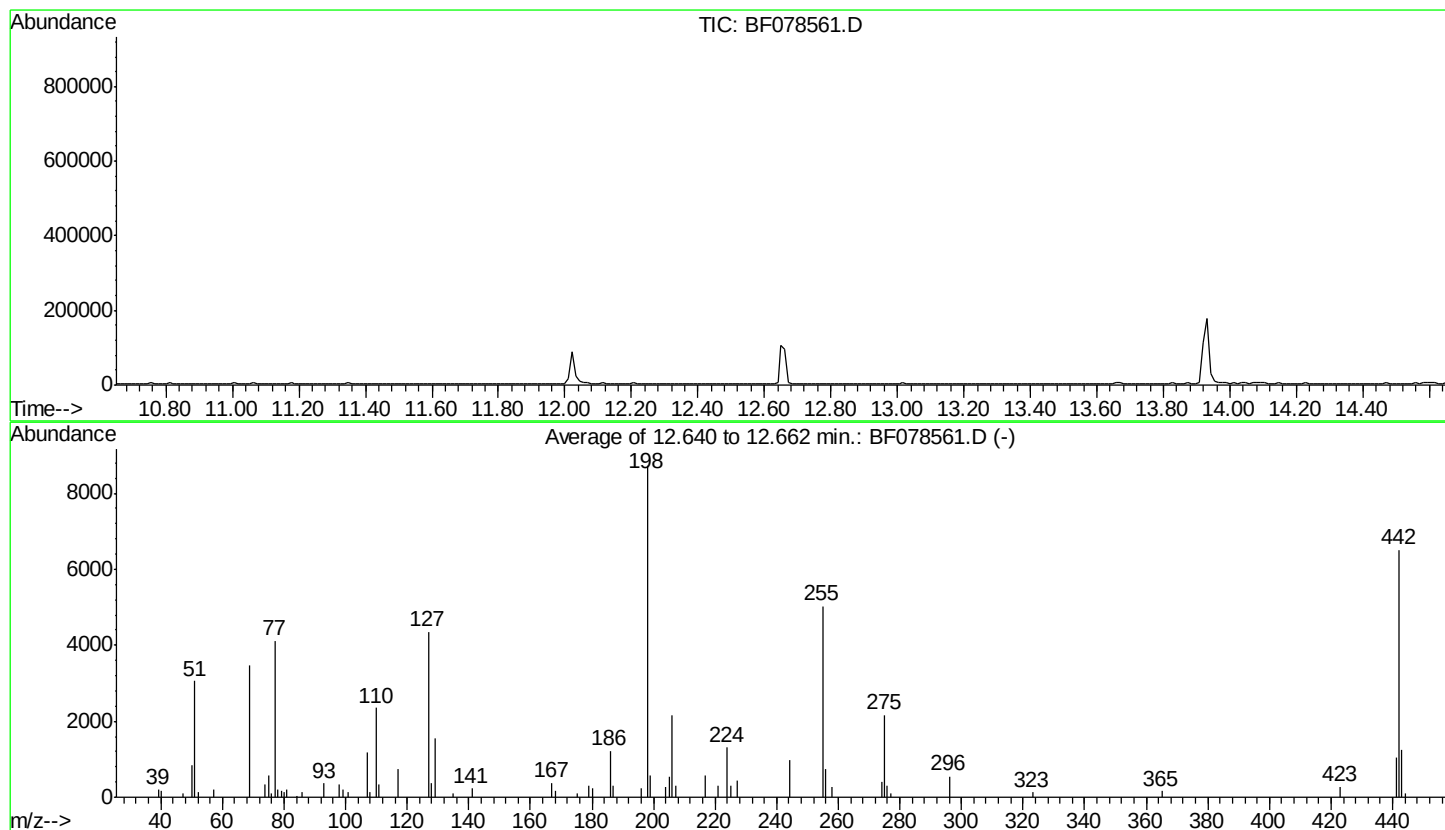

AutoFind: Scans 1002, 1003, 1004; Background Corrected with Scan 999

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	3057	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.8	3473	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.0	4361	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	8726	PASS
199	198	5	9	6.5	567	PASS
275	198	10	60	24.7	2156	PASS
365	198	1	100	1.9	163	PASS
441	442	0.01	24	16.0	1041	PASS
442	198	50	100	74.7	6516	PASS
443	442	15	24	19.2	1250	PASS